

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010126.D
 Acq On : 06 Mar 2020 19:20
 Operator : CG/JU
 Sample : PB127346BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	35	37	43	rBV2	26218	35149	1.98%	0.191%
2	4.481	287	288	290	rBV	8589	5041	0.28%	0.027%
3	4.569	300	303	305	rBV	7852	10407	0.59%	0.057%
4	4.669	318	320	322	rBV	7540	7363	0.41%	0.040%
5	4.693	322	324	327	rVV	6239	5917	0.33%	0.032%
6	5.058	382	386	387	rBV	9332	9184	0.52%	0.050%
7	5.587	474	476	478	rBV	7871	9775	0.55%	0.053%
8	5.728	497	500	501	rBV	9337	8225	0.46%	0.045%
9	6.234	584	586	589	rBV	6342	7299	0.41%	0.040%
10	6.563	636	642	653	rBV2	322470	589927	33.19%	3.203%
11	6.710	663	667	678	rVB	230229	400182	22.51%	2.173%
12	6.816	684	685	687	rBV	7315	5363	0.30%	0.029%
13	6.893	693	698	708	rBV	351690	578283	32.53%	3.140%
14	7.352	771	776	791	rVB2	253783	453853	25.53%	2.464%
15	7.452	791	793	794	rBV	8303	5365	0.30%	0.029%
16	7.481	796	798	801	rBV	6846	10177	0.57%	0.055%
17	7.552	808	810	811	rBV	7387	6662	0.37%	0.036%
18	7.728	838	840	842	rVB	7988	6648	0.37%	0.036%
19	7.781	847	849	851	rBV	7072	6054	0.34%	0.033%
20	8.075	893	899	910	rBV2	371323	707310	39.79%	3.840%
21	8.269	930	932	935	rBV	7088	9706	0.55%	0.053%
22	8.499	965	971	982	rBV2	343580	645450	36.31%	3.504%
23	8.616	989	991	995	rBV	8435	11054	0.62%	0.060%
24	8.669	998	1000	1001	rVB	8119	5586	0.31%	0.030%
25	8.705	1004	1006	1009	rBV	6172	5848	0.33%	0.032%
26	8.740	1009	1012	1013	rBV	6860	6118	0.34%	0.033%
27	8.899	1038	1039	1041	rBV	6662	5602	0.32%	0.030%
28	8.952	1045	1048	1050	rVV	6316	6856	0.39%	0.037%
29	8.975	1050	1052	1054	rVB	7750	5674	0.32%	0.031%
30	9.210	1087	1092	1102	rBV	283011	488967	27.51%	2.655%
31	9.316	1109	1110	1114	rBV	11669	14271	0.80%	0.077%
32	9.399	1122	1124	1126	rBV	6201	6321	0.36%	0.034%
33	9.434	1126	1130	1132	rVV	7865	10232	0.58%	0.056%
34	9.499	1138	1141	1143	rBV	8765	10157	0.57%	0.055%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010126.D
 Acq On : 06 Mar 2020 19:20
 Operator : CG/JU
 Sample : PB127346BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	9.581	1154	1155	1158	rBV	7534	5148	0.29%	0.028%
36	9.746	1177	1183	1196	rBV	345655	663005	37.30%	3.600%
37	9.999	1223	1226	1227	rBV	6436	5607	0.32%	0.030%
38	10.099	1237	1243	1251	rVB	364181	608482	34.23%	3.304%
39	10.187	1256	1258	1261	rBV	5807	6366	0.36%	0.035%
40	10.263	1265	1271	1280	rBV	286581	643131	36.18%	3.492%
41	10.428	1296	1299	1300	rBV	7747	5855	0.33%	0.032%
42	10.651	1335	1337	1340	rBV	7213	8018	0.45%	0.044%
43	10.893	1376	1378	1380	rBV	5549	5069	0.29%	0.028%
44	10.993	1393	1395	1396	rBV	8338	6743	0.38%	0.037%
45	11.099	1409	1413	1415	rBV	8599	8980	0.51%	0.049%
46	11.187	1427	1428	1430	rBV	8271	6317	0.36%	0.034%
47	11.269	1441	1442	1444	rBV	9571	6121	0.34%	0.033%
48	11.357	1455	1457	1460	rBV	4886	5127	0.29%	0.028%
49	11.640	1504	1505	1508	rBV	6556	5439	0.31%	0.030%
50	11.828	1535	1537	1541	rBV	9065	14473	0.81%	0.079%
51	11.963	1559	1560	1563	rVB	8612	6208	0.35%	0.034%
52	12.281	1612	1614	1616	rBV	9825	9705	0.55%	0.053%
53	12.328	1619	1622	1625	rBV	12221	15125	0.85%	0.082%
54	12.351	1625	1626	1630	rVB	6350	5968	0.34%	0.032%
55	13.334	1791	1793	1796	rBV	8276	9180	0.52%	0.050%
56	13.428	1804	1809	1819	rVB	714929	1069171	60.15%	5.805%
57	13.687	1847	1853	1859	rBV	786520	1189304	66.91%	6.457%
58	13.998	1900	1906	1913	rVB	538903	788168	44.34%	4.279%
59	14.263	1946	1951	1962	rBV2	183804	430324	24.21%	2.336%
60	15.004	2072	2077	2089	rVB	1031719	1547914	87.08%	8.404%
61	15.175	2102	2106	2116	rBV	234488	451594	25.40%	2.452%
62	16.757	2370	2375	2382	rBV	640868	921809	51.86%	5.005%
63	16.857	2387	2392	2407	rVB2	1033562	1616296	90.93%	8.776%
64	19.175	2780	2786	2796	rBV	1226544	1777587	100.00%	9.651%
65	20.986	3090	3094	3102	rBV2	656253	922090	51.87%	5.006%
66	22.951	3423	3428	3433	rBV	947946	1553816	87.41%	8.436%


Sum of corrected areas: 18418166

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010126.D
Acq On : 06 Mar 2020 19:20
Operator : CG/JU
Sample : PB127346BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

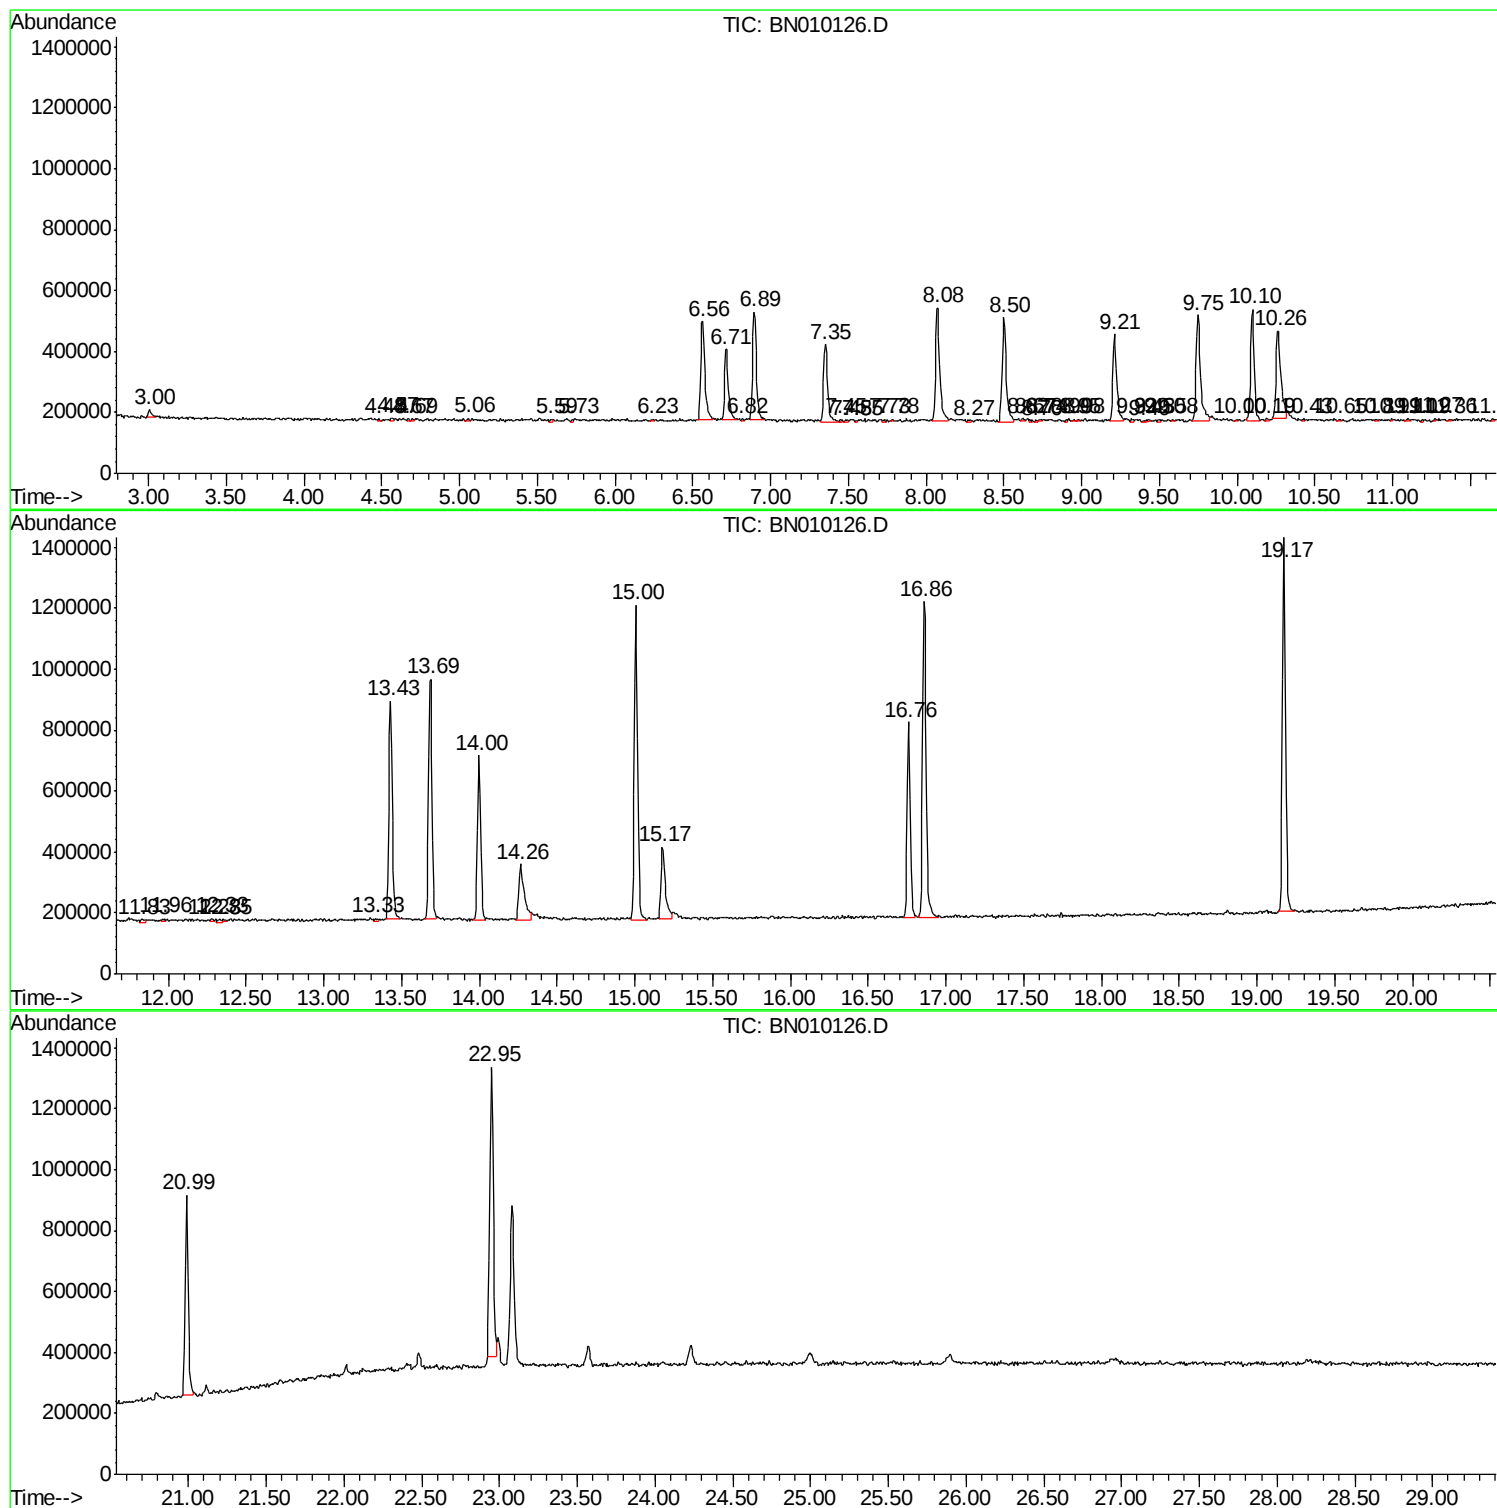

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010126.D
Acq On : 06 Mar 2020 19:20
Operator : CG/JU
Sample : PB127346BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010126.D
Acq On : 06 Mar 2020 19:20
Operator : CG/JU
Sample : PB127346BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc