

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010135.D
 Acq On : 07 Mar 2020 00:45
 Operator : CG/JU
 Sample : L1834-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0DH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	178	179	182	rBV	6897	5828	0.46%	0.051%
2	4.534	294	297	299	rVB	10763	12199	0.96%	0.106%
3	4.558	299	301	302	rBV	9544	7018	0.55%	0.061%
4	4.911	359	361	364	rBV	5835	6350	0.50%	0.055%
5	4.987	372	374	375	rBV	5908	4326	0.34%	0.038%
6	5.152	401	402	407	rVB	9585	9585	0.75%	0.083%
7	5.193	407	409	411	rBV	10315	7949	0.62%	0.069%
8	5.222	411	414	416	rBV	7139	8618	0.68%	0.075%
9	5.363	436	438	440	rBV	5657	6601	0.52%	0.057%
10	5.410	442	446	448	rBV	8314	12714	1.00%	0.111%
11	5.481	457	458	460	rBV	7600	5484	0.43%	0.048%
12	5.540	466	468	469	rBV	9859	6749	0.53%	0.059%
13	5.569	472	473	475	rVV	9638	6166	0.48%	0.054%
14	5.605	477	479	481	rBV	14702	14858	1.16%	0.129%
15	5.710	495	497	499	rBV	4980	4672	0.37%	0.041%
16	5.746	501	503	506	rVB	10668	7345	0.58%	0.064%
17	5.952	535	538	540	rBV	8499	11107	0.87%	0.097%
18	6.005	546	547	549	rBV	11024	6017	0.47%	0.052%
19	6.087	559	561	562	rBV	7080	5801	0.45%	0.050%
20	6.252	587	589	591	rVB	10917	6974	0.55%	0.061%
21	6.357	603	607	609	rBV	9425	11384	0.89%	0.099%
22	6.434	619	620	622	rBV	8300	6615	0.52%	0.058%
23	6.575	640	644	647	rBV	35528	58649	4.60%	0.510%
24	6.716	663	668	678	rBV2	130139	228649	17.92%	1.989%
25	6.899	694	699	709	rVB2	163756	282715	22.16%	2.460%
26	7.057	724	726	729	rVB	6290	6186	0.48%	0.054%
27	7.087	729	731	733	rVV	5486	5966	0.47%	0.052%
28	7.116	735	736	738	rBV	8062	5421	0.42%	0.047%
29	7.210	751	752	755	rBV	8052	7406	0.58%	0.064%
30	7.352	770	776	786	rBV	347280	609191	47.76%	5.301%
31	7.481	796	798	804	rVB	11057	13866	1.09%	0.121%
32	7.522	804	805	808	rBV	8158	8125	0.64%	0.071%
33	7.852	860	861	864	rBV	7510	6889	0.54%	0.060%
34	8.052	891	895	896	rBV	9004	10151	0.80%	0.088%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010135.D
 Acq On : 07 Mar 2020 00:45
 Operator : CG/JU
 Sample : L1834-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0DH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	8.081	896	900	908	rVV2	111765	203674	15.97%	1.772%
36	8.299	936	937	941	rVB	9865	9426	0.74%	0.082%
37	8.346	943	945	947	rBV	7210	5596	0.44%	0.049%
38	8.452	960	963	964	rBV	6241	6012	0.47%	0.052%
39	8.504	967	972	980	rVV	168249	313618	24.59%	2.729%
40	8.616	990	991	994	rVB	8120	4782	0.37%	0.042%
41	9.146	1078	1081	1084	rBV	12765	18613	1.46%	0.162%
42	9.216	1088	1093	1104	rVV	140554	279470	21.91%	2.432%
43	9.340	1112	1114	1115	rBV	6501	5497	0.43%	0.048%
44	9.481	1136	1138	1142	rBV	9251	12230	0.96%	0.106%
45	9.551	1148	1150	1152	rBV	7465	7106	0.56%	0.062%
46	9.587	1154	1156	1159	rBV	7256	7846	0.62%	0.068%
47	9.687	1171	1173	1176	rVB	7951	6979	0.55%	0.061%
48	9.710	1176	1177	1179	rVB	9491	4510	0.35%	0.039%
49	9.769	1179	1187	1198	rBV2	112483	356870	27.98%	3.105%
50	9.969	1219	1221	1224	rVB	8681	9016	0.71%	0.078%
51	10.010	1226	1228	1231	rBV	7879	9685	0.76%	0.084%
52	10.098	1237	1243	1250	rBV	442779	776585	60.88%	6.757%
53	10.269	1270	1272	1274	rBV	9772	11137	0.87%	0.097%
54	10.440	1300	1301	1304	rBV	6459	5313	0.42%	0.046%
55	10.775	1356	1358	1361	rBV	7942	6140	0.48%	0.053%
56	11.016	1395	1399	1400	rBV	6907	7037	0.55%	0.061%
57	11.216	1431	1433	1437	rBV	11429	14299	1.12%	0.124%
58	12.822	1704	1706	1707	rBV	8911	6733	0.53%	0.059%
59	13.428	1804	1809	1815	rBV	387819	602907	47.26%	5.246%
60	13.687	1847	1853	1859	rBV	462070	672548	52.72%	5.852%
61	13.834	1876	1878	1880	rBV	12277	9514	0.75%	0.083%
62	13.998	1900	1906	1916	rBV	702254	1052642	82.52%	9.159%
63	15.010	2072	2078	2088	rVB	550891	903593	70.84%	7.862%
64	15.181	2103	2107	2118	rBV2	109671	235188	18.44%	2.046%
65	16.757	2370	2375	2384	rVB	888994	1219907	95.63%	10.614%
66	16.863	2388	2393	2403	rVB	634590	971175	76.13%	8.450%
67	19.169	2781	2785	2792	rBV2	766273	1044197	81.86%	9.085%
68	20.986	3090	3094	3103	rVB	1016418	1275598	100.00%	11.099%


Sum of corrected areas: 11493017

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010135.D
Acq On : 07 Mar 2020 00:45
Operator : CG/JU
Sample : L1834-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
C0DH6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

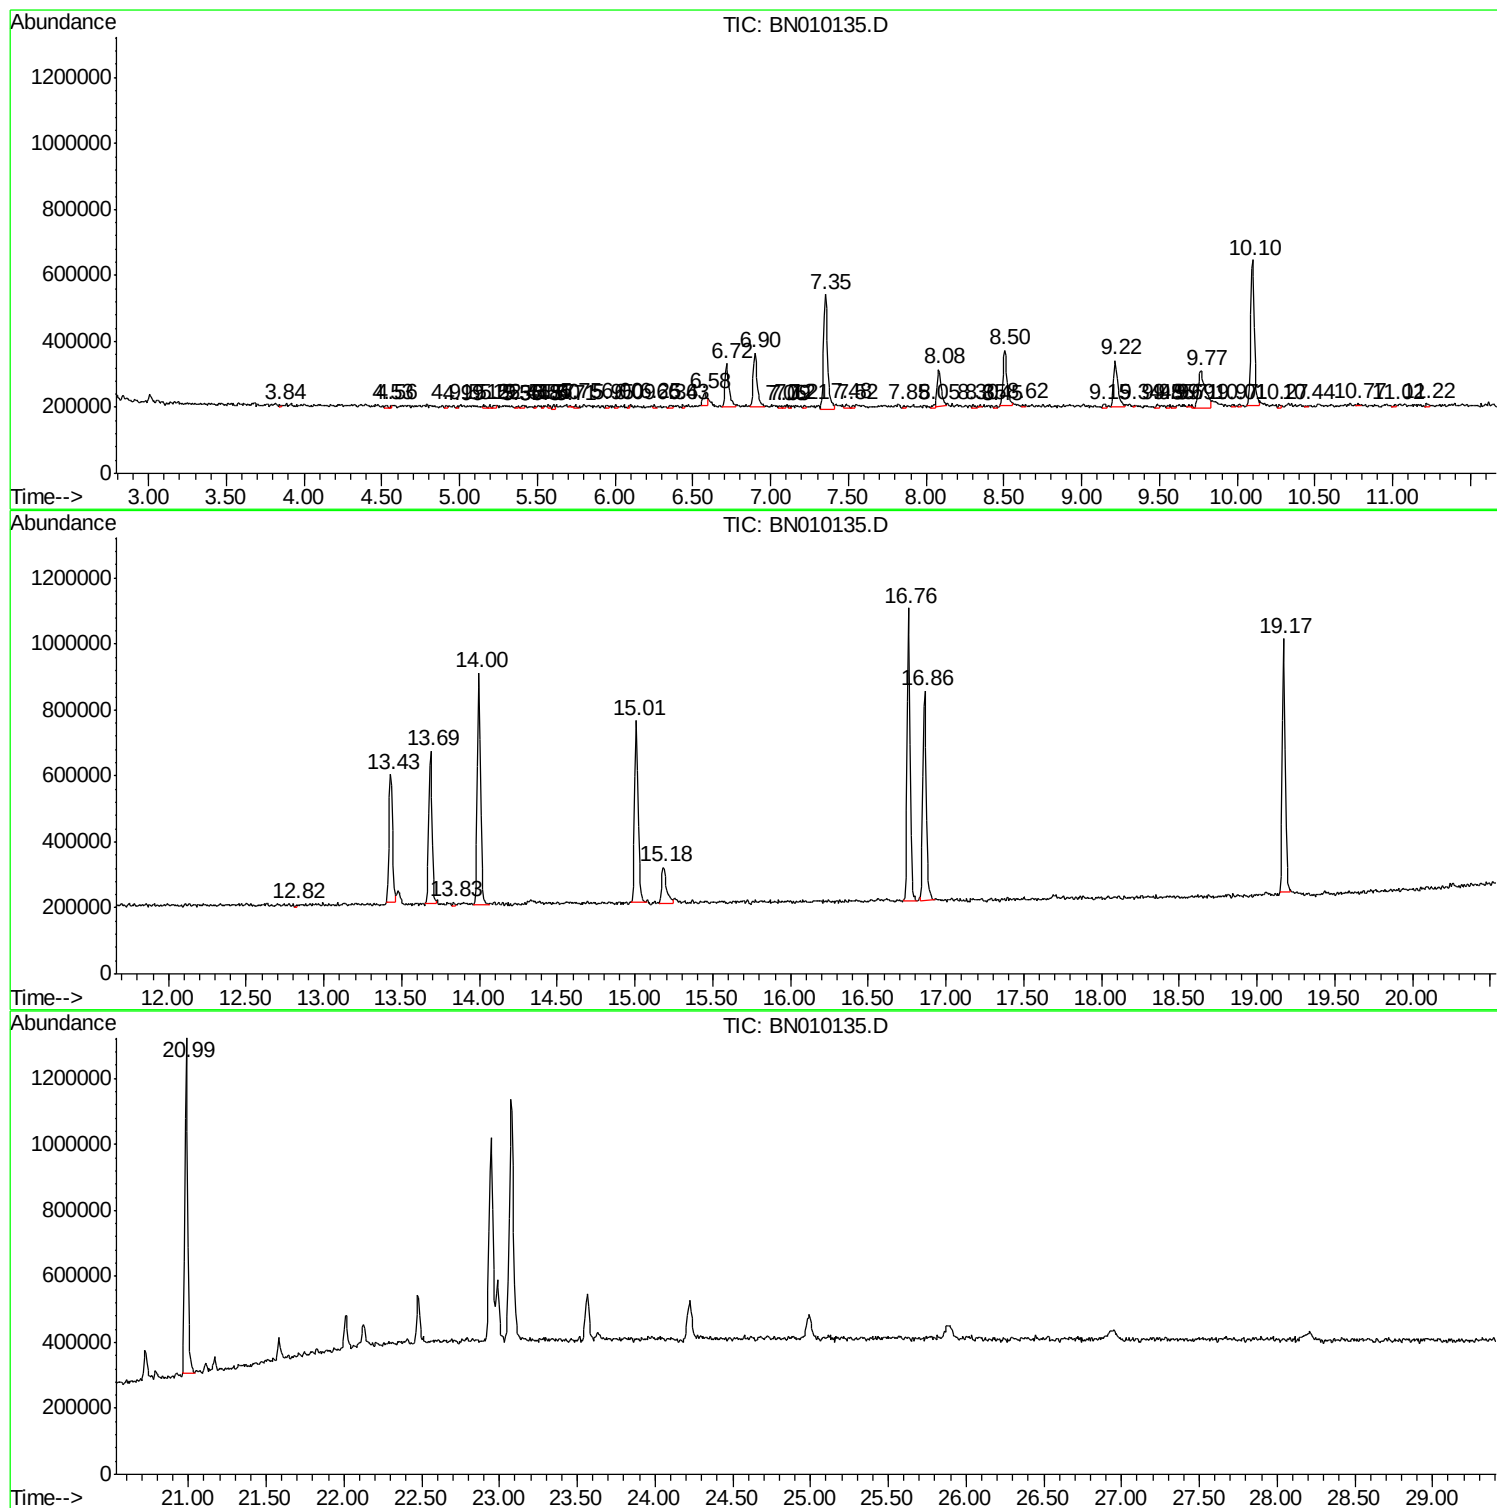

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010135.D
Acq On : 07 Mar 2020 00:45
Operator : CG/JU
Sample : L1834-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0DH6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010135.D
Acq On : 07 Mar 2020 00:45
Operator : CG/JU
Sample : L1834-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0DH6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc