

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
 Data File : BN004645.D
 Acq On : 07 Mar 2019 20:04
 Operator : JU/SJ
 Sample : K1657-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB653

Quant Time: Mar 08 01:08:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	34101	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	156785	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	99647	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	242010	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	293682	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	301940	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	4059	6.71	ng/uL	0.00
5) Phenol-d5	6.88	99	48093	17.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	28045	19.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	44436	18.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	44627	18.21	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	23647	19.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	27291	20.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	46288	17.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	67221	21.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	188532	21.88	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	204173	19.69	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	26963	16.86	ng/ul	0.00
58) Fluorene-d10	15.36	176	152510	20.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	28947	17.33	ng/ul	0.00
71) Anthracene-d10	17.21	188	240310	20.39	ng/ul	0.00
79) Pyrene-d10	19.51	212	276373	19.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	289862	17.88	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.82	163	19994	2.365	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030719\
Data File : BN004645.D
Acq On : 07 Mar 2019 20:04
Operator : JU/SJ
Sample : K1657-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB653

Quant Time: Mar 08 01:08:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

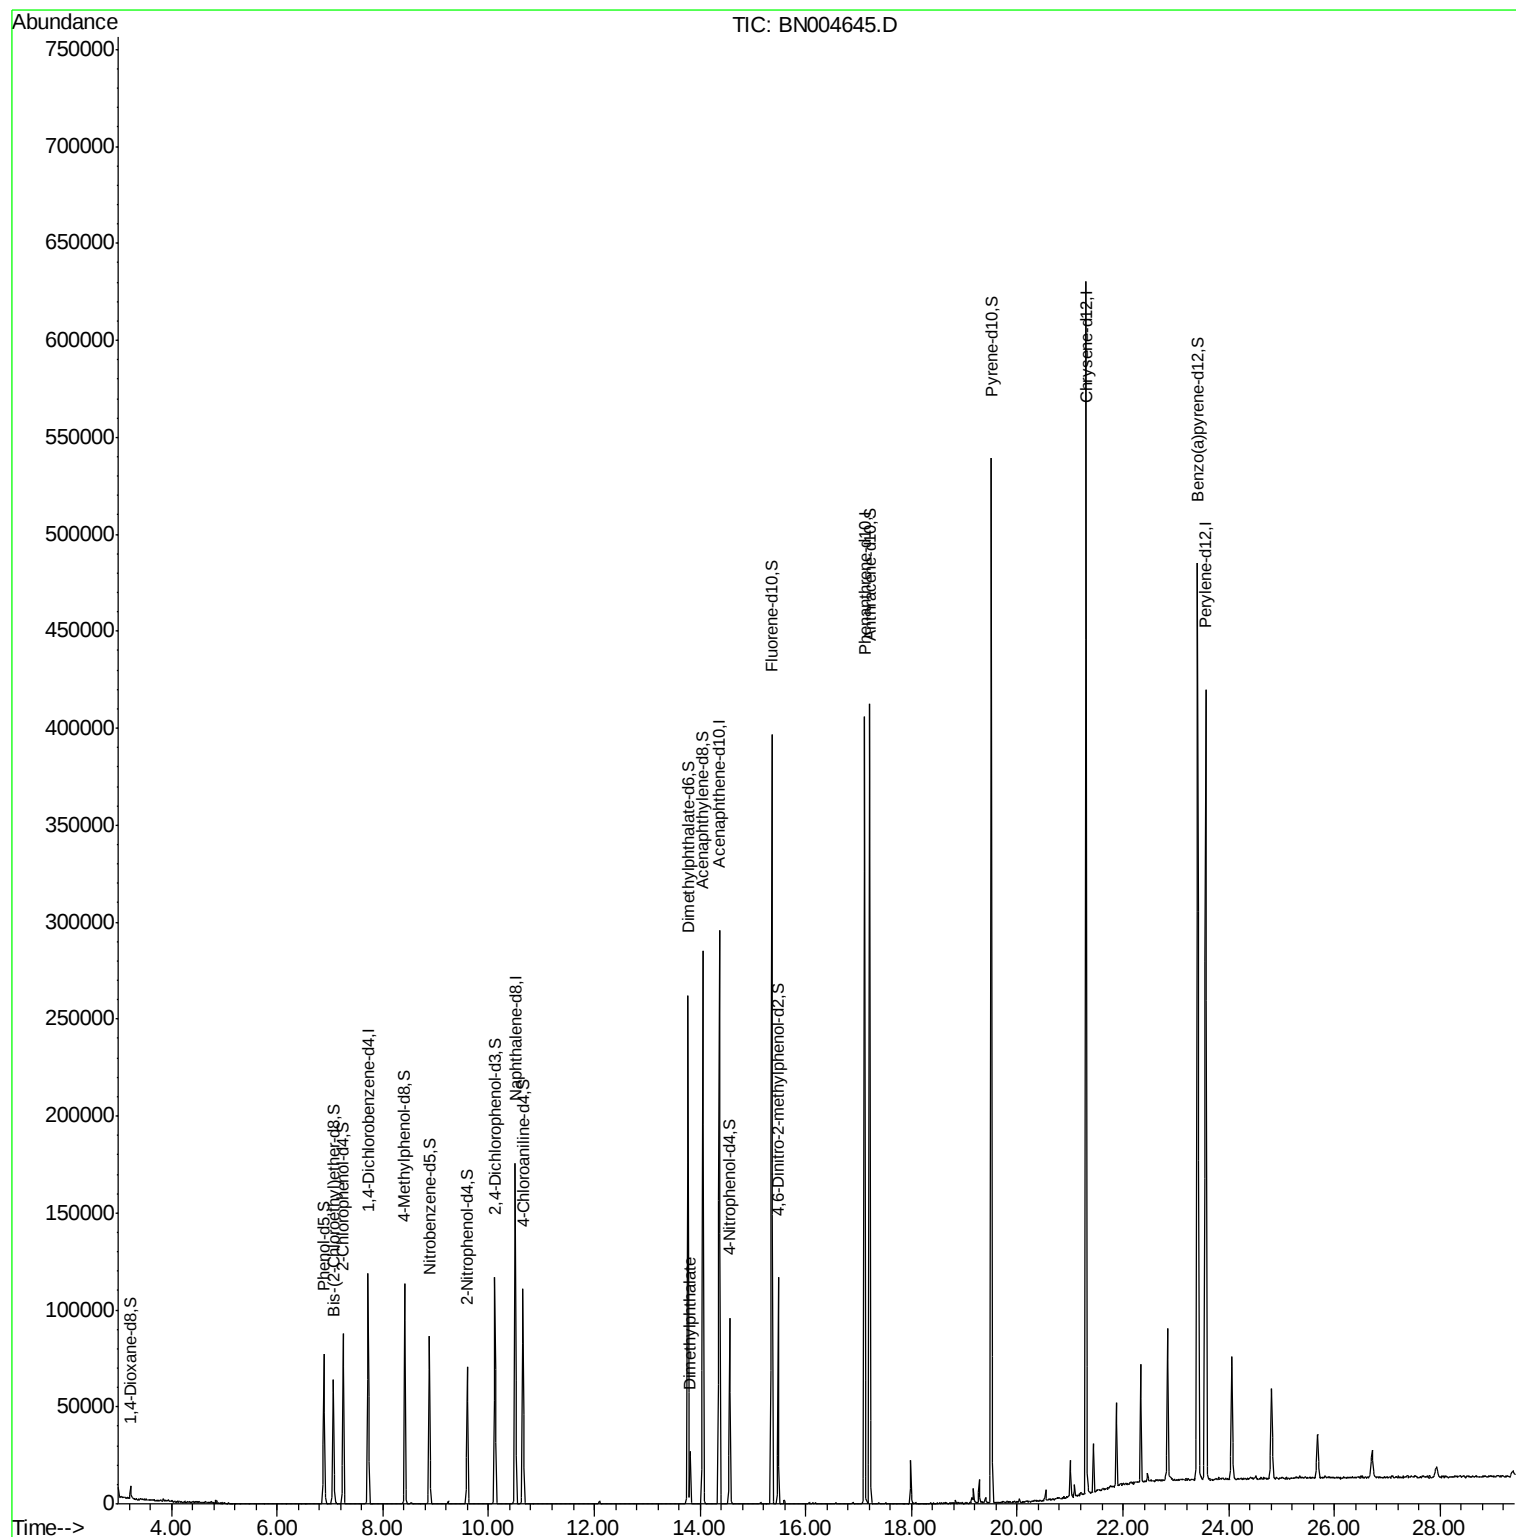

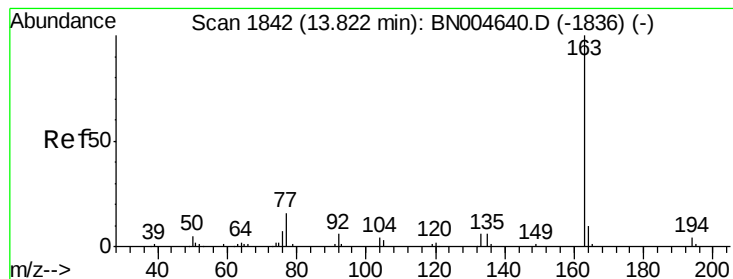

#45

Dimethylphthalate

Concen: 2.365 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BN004645.D

Acq: 07 Mar 2019 20:04

Instrument :

BNA_N

ClientSampleId :

DB653


Tot Ion:163 Resp: 19994

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.2 7.9 11.9

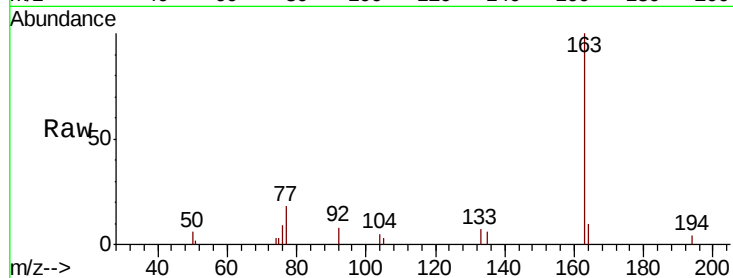

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

