

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030719\
 Data File : BN004647.D
 Acq On : 07 Mar 2019 21:14
 Operator : JU/SJ
 Sample : K1662-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFC59

Quant Time: Mar 08 01:14:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	34555	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	160466	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	104383	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	253532	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	312041	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	331272	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	3206	5.23	ng/uL	0.00
5) Phenol-d5	6.88	99	29892	10.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	17919	12.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	27798	11.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	27957	11.26	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	14364	11.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	15918	11.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	28413	10.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	43879	13.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	124350	13.78	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	126796	11.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	12609	7.53	ng/ul	0.00
58) Fluorene-d10	15.36	176	98528	12.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	12046	6.88	ng/ul	0.00
71) Anthracene-d10	17.21	188	156803	12.70	ng/ul	0.00
79) Pyrene-d10	19.51	212	175773	11.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	189559	10.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.82	163	13955	1.576	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
Data File : BN004647.D
Acq On : 07 Mar 2019 21:14
Operator : JU/SJ
Sample : K1662-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFC59

Quant Time: Mar 08 01:14:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

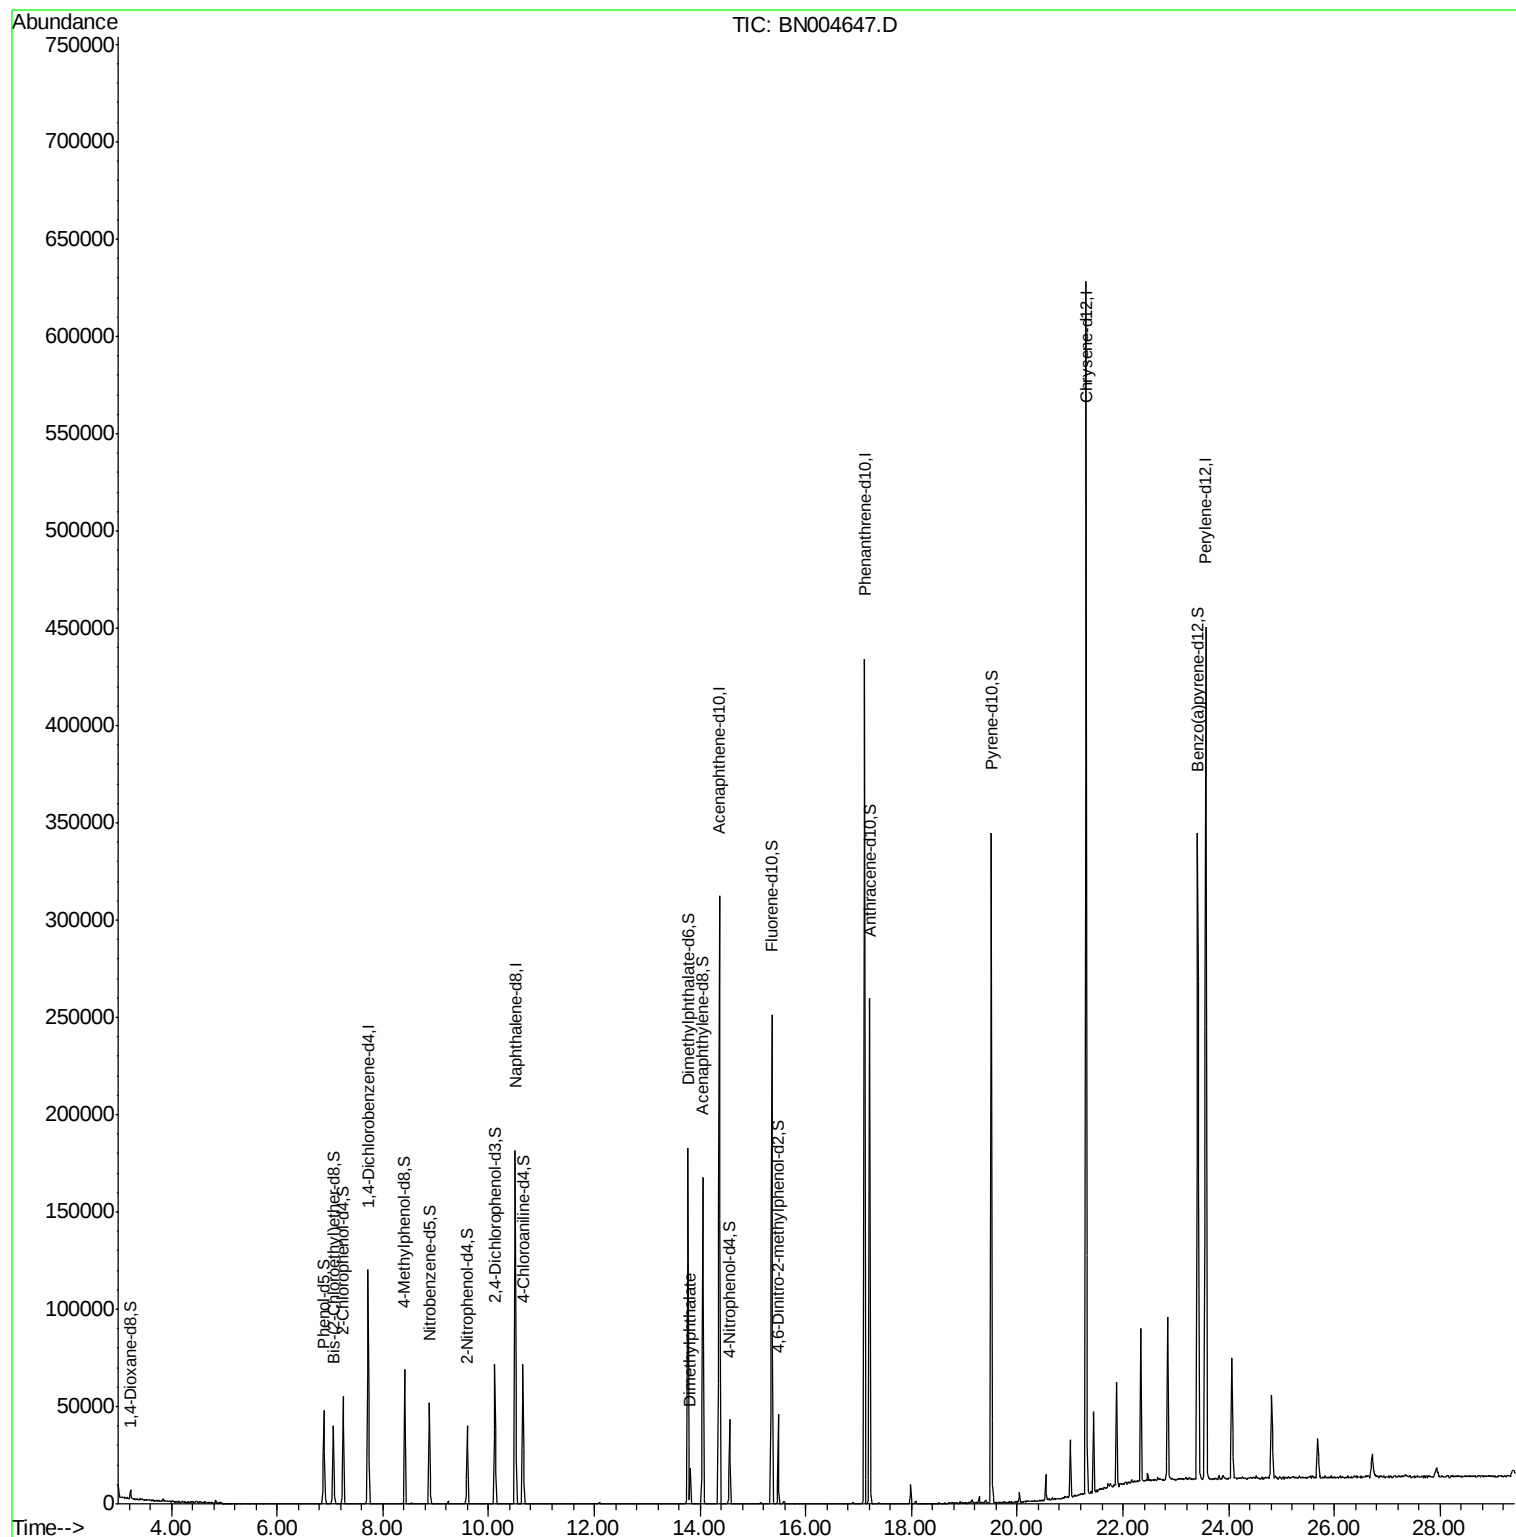

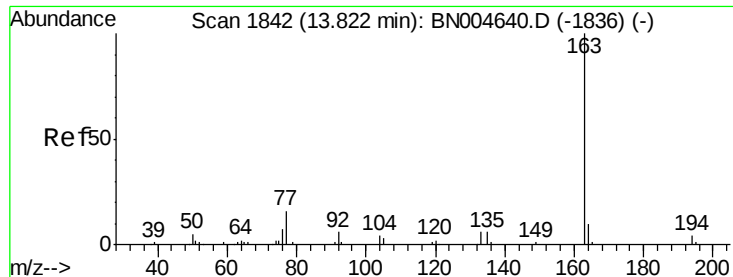

#45

Dimethylphthalate

Concen: 1.576 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BN004647.D

Acq: 07 Mar 2019 21:14

Instrument :

BNA_N

ClientSampleId :

BFC59


Tot Ion:163 Resp: 13955

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 10.7 7.9 11.9

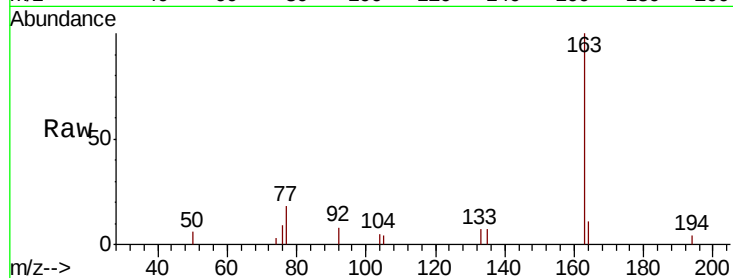

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

