

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
 Data File : BN004651.D
 Acq On : 07 Mar 2019 23:34
 Operator : JU/SJ
 Sample : K1721-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF8B9

Quant Time: Mar 08 01:30:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	27982	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	129096	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	80119	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	195182	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	261571	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	310683	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	1974	3.98	ng/uL	0.00
5) Phenol-d5	6.88	99	12297	5.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	28685	23.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	40631	20.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	22332	11.10	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	25310	25.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	29217	26.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	48841	22.93	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	13.77	166	182934	26.41	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	218427	26.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	5775	4.49	ng/ul	0.00
58) Fluorene-d10	15.36	176	157665	26.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	31570	23.43	ng/ul	0.00
71) Anthracene-d10	17.21	188	255065	26.83	ng/ul	0.00
79) Pyrene-d10	19.51	212	322148	25.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	429056	25.72	ng/ul	-0.01

Target Compounds


				Ovalue	
84) Bis(2-ethylhexyl)phthalate	21.21	149	29037	3.069	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030719\
Data File : BN004651.D
Acq On : 07 Mar 2019 23:34
Operator : JU/SJ
Sample : K1721-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF8B9

Quant Time: Mar 08 01:30:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

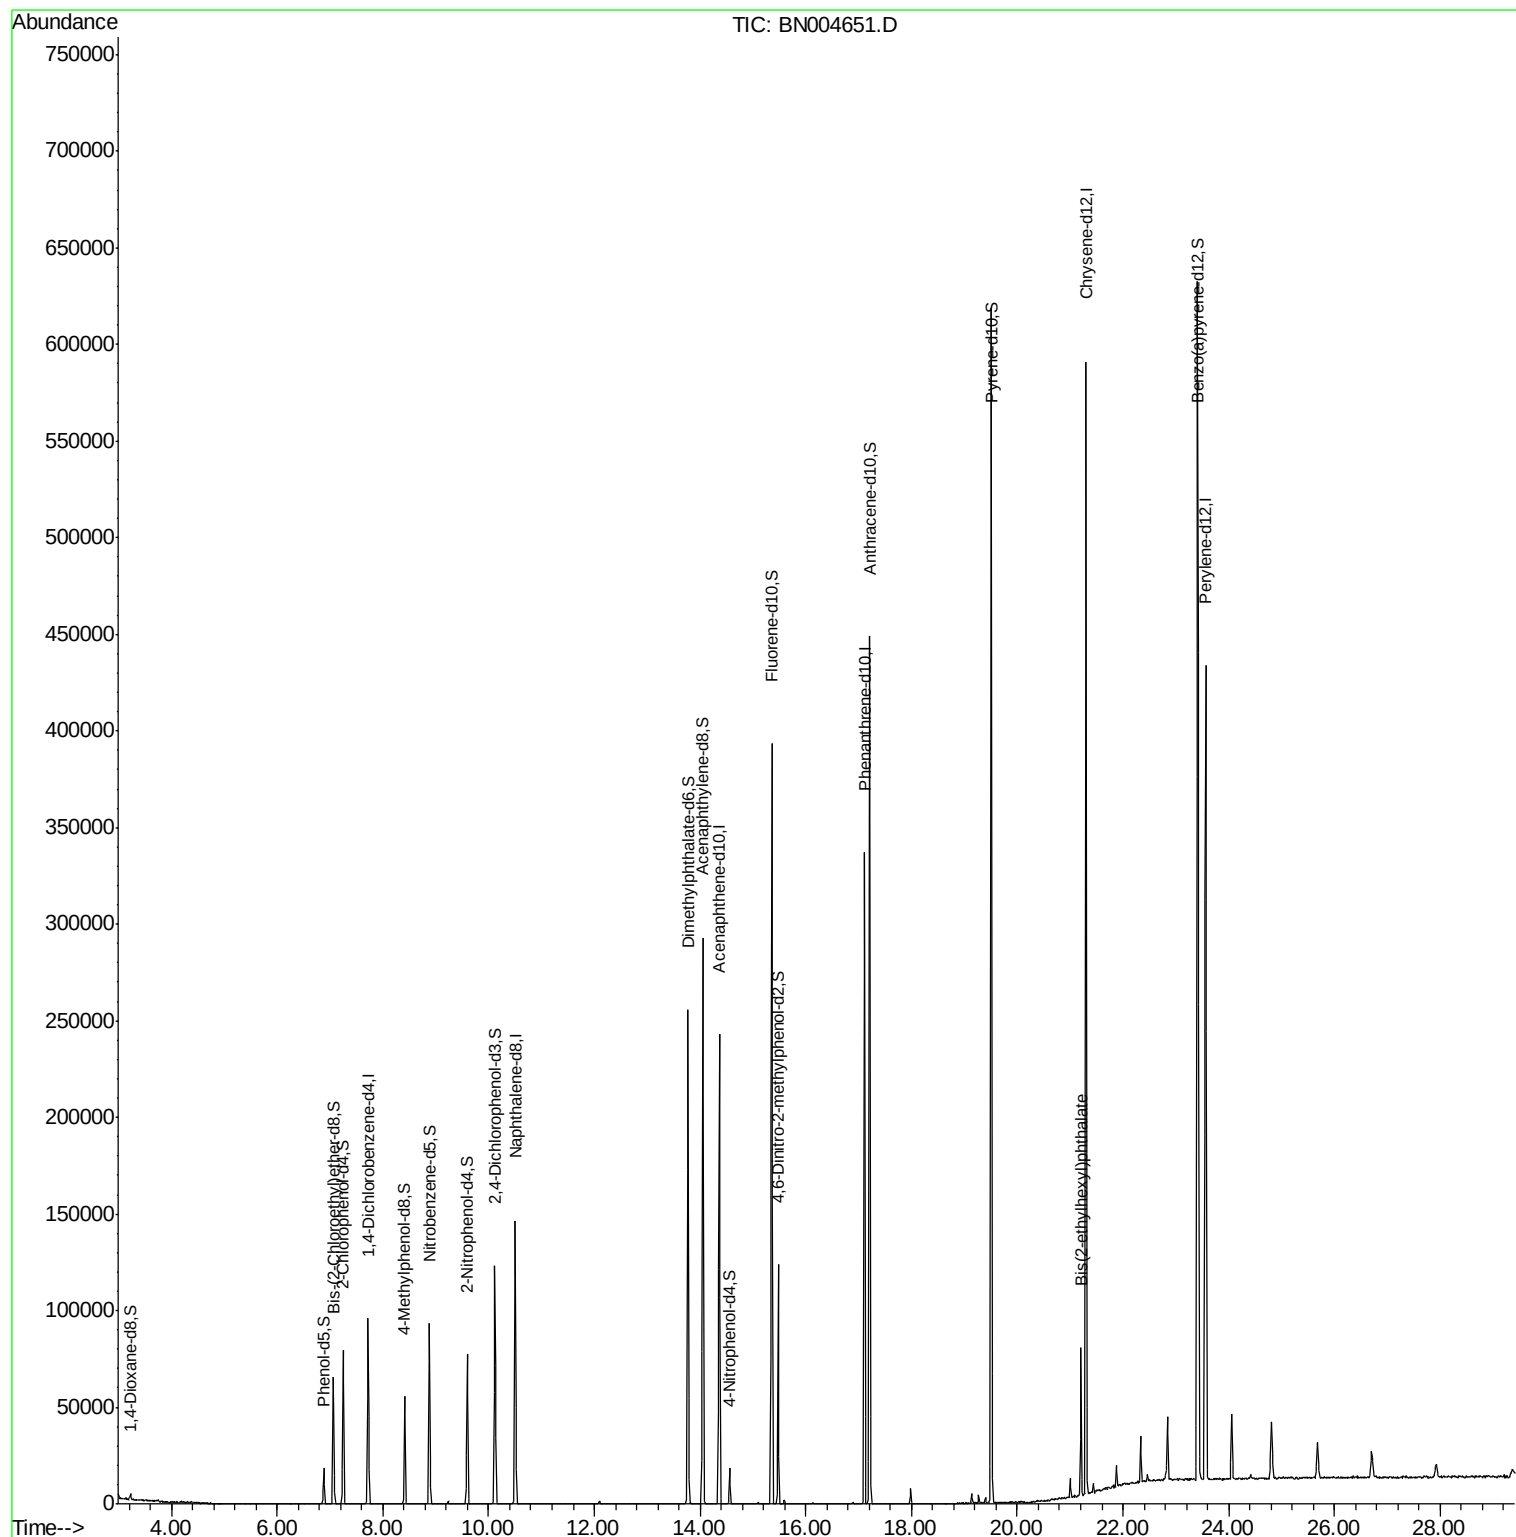

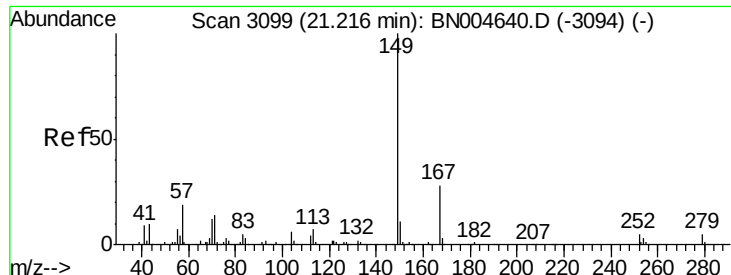

#84

Bis(2-ethylhexyl)phthalate

Concen: 3.069 ng/ul

RT: 21.21 min Scan# 3098

Delta R.T. -0.01 min

Lab File: BN004651.D

Acq: 07 Mar 2019 23:34

Instrument :

BNA_N

ClientSampleId :

BF8B9


Tot Ion:149 Resp: 29037

Ion Ratio Lower Upper

149 100

167 28.0 22.7 34.1

279 5.0 4.3 6.5

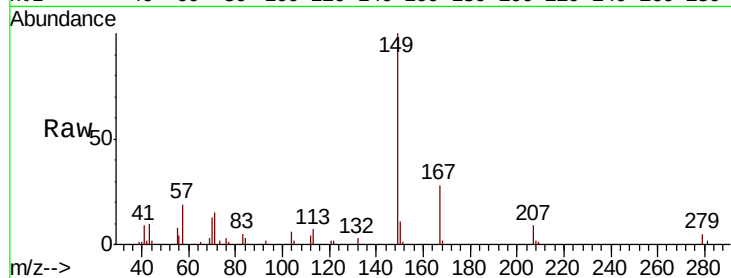

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

