

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
 Data File : BN004665.D
 Acq On : 08 Mar 2019 07:46
 Operator : JU/SJ
 Sample : K1662-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFC65

Quant Time: Mar 08 08:20:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 08 00:36:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	35134	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	170420	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	108258	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	256853	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	293659	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	250444	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.23	96	4142	6.65	ng/uL	0.00
5) Phenol-d5	6.88	99	57577	19.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	32266	21.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	52713	20.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	53798	21.31	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	28449	21.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	33158	22.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	57221	20.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	82781	24.54	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	211190	22.56	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	240939	21.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	26276	15.12	ng/ul	0.00
58) Fluorene-d10	15.36	176	174421	21.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	26581	14.99	ng/ul	0.00
71) Anthracene-d10	17.21	188	276575	22.11	ng/ul	0.00
79) Pyrene-d10	19.51	212	314919	21.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	269538	20.04	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.91	94	5462	1.849	ng/ul	98
45) Dimethylphthalate	13.82	163	24582	2.677	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
Data File : BN004665.D
Acq On : 08 Mar 2019 07:46
Operator : JU/SJ
Sample : K1662-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFC65

Quant Time: Mar 08 08:20:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 08 00:36:35 2019
Response via : Initial Calibration

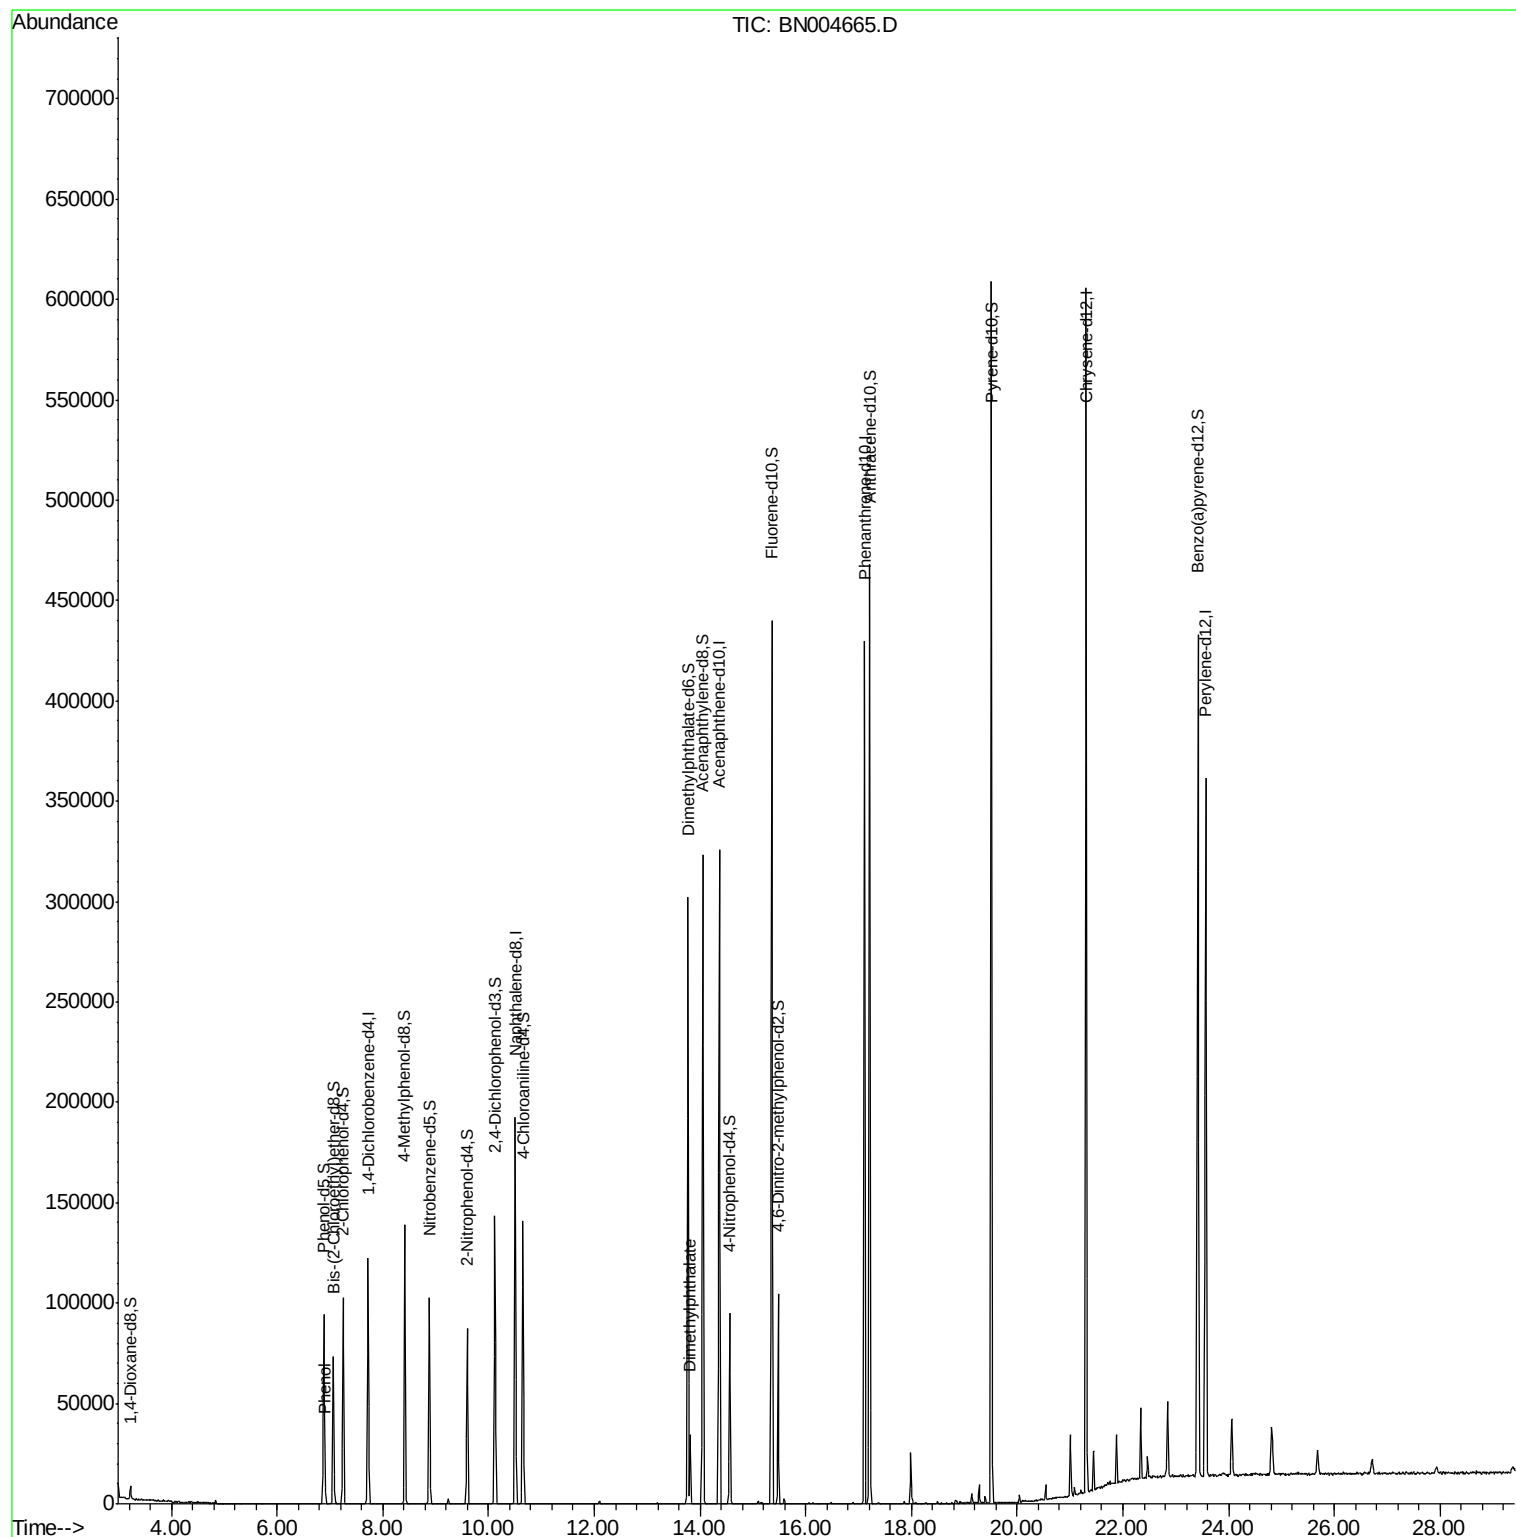

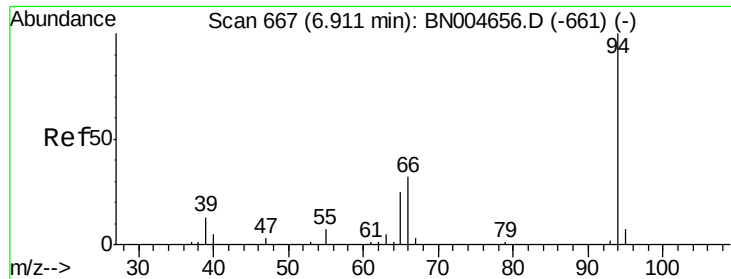


#6

Phenol




Concen: 1.849 ng/ul
 RT: 6.91 min Scan# 667
 Delta R.T. -0.00 min
 Lab File: BN004665.D
 Acq: 08 Mar 2019 07:46

Instrument :
 BNA_N
 ClientSampleId :
 BFC65

Tot Ion: 94 Resp: 5462
 Ion Ratio Lower Upper
 94 100
 65 25.9 20.2 30.4
 66 36.5 28.2 42.2

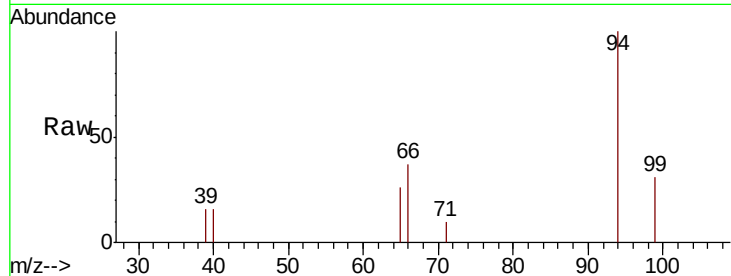

Abundance Ion 94.00 (93.70 to 94.70): BN0
 Ion 65.00 (64.70 to 65.70): BN0
 Ion 66.00 (65.70 to 66.70): BN0

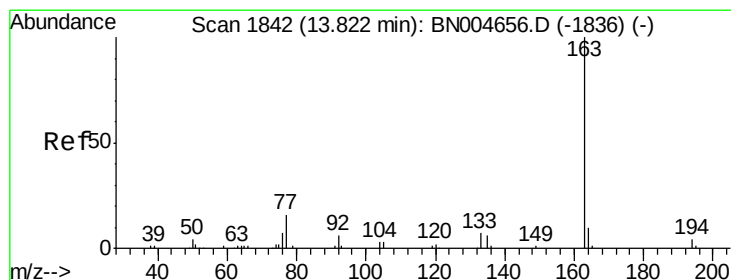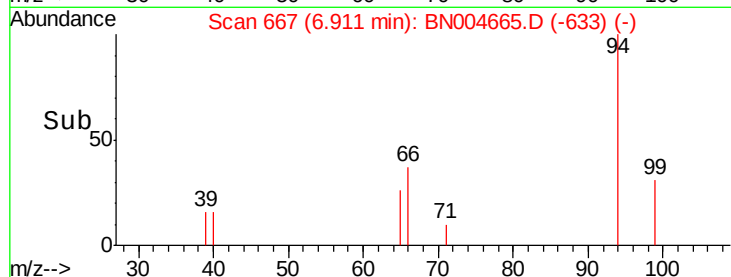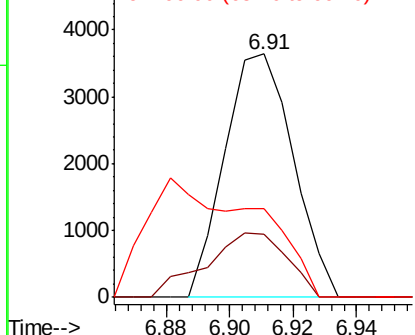


#45

Dimethylphthalate

Concen: 2.677 ng/ul
 RT: 13.82 min Scan# 1841
 Delta R.T. -0.01 min
 Lab File: BN004665.D
 Acq: 08 Mar 2019 07:46

Tgt Ion:163 Resp: 24582
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.4 5.2
 164 10.7 7.9 11.9

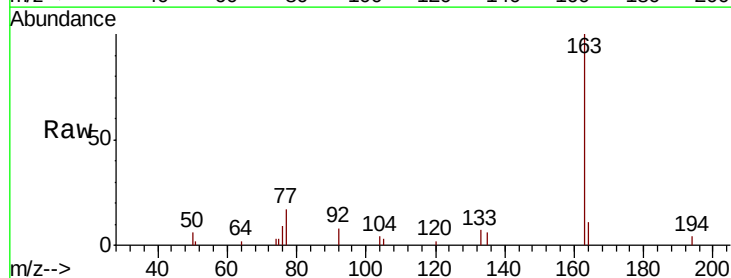

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

