

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
 Data File : BN004670.D
 Acq On : 08 Mar 2019 10:52
 Operator : JU/SJ
 Sample : K1626-09DL 2X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF668DL

Quant Time: Mar 08 11:28:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 07 15:17:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	38129	20.00	ng/ul	-0.03
18) Naphthalene-d8	10.50	136	178255	20.00	ng/ul	-0.03
36) Acenaphthene-d10	14.36	164	102203	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.11	188	217985	20.00	ng/ul	-0.02
78) Chrysene-d12	21.32	240	162492	20.00	ng/ul	-0.01
86) Perylene-d12	23.57	264	169669	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	540	0.80	ng/uL	-0.02
5) Phenol-d5	6.88	99	19603	6.22	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.06	67	9876	6.01	ng/ul	-0.03
9) 2-Chlorophenol-d4	7.25	132	17826	6.52	ng/ul	-0.03
13) 4-Methylphenol-d8	8.42	113	16744	6.11	ng/ul	-0.02
19) Nitrobenzene-d5	8.88	128	8698	6.40	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.59	143	9893	6.41	ng/ul	-0.03
26) 2,4-Dichlorophenol-d3	10.12	165	18530	6.30	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.65	131	18547	5.26	ng/ul	-0.02
44) Dimethylphthalate-d6	13.77	166	58138	6.58	ng/ul	-0.03
47) Acenaphthylene-d8	14.06	160	69136	6.50	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.56	143	5899	3.60	ng/ul	-0.02
58) Fluorene-d10	15.36	176	49549	6.60	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.48	200	4689	3.12	ng/ul	-0.02
71) Anthracene-d10	17.21	188	72899	6.87	ng/ul	-0.02
79) Pyrene-d10	19.51	212	64540	8.13	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.43	264	54572	5.99	ng/ul	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
84) Bis(2-ethylhexyl)phthalate	21.22	149	291945	49.668	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
Data File : BN004670.D
Acq On : 08 Mar 2019 10:52
Operator : JU/SJ
Sample : K1626-09DL 2X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF668DL

Quant Time: Mar 08 11:28:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 07 15:17:26 2019
Response via : Initial Calibration

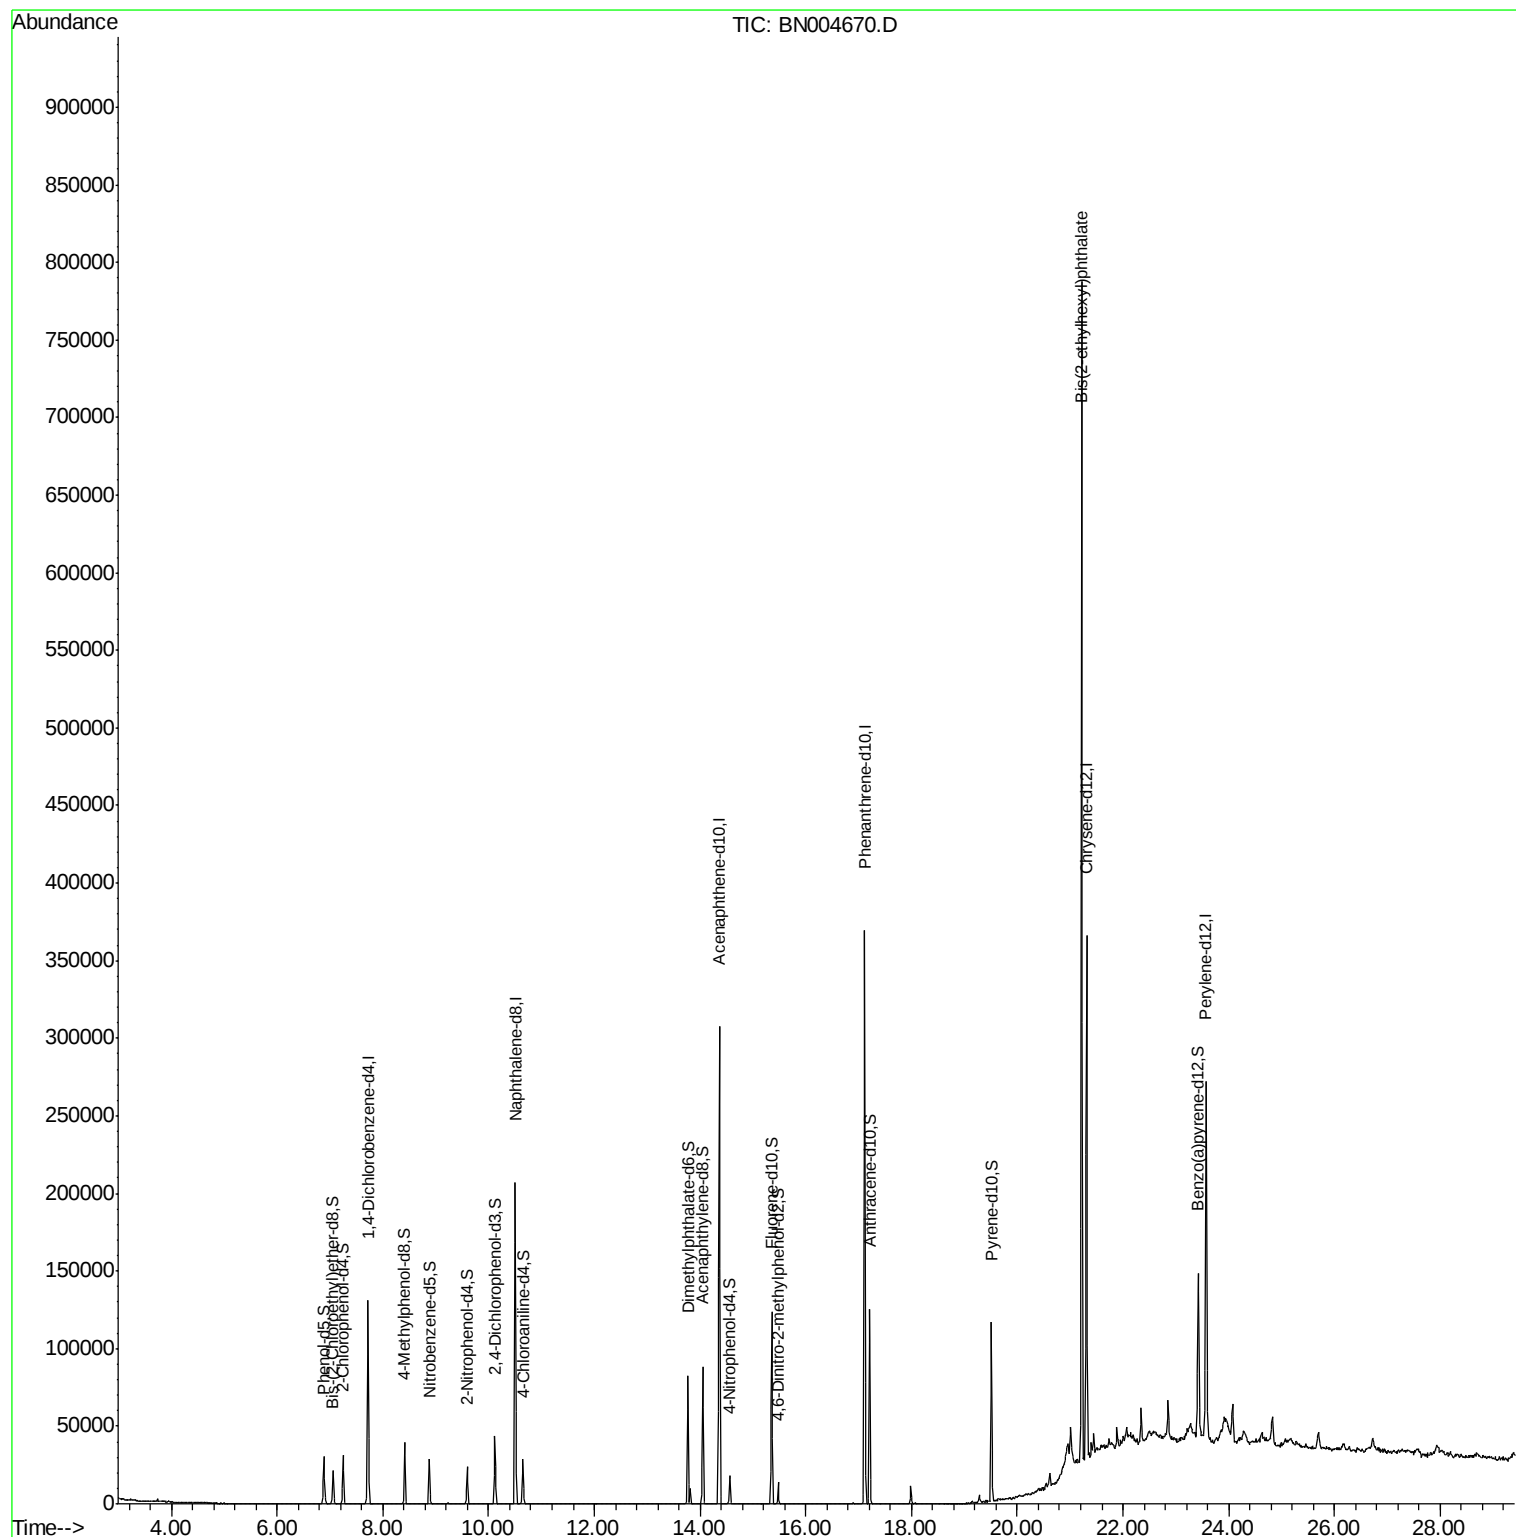

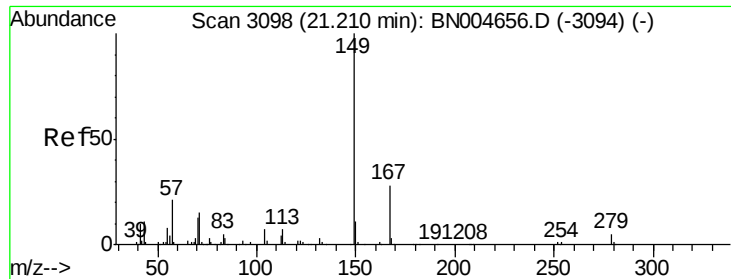

#84

Bis(2-ethylhexyl)phthalate

Concen: 49.668 ng/ul

RT: 21.22 min Scan# 3099

Delta R.T. -0.02 min

Lab File: BN004670.D

Acq: 08 Mar 2019 10:52

Instrument :

BNA_N

ClientSampleId :

BF668DL



Tot Ion:149 Resp: 291945

Ion Ratio Lower Upper

149 100

167 28.3 22.7 34.1

279 5.3 4.3 6.5

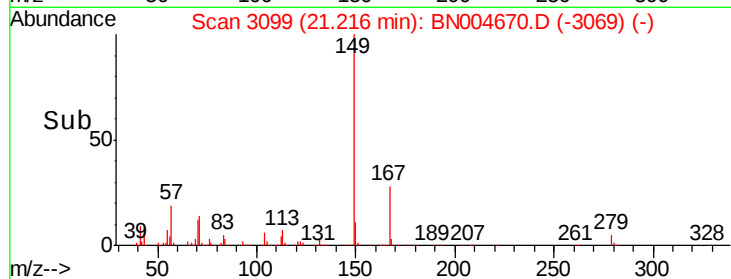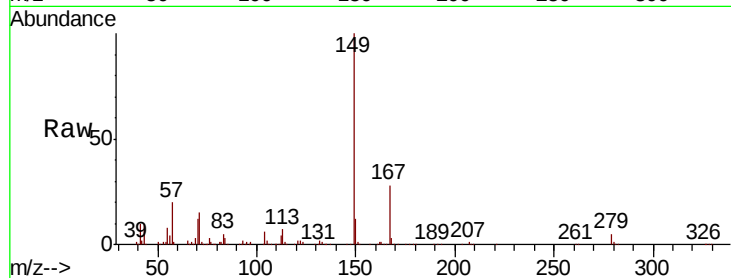

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

