

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030719\
 Data File : BN004665.D
 Acq On : 08 Mar 2019 07:46
 Operator : JU/SJ
 Sample : K1662-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFC65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	38	40	46	rVB	6569	8660	1.07%	0.099%
2	3.840	143	145	149	rVB	767	995	0.12%	0.011%
3	4.840	313	315	319	rVB2	1656	1936	0.24%	0.022%
4	6.881	656	662	671	rBB	94487	150615	18.69%	1.716%
5	7.063	687	693	702	rBB	73663	115881	14.38%	1.320%
6	7.252	719	725	731	rBB	102434	154764	19.21%	1.763%
7	7.722	799	805	811	rBB	122751	184621	22.92%	2.103%
8	8.416	917	923	930	rBB	139201	206438	25.62%	2.352%
9	8.881	996	1002	1009	rBB	102596	160472	19.92%	1.828%
10	9.240	1059	1063	1066	rBB	2775	3617	0.45%	0.041%
11	9.593	1118	1123	1130	rBB	87687	136171	16.90%	1.551%
12	10.122	1207	1213	1220	rBB	143693	224457	27.86%	2.557%
13	10.504	1271	1278	1285	rBB	192717	317894	39.46%	3.622%
14	10.646	1296	1302	1312	rBB	141088	230214	28.58%	2.623%
15	12.093	1546	1548	1551	rBB	1533	1829	0.23%	0.021%
16	13.769	1828	1833	1838	rBV	302173	407266	50.55%	4.640%
17	13.816	1838	1841	1846	rVB	34756	42176	5.24%	0.481%
18	14.057	1875	1882	1889	rBB	323557	472271	58.62%	5.381%
19	14.363	1928	1934	1940	rBB2	325800	477685	59.29%	5.442%
20	14.563	1962	1968	1976	rBB	94822	129008	16.01%	1.470%
21	15.104	2057	2060	2062	rBB	1362	1183	0.15%	0.013%
22	15.357	2097	2103	2109	rBB	439977	611059	75.85%	6.962%
23	15.475	2119	2123	2129	rBB	104351	133109	16.52%	1.517%
24	15.592	2140	2143	2147	rBB	2647	2773	0.34%	0.032%
25	16.892	2362	2364	2367	rBB	827	934	0.12%	0.011%
26	17.110	2395	2401	2407	rBB	429636	597985	74.22%	6.813%
27	17.210	2411	2418	2426	rBB	468023	664635	82.50%	7.572%
28	17.869	2528	2530	2533	rBB	1317	1367	0.17%	0.016%
29	17.992	2547	2551	2558	rBB	25590	32572	4.04%	0.371%
30	18.069	2562	2564	2567	rBB	938	977	0.12%	0.011%
31	18.839	2691	2695	2697	rBV	1612	2139	0.27%	0.024%
32	19.139	2742	2746	2751	rVB	4589	5105	0.63%	0.058%
33	19.280	2767	2770	2775	rBV	9223	10698	1.33%	0.122%
34	19.392	2786	2789	2793	rBV2	3531	4494	0.56%	0.051%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
Data File : BN004665.D
Acq On : 08 Mar 2019 07:46
Operator : JU/SJ
Sample : K1662-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFC65

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Title : SVOA CALIBRATION

35	19.510	2803	2809	2817	rBV	608451	805647	100.00%	9.179%
36	20.045	2896	2900	2902	rBV	3395	3329	0.41%	0.038%
37	20.110	2905	2911	2914	rBV	824	1489	0.18%	0.017%
38	20.539	2980	2984	2987	rVB	7710	7875	0.98%	0.090%
39	21.004	3059	3063	3070	rBV	30791	37346	4.64%	0.425%
40	21.080	3073	3076	3080	rBV	4546	5556	0.69%	0.063%
41	21.210	3095	3098	3101	rBV	2078	2025	0.25%	0.023%
42	21.304	3109	3114	3122	rBV	599707	764521	94.90%	8.710%
43	21.439	3134	3137	3142	rBV	19785	22041	2.74%	0.251%
44	21.874	3208	3211	3217	rBV	24610	28786	3.57%	0.328%
45	22.339	3285	3290	3295	rVB	35428	43337	5.38%	0.494%
46	22.469	3308	3312	3316	rBV	10334	12537	1.56%	0.143%
47	22.845	3372	3376	3381	rVB	36870	49579	6.15%	0.565%
48	23.421	3466	3474	3482	rVB	418744	734402	91.16%	8.367%
49	23.563	3490	3498	3508	rBV	348028	628361	77.99%	7.159%
50	24.063	3577	3583	3589	rVB	27799	51786	6.43%	0.590%
51	24.810	3704	3710	3719	rBV2	23119	55083	6.84%	0.628%
52	25.686	3853	3859	3867	rVB3	11853	27604	3.43%	0.314%


Sum of corrected areas: 8777304

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
Data File : BN004665.D
Acq On : 08 Mar 2019 07:46
Operator : JU/SJ
Sample : K1662-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFC65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

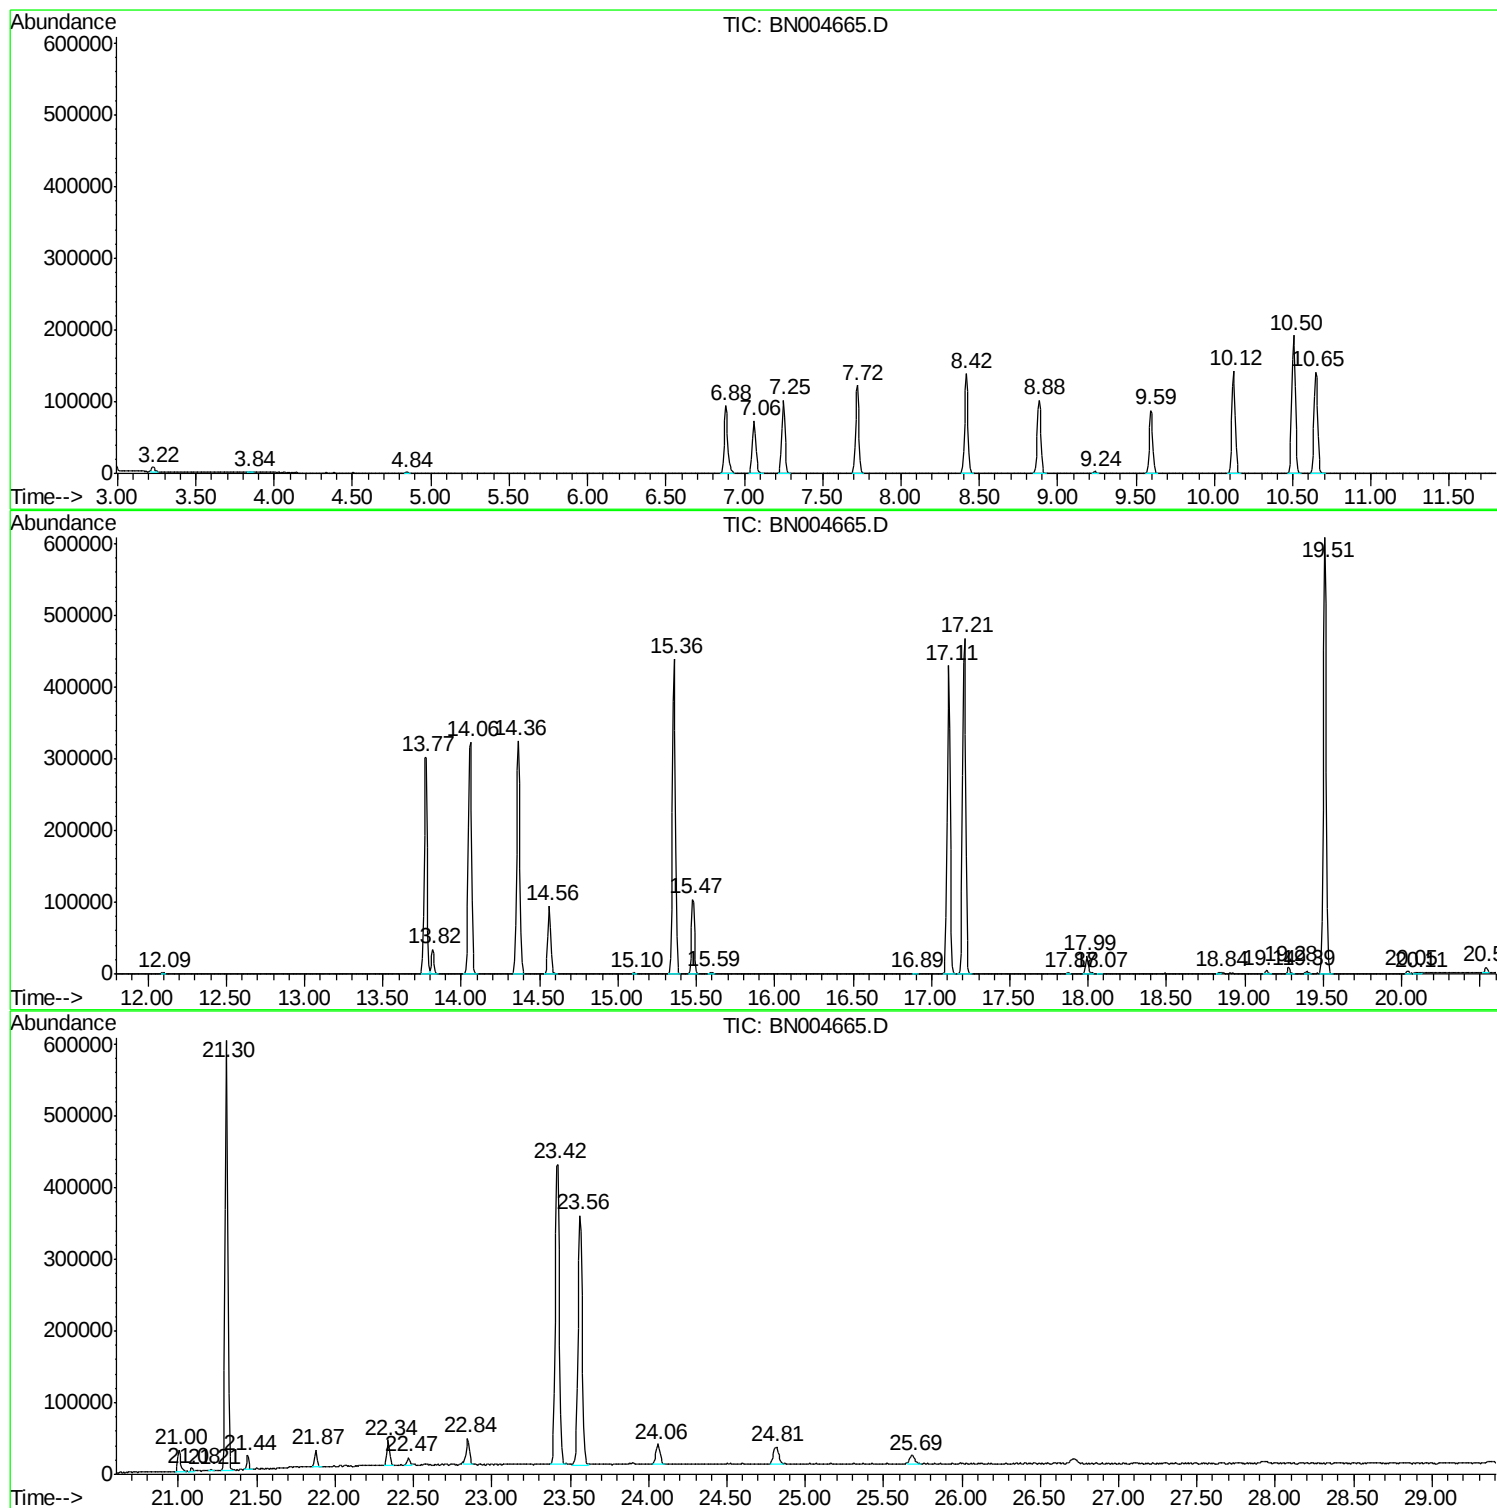

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
Data File : BN004665.D
Acq On : 08 Mar 2019 07:46
Operator : JU/SJ
Sample : K1662-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFC65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030719\
Data File : BN004665.D
Acq On : 08 Mar 2019 07:46
Operator : JU/SJ
Sample : K1662-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFC65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc