


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030722\
 Data File : BN018855.D
 Acq On : 07 Mar 2022 12:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN030322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 03 00:44:34 2022

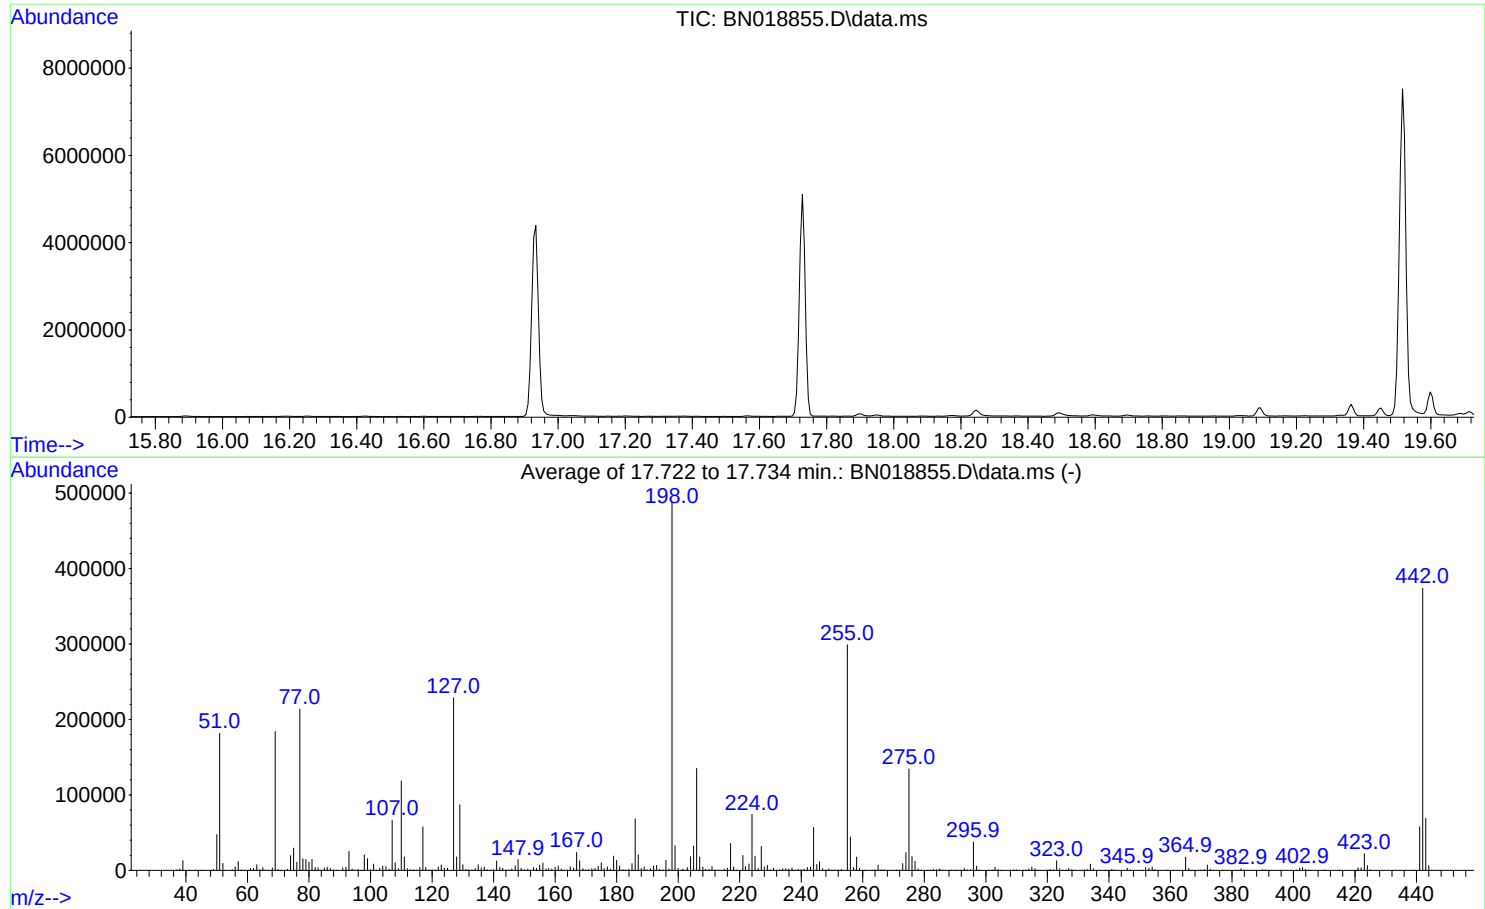




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	181612	PASS
68	69	0.00	2	1.7	3217	PASS
69	198	0.00	100	37.8	184178	PASS
70	69	0.00	2	0.6	1041	PASS
127	198	10	80	46.9	228629	PASS
197	198	0.00	2	0.4	1953	PASS
198	198	100	100	100.0	487573	PASS
199	198	5	9	6.7	32843	PASS
275	198	10	60	27.6	134440	PASS
365	198	1	100	3.6	17451	PASS
441	198	0.01	100	11.8	57603	PASS
442	442	50	100	100.0	373995	PASS
443	442	15	24	18.4	68931	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030722\
Data File : BN018855.D
Acq On : 07 Mar 2022 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 05:27:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 08 05:27:43 2022
Response via : Initial Calibration

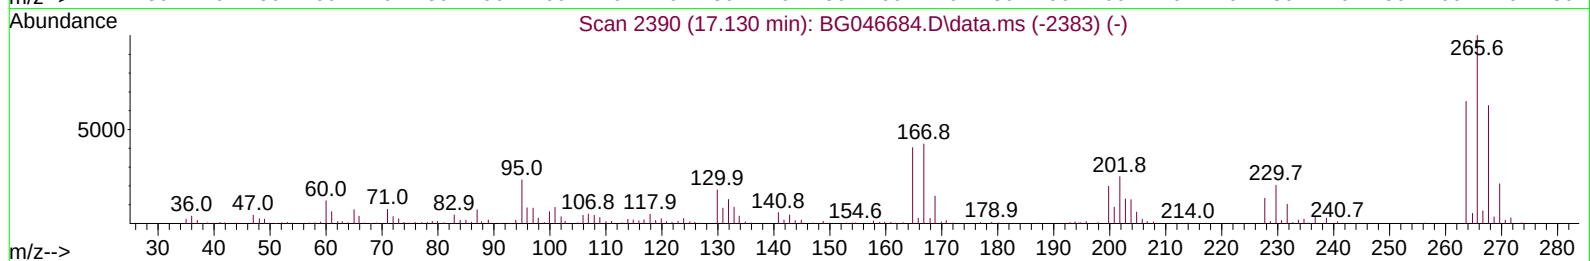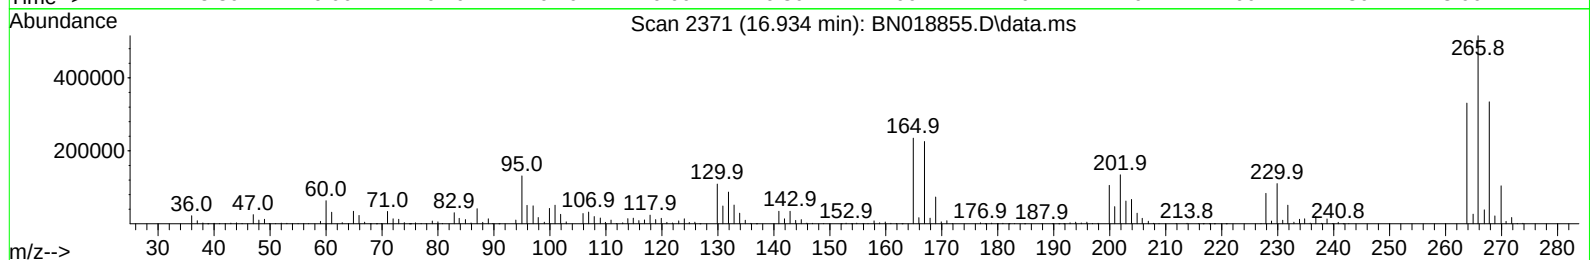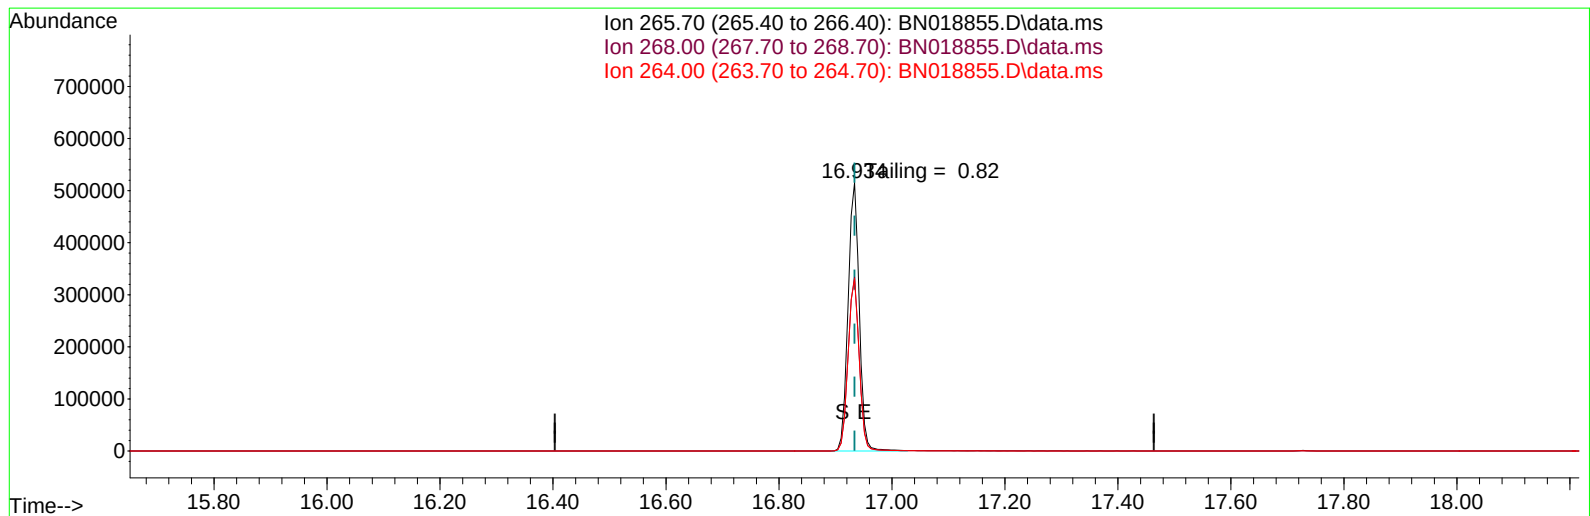

TIC: BN018855.D\data.ms

(70) Pentachlorophenol (C)

16.934min (0.000) 26548.49 ng




response 708376

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.83
264.00	61.60	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030722\
Data File : BN018855.D
Acq On : 07 Mar 2022 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 05:27:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 08 05:27:43 2022
Response via : Initial Calibration

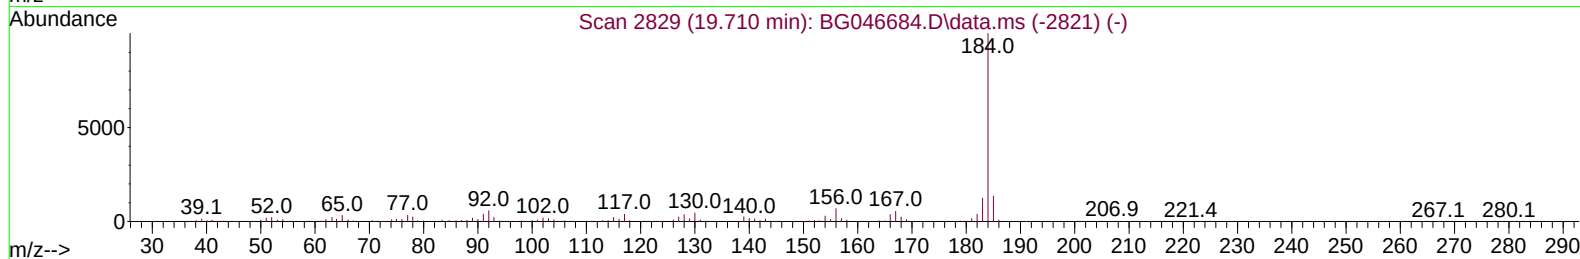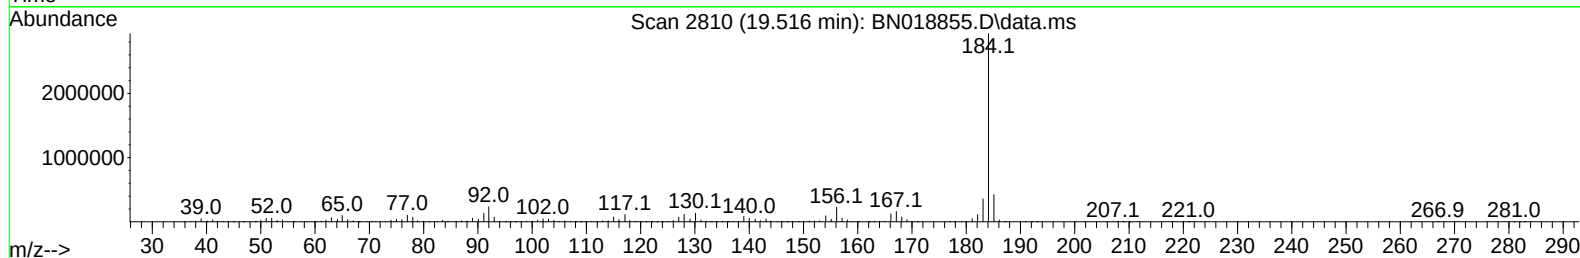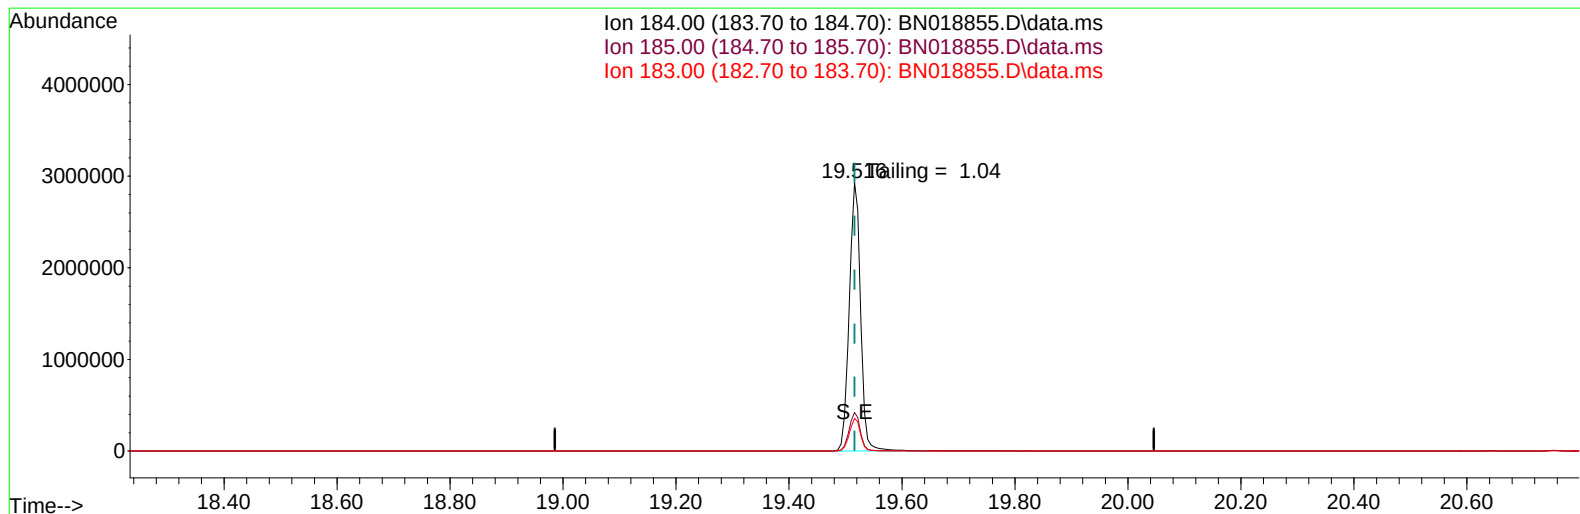

TIC: BN018855.D\data.ms

(77) Benzidine

19.516min (0.000) 0.00 ng

response 4103226

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2022	BNA_N	<u>BN018855.D</u>
Compound Name	Response	Retention Time
DDT	2092852	20.757
DDD	36332	20.316
DDE	1593	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37925	2130777	1.78

Instrument :
BNA_N
ClientSampleId :
DFTPP