
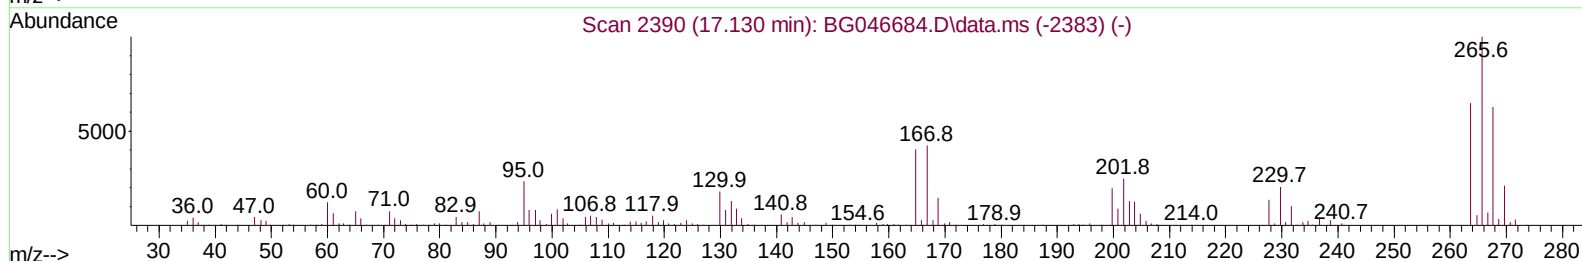
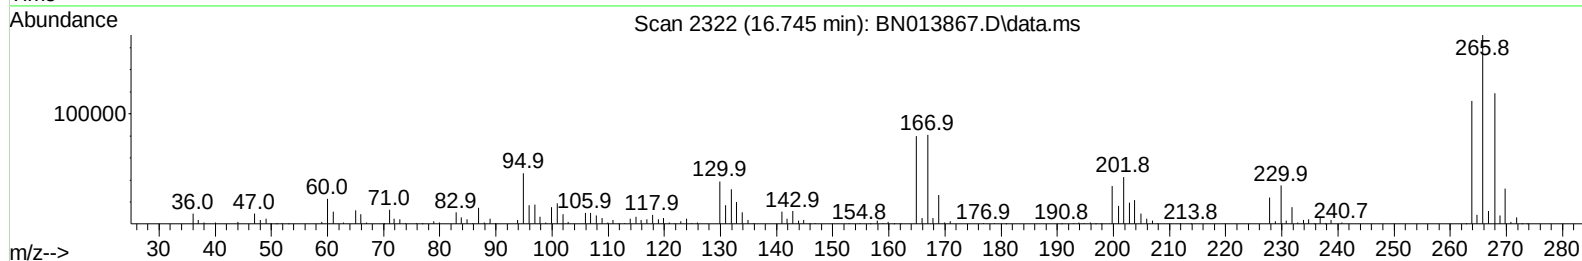


Quant Time: Mar 08 15:27:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

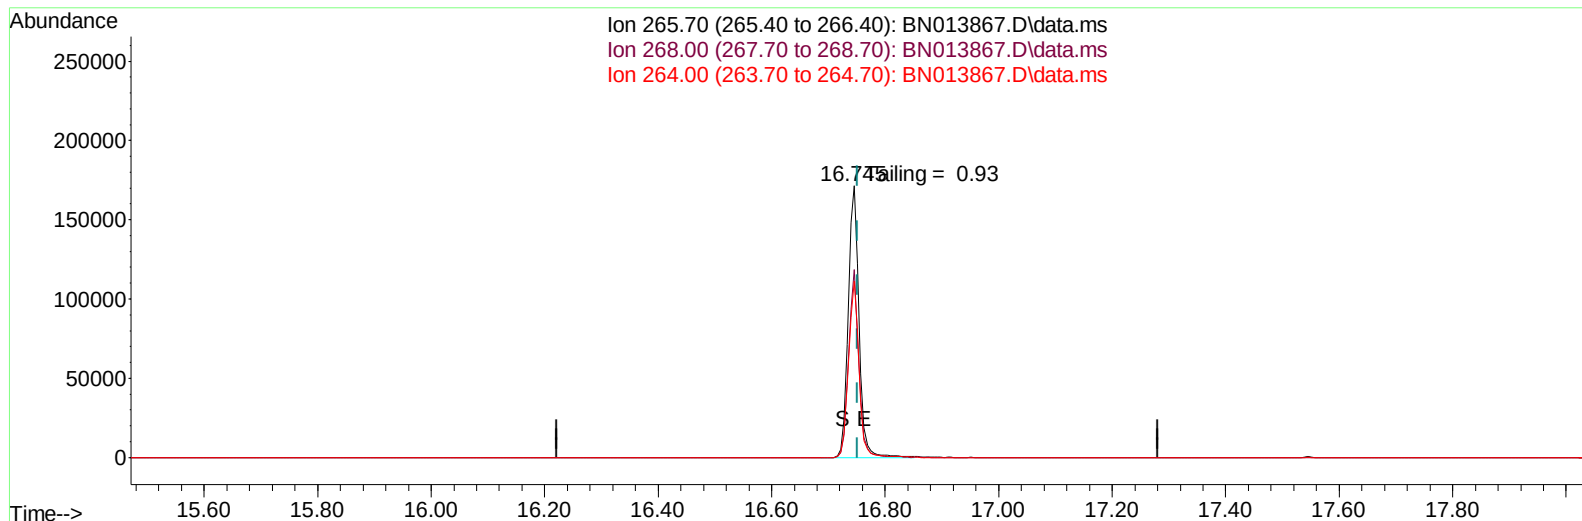




TIC: BN013867.D\data.ms

16.745min (-0.006) 20438.80 ng

response **226162**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.15
264.00	61.60	65.04
0.00	0.00	0.00

Quant Time: Mar 08 15:27:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

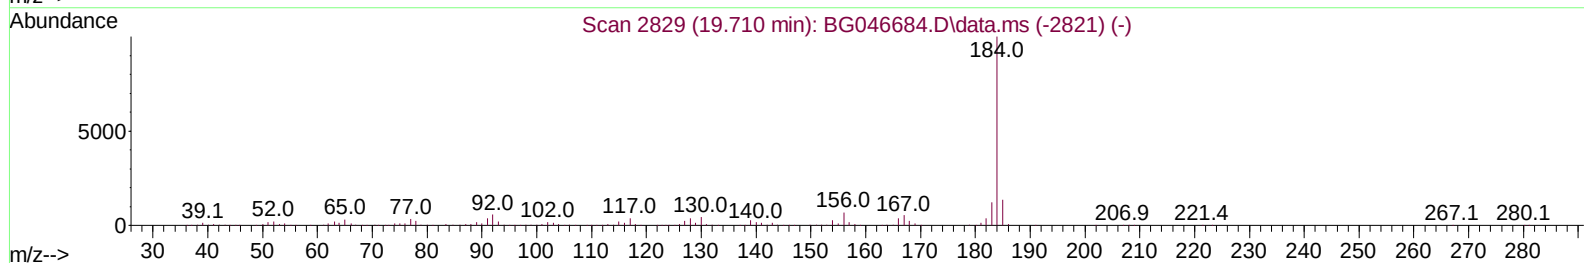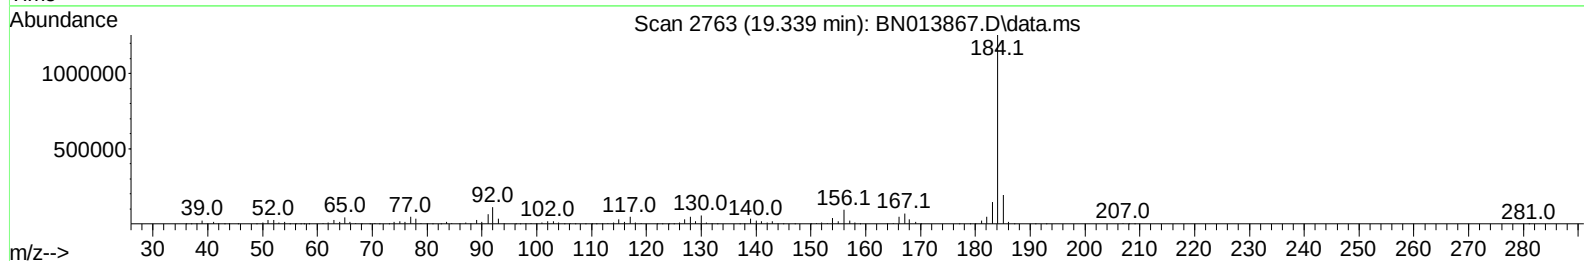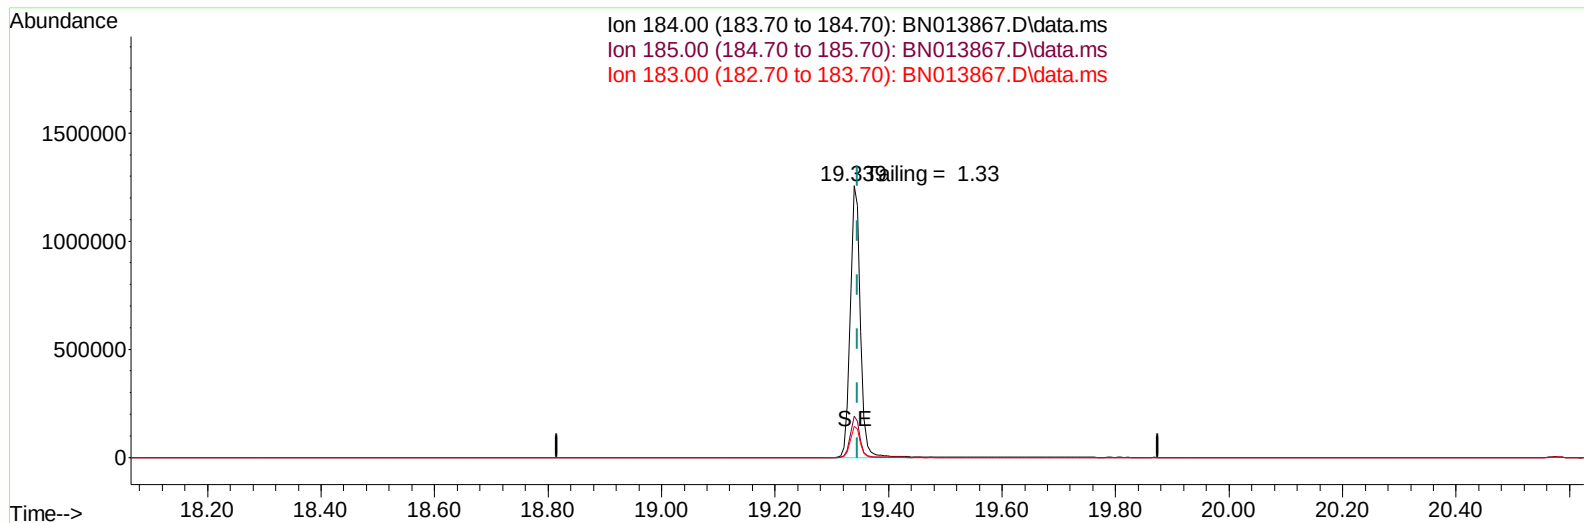

TIC: BN013867.D\data.ms

(77) Benzidine

19.339min (-0.006) 0.00 ng

response **1569237**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.21
183.00	13.20	11.45
0.00	0.00	0.00