

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
 Data File : BN013878.D
 Acq On : 08 Mar 2021 20:11
 Operator : CG/JU
 Sample : M1584-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-VPB-RW6-GW-818-820

Quant Time: Mar 08 23:12:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 08 10:32:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.724	152	5928	0.40	ng	0.00
7) Naphthalene-d8	10.505	136	23160	0.40	ng	# 0.00
13) Acenaphthene-d10	14.346	164	13026	0.40	ng	0.00
19) Phenanthrene-d10	17.092	188	28876	0.40	ng	# 0.00
29) Chrysene-d12	21.271	240	29663	0.40	ng	# 0.00
36) Perylene-d12	23.492	264	28035	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.316	112	1228	0.08	ng	0.00
5) Phenol-d6	6.887	99	1102	0.05	ng	0.00
8) Nitrobenzene-d5	8.857	82	3551	0.24	ng	0.00
11) 2-Methylnaphthalene-d10	12.093	152	8479	0.23	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	778	0.15	ng	0.00
15) 2-Fluorobiphenyl	12.976	172	12435	0.27	ng	0.00
27) Fluoranthene-d10	19.119	212	23073	0.27	ng	0.00
31) Terphenyl-d14	19.719	244	30844	0.47	ng	0.00
Target Compounds						Qvalue
25) Phenanthrene	17.128	178	4611	0.06	ng	# 94
34) Bis(2-ethylhexyl)phtha...	21.186	149	59339	1.37	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
Data File : BN013878.D
Acq On : 08 Mar 2021 20:11
Operator : CG/JU
Sample : M1584-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820

Quant Time: Mar 08 23:12:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 08 10:32:09 2021
Response via : Initial Calibration




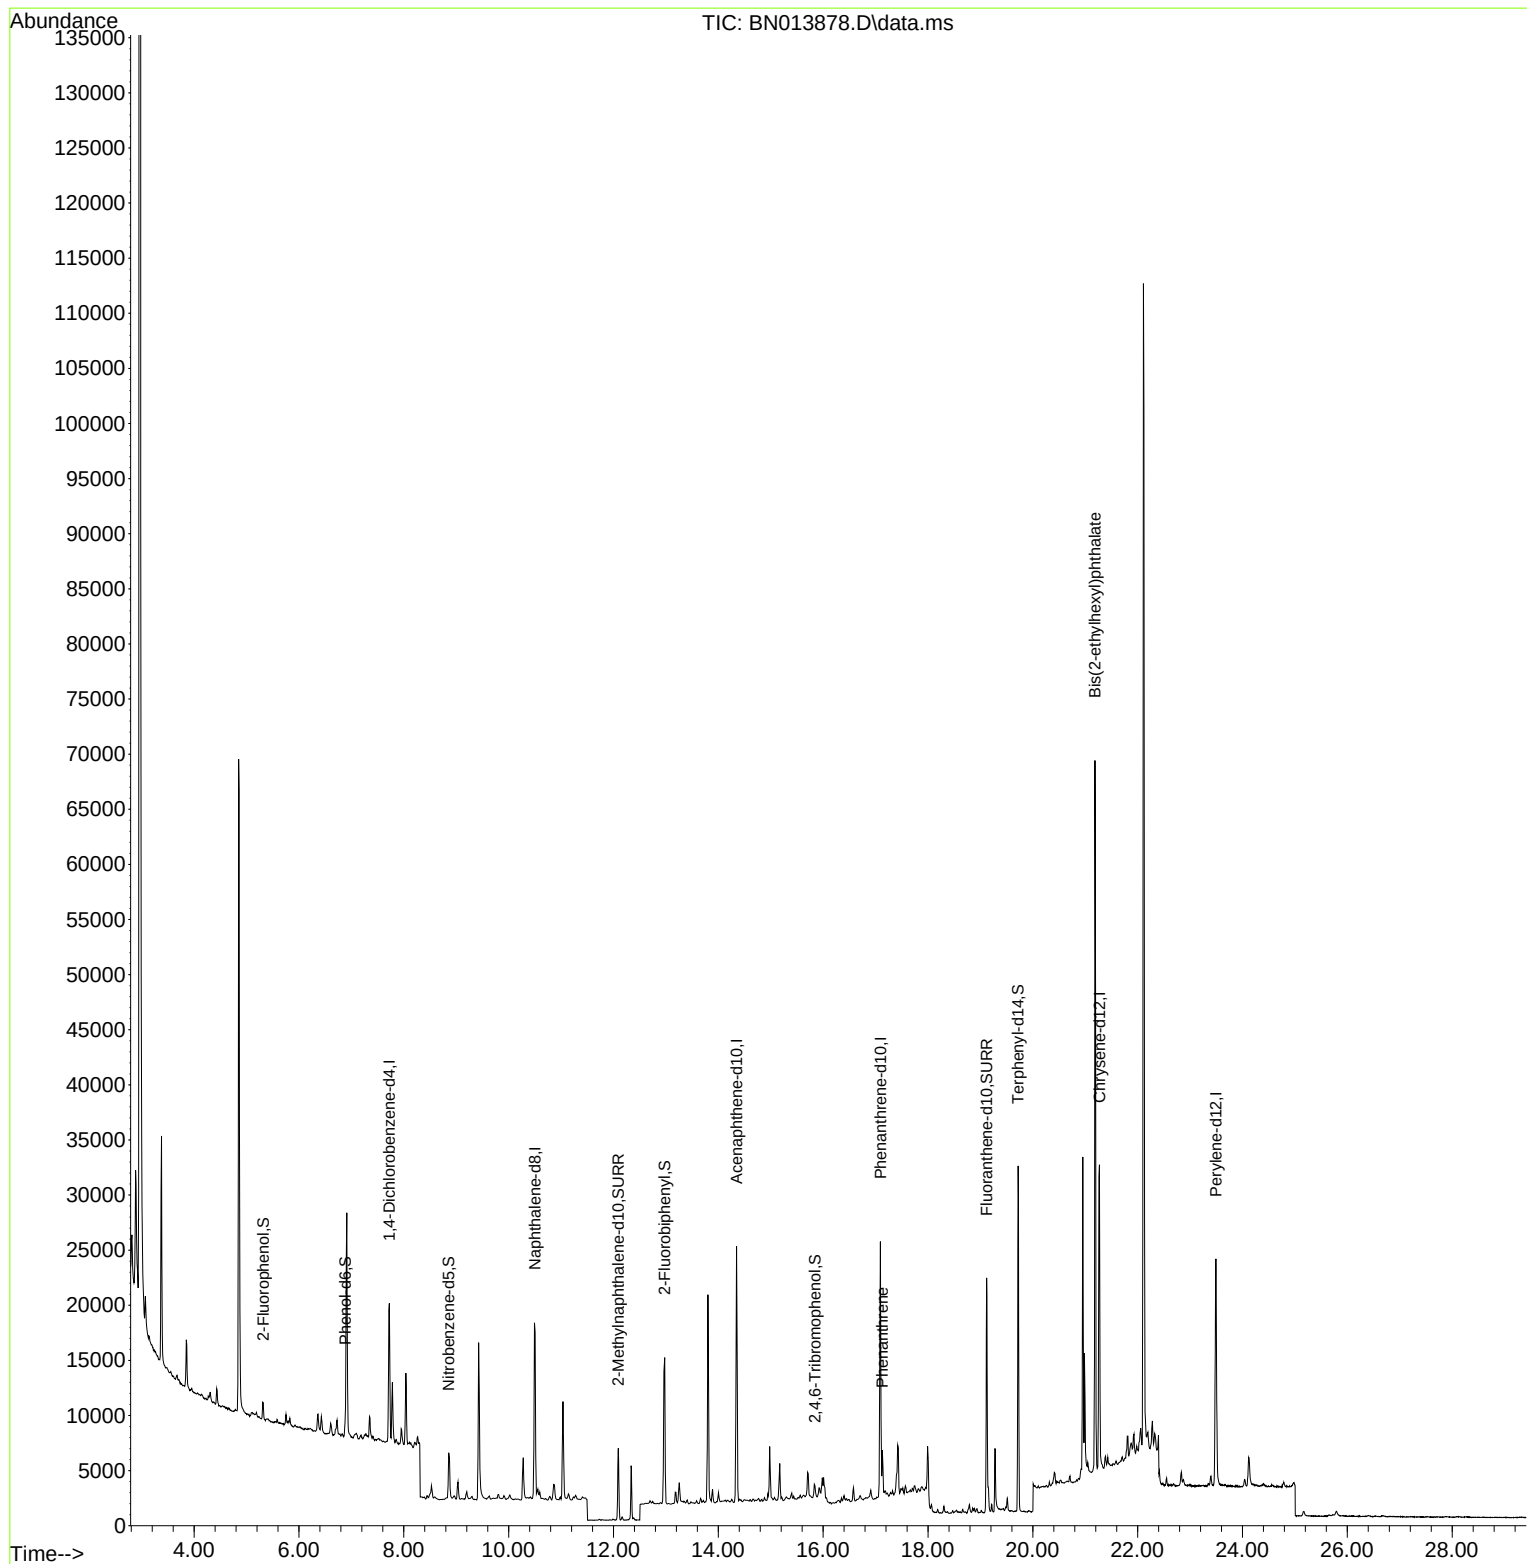


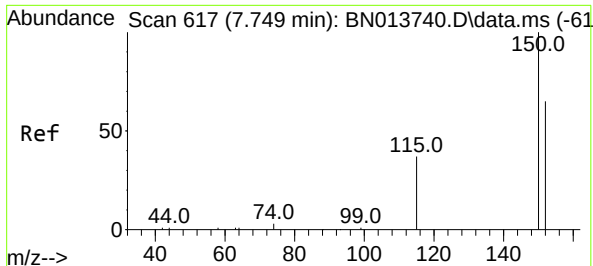

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.724 min Scan# 614
Delta R.T. 0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820


Tgt Ion:152 Resp: 5928
Ion Ratio Lower Upper
152 100
150 153.2 121.8 182.8
115 58.0 46.6 69.8

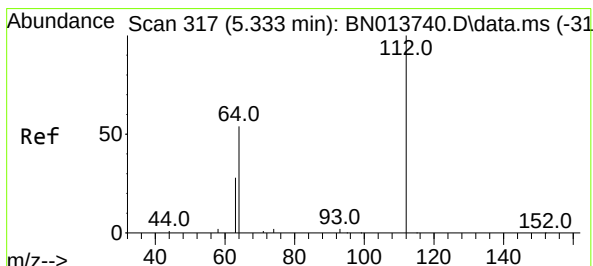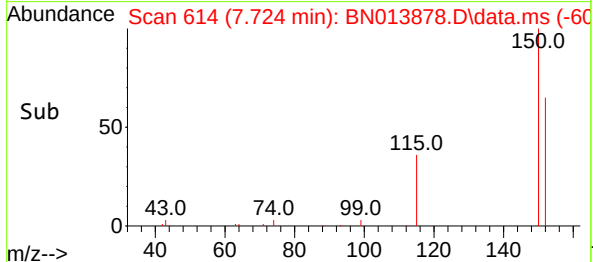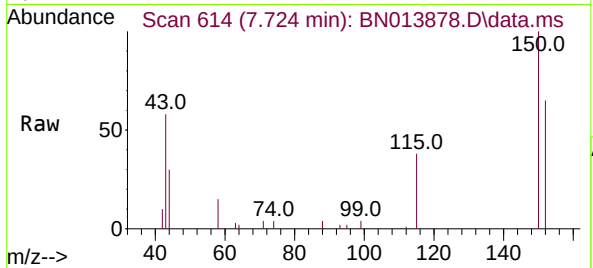

#4
2-Fluorophenol
Concen: 0.08 ng
RT: 5.316 min Scan# 315
Delta R.T. 0.008 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion:112 Resp: 1228
Ion Ratio Lower Upper
112 100
64 59.7 44.3 66.5
63 34.3 23.0 34.6


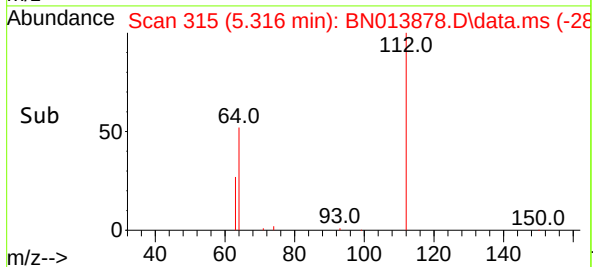

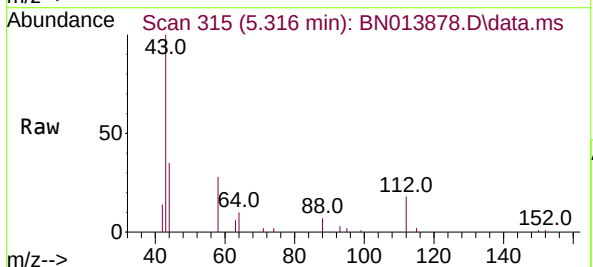


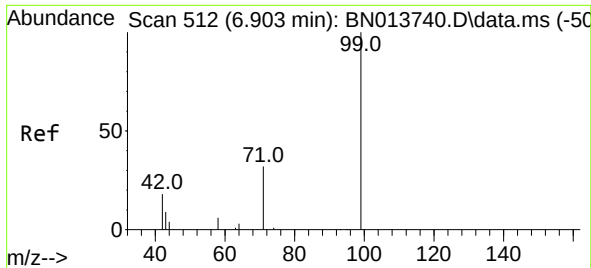

#5
Phenol-d6
Concen: 0.05 ng
RT: 6.887 min Scan# 510
Delta R.T. 0.008 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820


Tgt Ion: 99 Resp: 1102
Ion Ratio Lower Upper
99 100
42 174.7 15.2 22.8#
71 50.9 26.1 39.1#

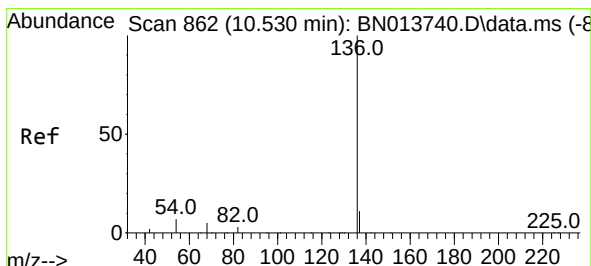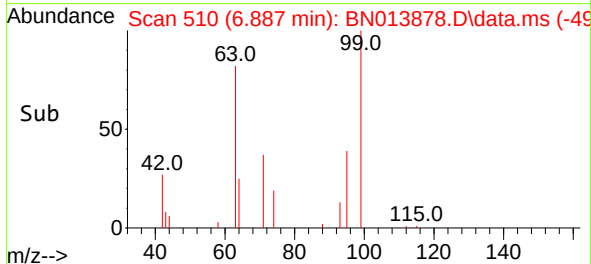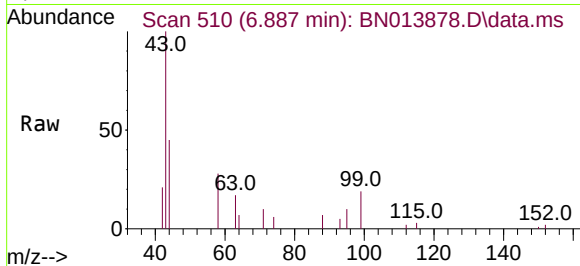

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.505 min Scan# 860
Delta R.T. -0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion: 136 Resp: 23160
Ion Ratio Lower Upper
136 100
137 11.3 9.0 13.6
54 5.9 6.4 9.6#
68 4.6 4.5 6.7


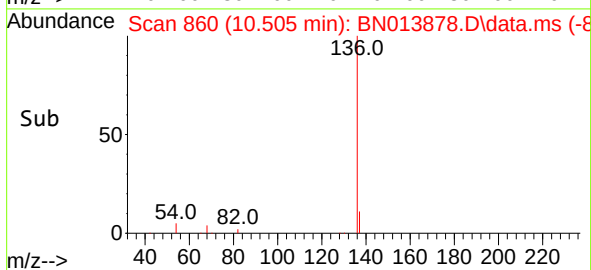

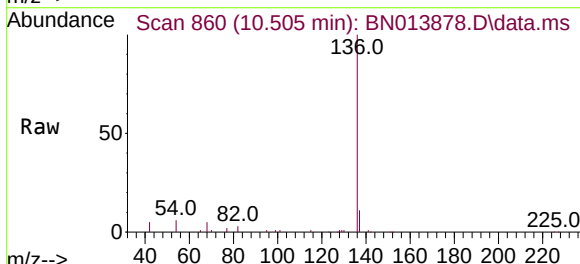


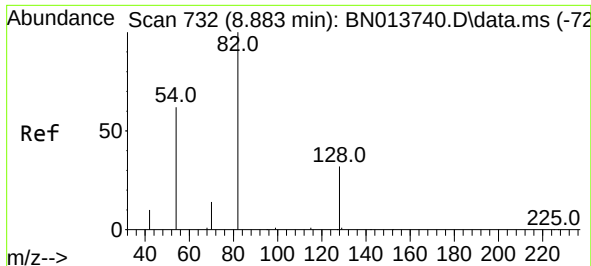

#8
Nitrobenzene-d5
Concen: 0.24 ng
RT: 8.857 min Scan# 730
Delta R.T. -0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820


Tgt Ion: 82 Resp: 3551
Ion Ratio Lower Upper
82 100
128 32.9 39.2 58.8#
54 63.8 40.1 60.1#

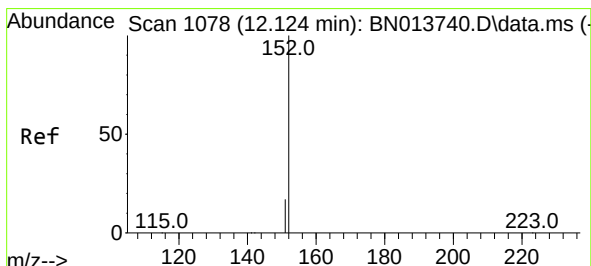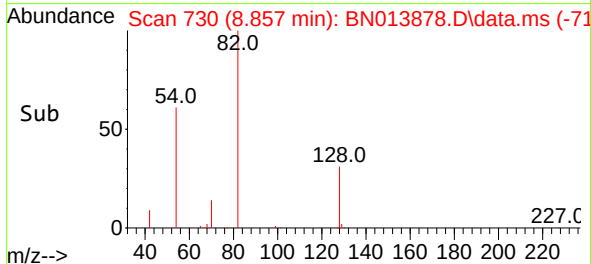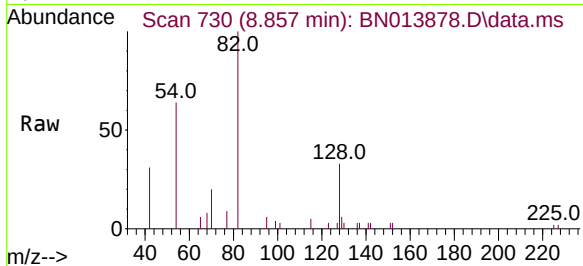

#11
2-Methylnaphthalene-d10
Concen: 0.23 ng
RT: 12.093 min Scan# 1071
Delta R.T. -0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion: 152 Resp: 8479
Ion Ratio Lower Upper
152 100
151 21.0 16.2 24.2


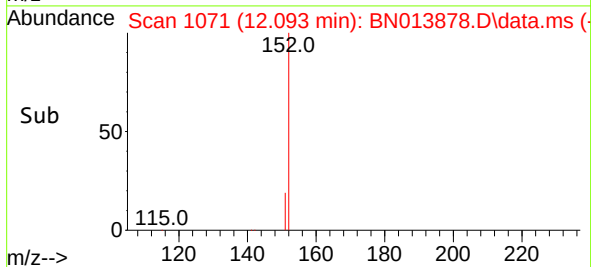

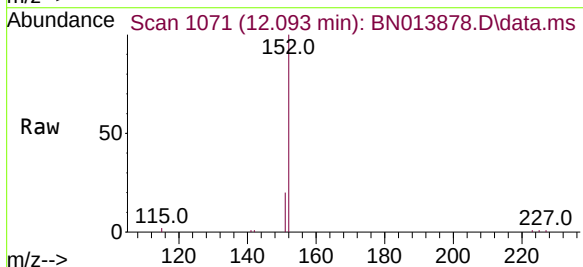


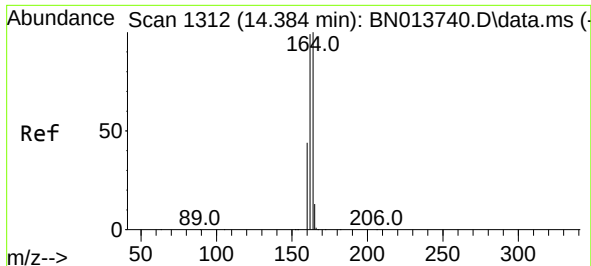

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1309
Delta R.T. -0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820


Tgt Ion:164	Resp:	13026
Ion Ratio	Lower	Upper
164	100	
162	103.2	79.6 119.4
160	47.9	36.0 54.0

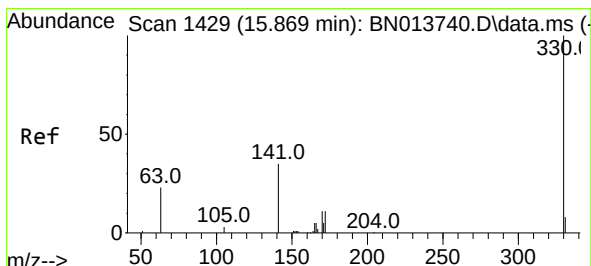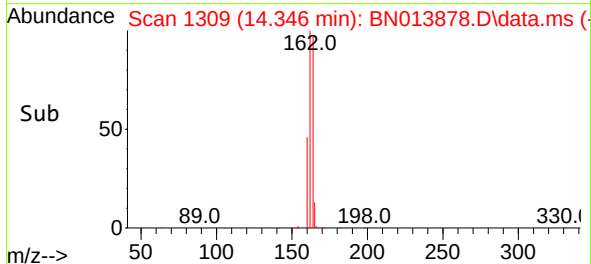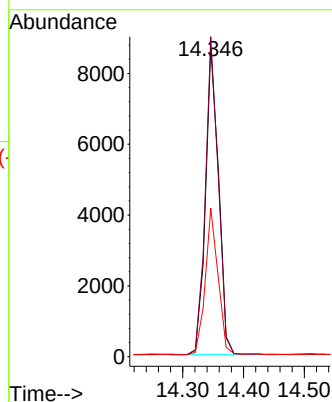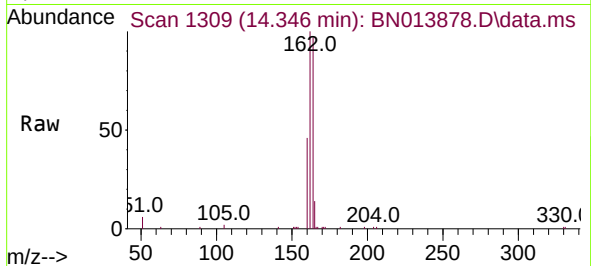

#14
2,4,6-Tribromophenol
Concen: 0.15 ng
RT: 15.843 min Scan# 1427
Delta R.T. -0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion:330	Resp:	778
Ion Ratio	Lower	Upper
330	100	
332	0.0	0.0 0.0
141	56.4	26.8 40.2#


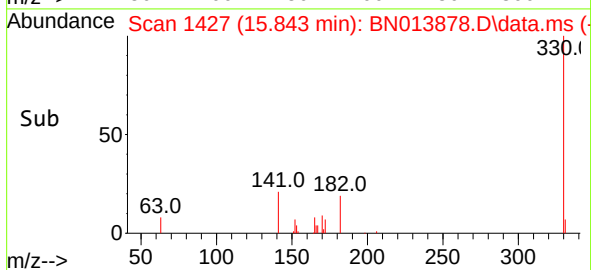

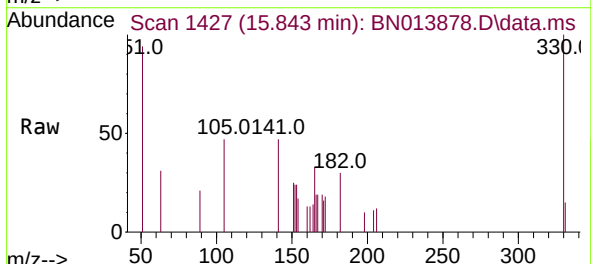


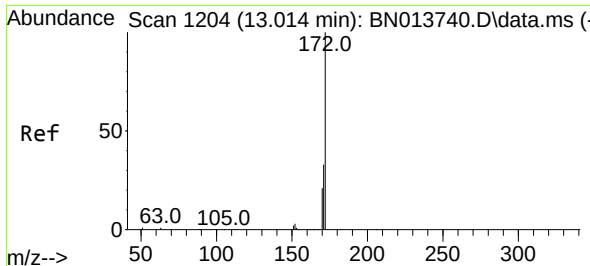

#15
2-Fluorobiphenyl
Concen: 0.27 ng
RT: 12.976 min Scan# 1201
Delta R.T. -0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820


Tgt Ion:172	Resp:	12435
Ion Ratio	Lower	Upper
172	100	
171	33.6	28.6 42.8
170	22.3	18.9 28.3

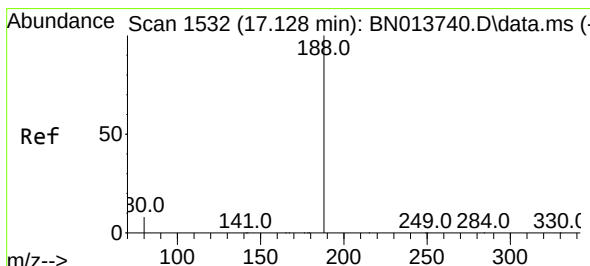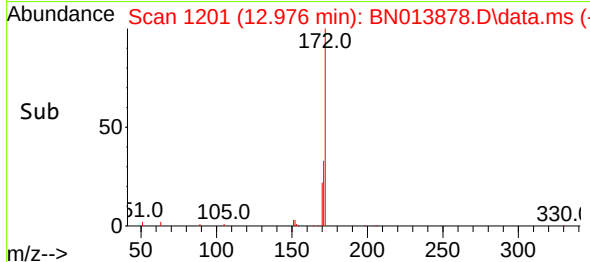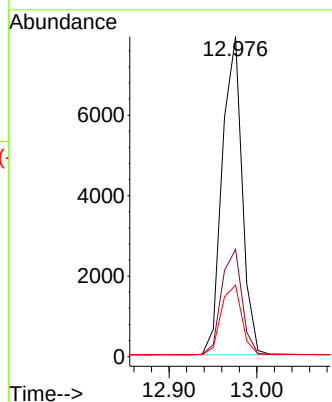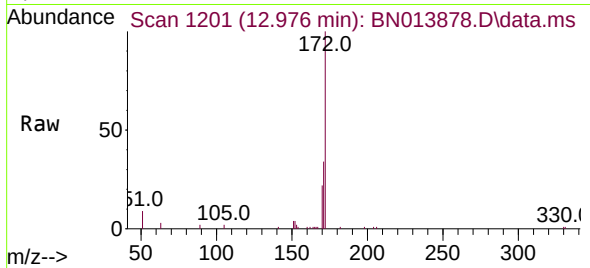

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.092 min Scan# 1529
Delta R.T. 0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion:188	Resp:	28876
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	8.6	9.0 13.6#


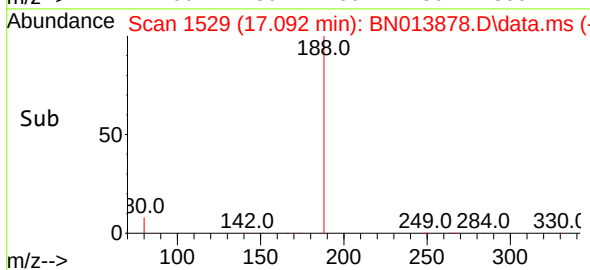

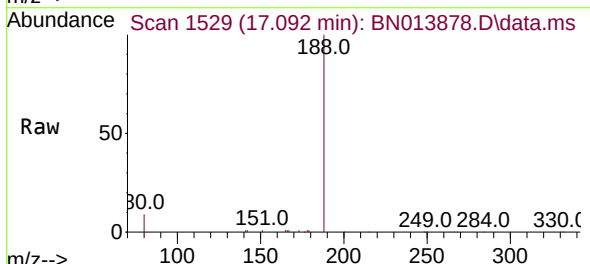


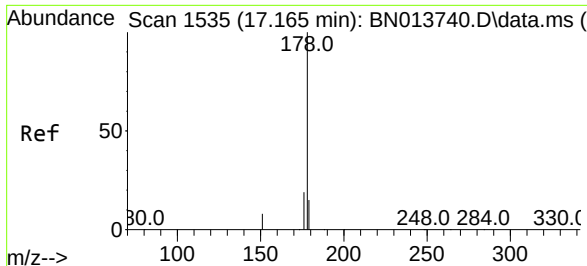

#25
Phenanthrene
Concen: 0.06 ng
RT: 17.128 min Scan# 1532
Delta R.T. 0.000 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820


Tgt Ion:178 Resp: 4611
Ion Ratio Lower Upper
178 100
176 19.1 15.0 22.4
179 20.2 12.3 18.5#

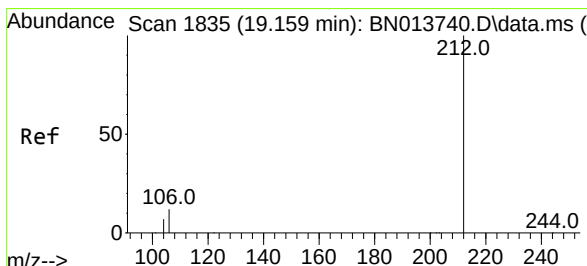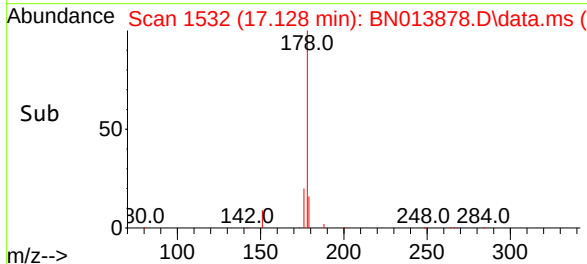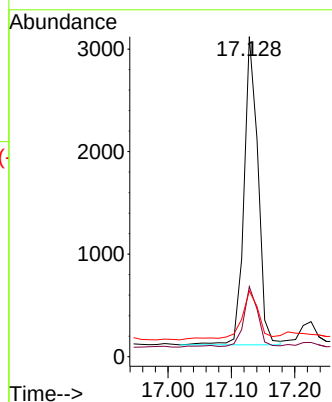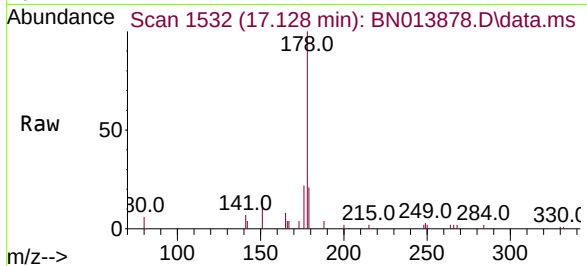

#27
Fluoranthene-d10
Concen: 0.27 ng
RT: 19.119 min Scan# 1827
Delta R.T. -0.002 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion:212 Resp: 23073
Ion Ratio Lower Upper
212 100
106 13.2 9.7 14.5
104 7.8 5.5 8.3


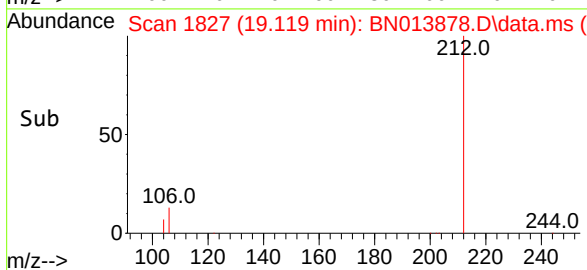

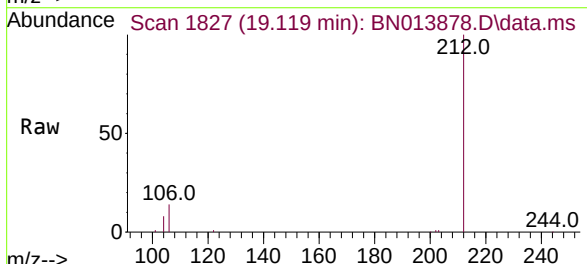


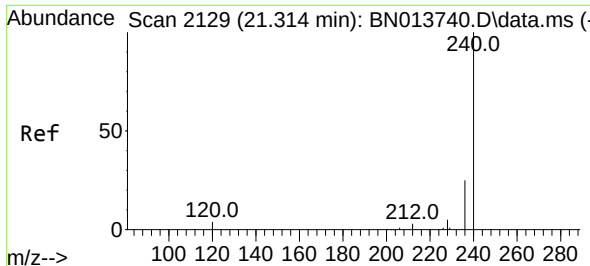

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.271 min Scan# 2125
Delta R.T. 0.003 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820


Tgt Ion:240 Resp: 29663
Ion Ratio Lower Upper
240 100
120 6.7 10.2 15.4#
236 25.7 21.3 31.9

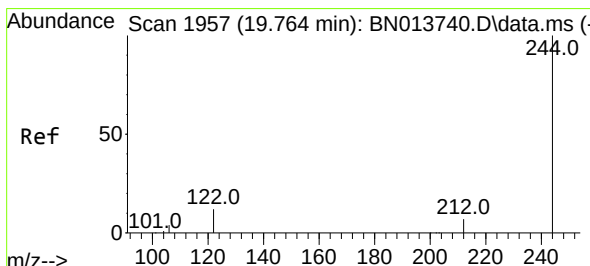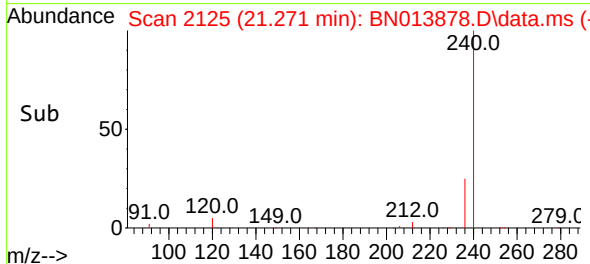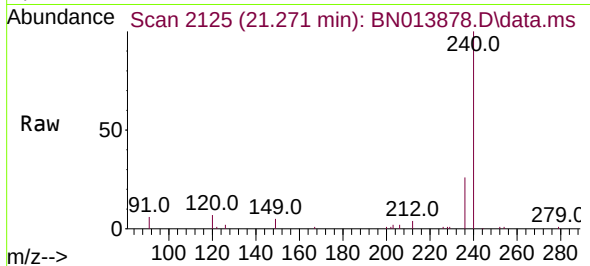

#31
Terphenyl-d14
Concen: 0.47 ng
RT: 19.719 min Scan# 1948
Delta R.T. -0.002 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion:244 Resp: 30844
Ion Ratio Lower Upper
244 100
212 7.9 6.1 9.1
122 12.9 9.8 14.8


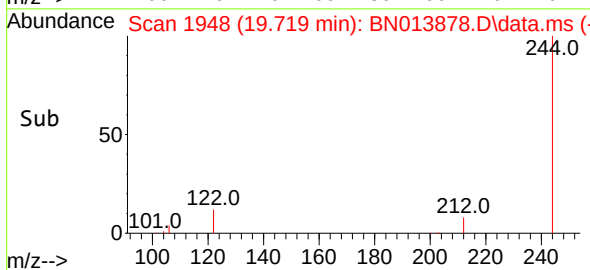

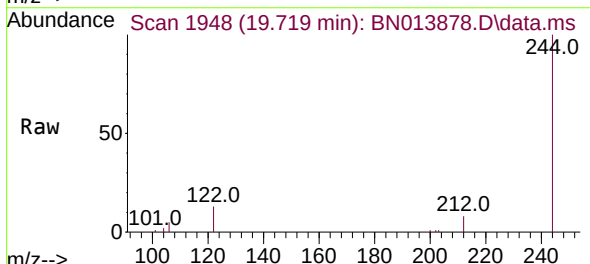


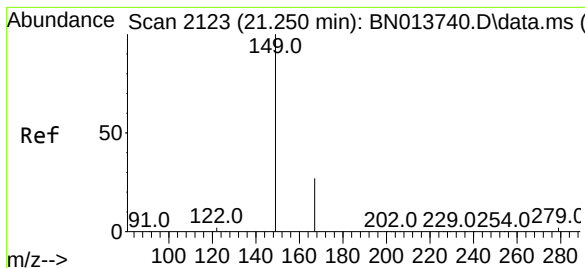

#34
Bis(2-ethylhexyl)phthalate
Concen: 1.37 ng
RT: 21.186 min Scan# 2117
Delta R.T. -0.008 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW6-GW-818-820

Tgt Ion:	149	Resp:	59339
Ion Ratio	Lower	Upper	
149	100		
167	27.0	22.1	33.1
279	3.9	3.5	5.3

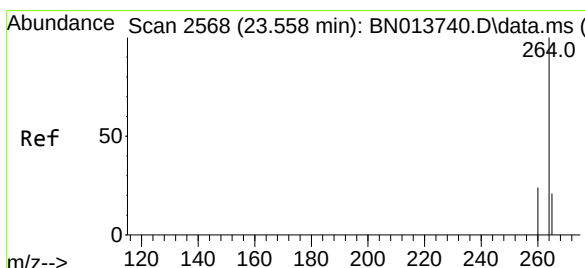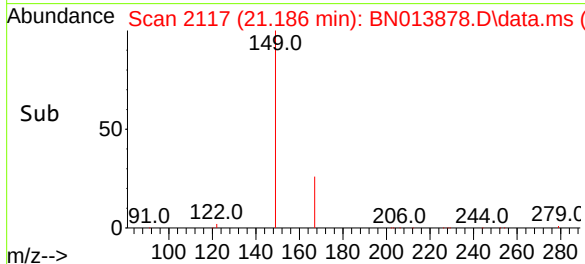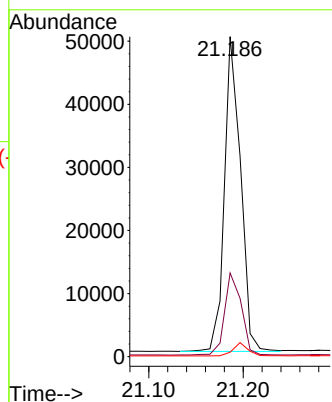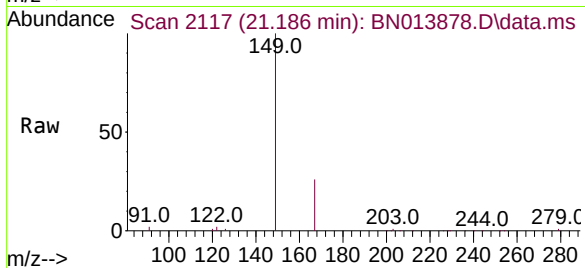

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.492 min Scan# 2549
Delta R.T. -0.001 min
Lab File: BN013878.D
Acq: 08 Mar 2021 20:11

Tgt Ion:	264	Resp:	28035
Ion Ratio	Lower	Upper	
264	100		
260	24.8	19.3	28.9
265	32.3	66.2	99.4#

