
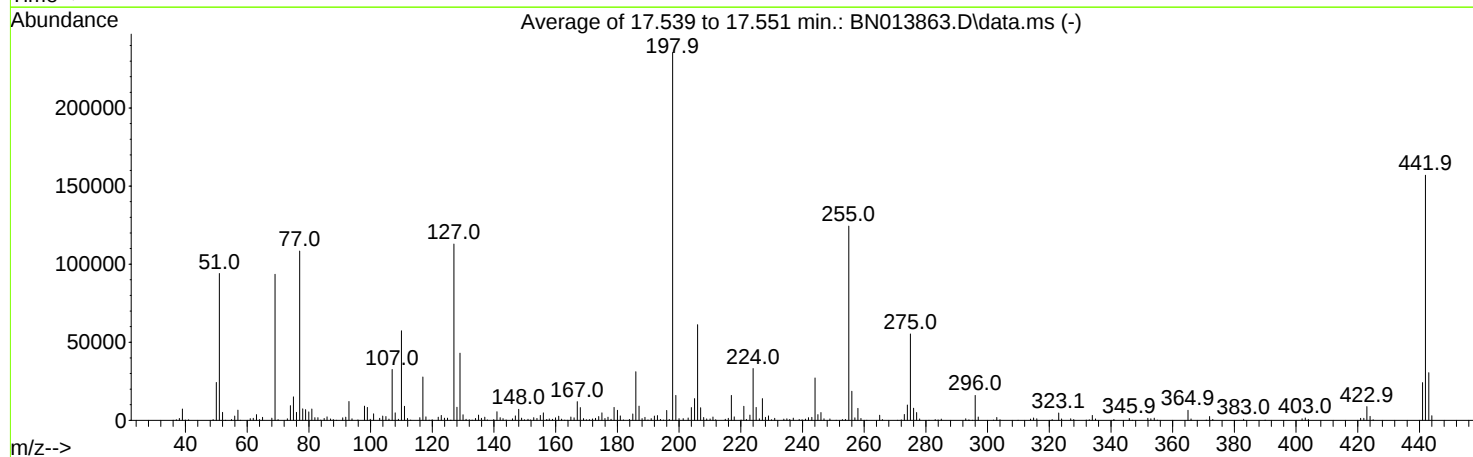


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
 Data File : BN013863.D
 Acq On : 08 Mar 2021 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 08 10:32:09 2021

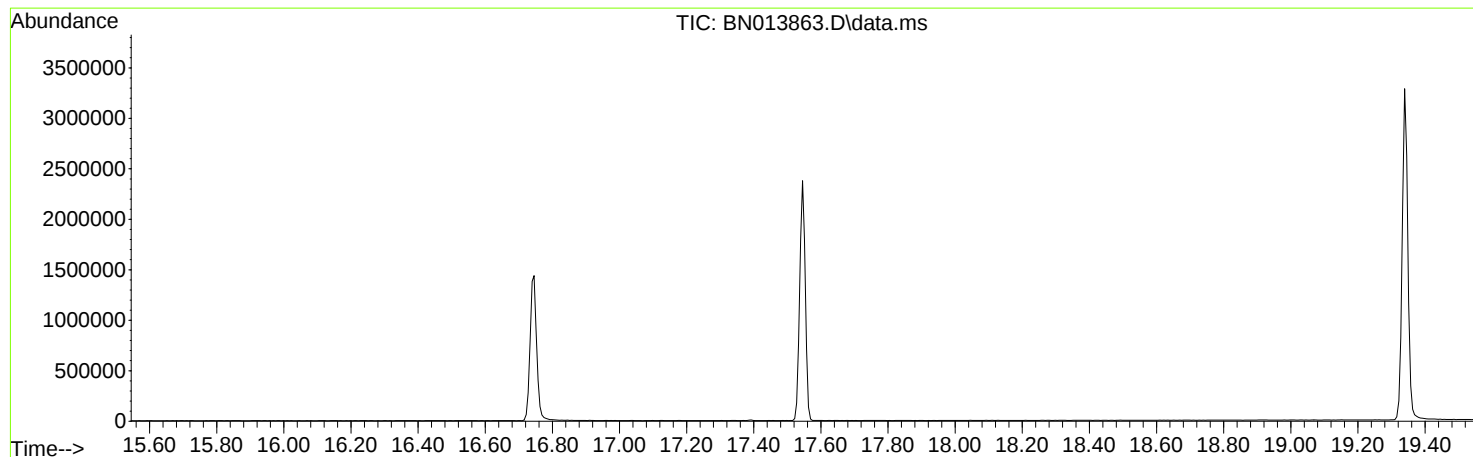

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451




Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	94072	PASS
68	69	0.00	2	1.6	1485	PASS
69	198	0.00	100	39.7	93493	PASS
70	69	0.00	2	0.6	521	PASS
127	198	10	80	47.9	112853	PASS
197	198	0.00	2	0.3	635	PASS
198	198	100	100	100.0	235520	PASS
199	198	5	9	6.8	15980	PASS
275	198	10	60	23.5	55293	PASS
365	198	1	100	2.7	6437	PASS
441	198	0.01	100	10.3	24163	PASS
442	442	50	100	100.0	156909	PASS
443	442	15	24	19.5	30581	PASS

	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
3/8/2021	BNA_N	<u>BN013863.D</u>
Compound Name	Response	Retention Time
DDT	745216	20.575
DDD	2270	20.133
DDE	1013	19.628
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3283	748499	0.44

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
Data File : BN013863.D
Acq On : 08 Mar 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 10:14:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

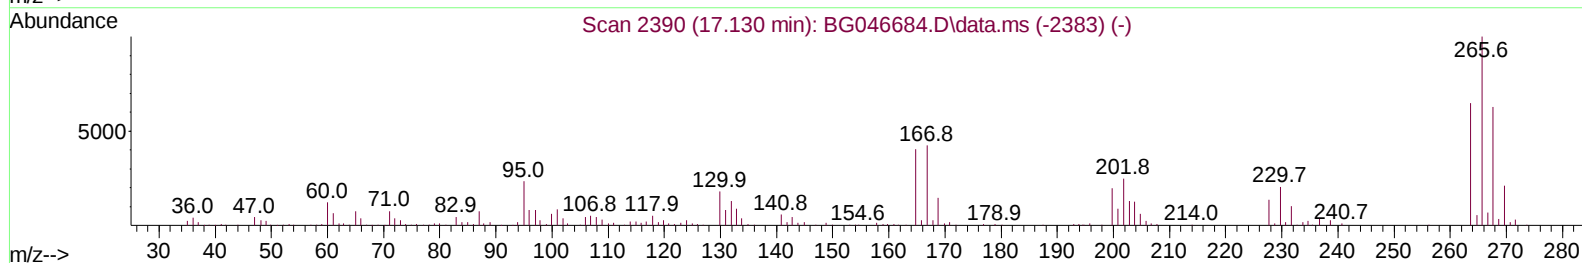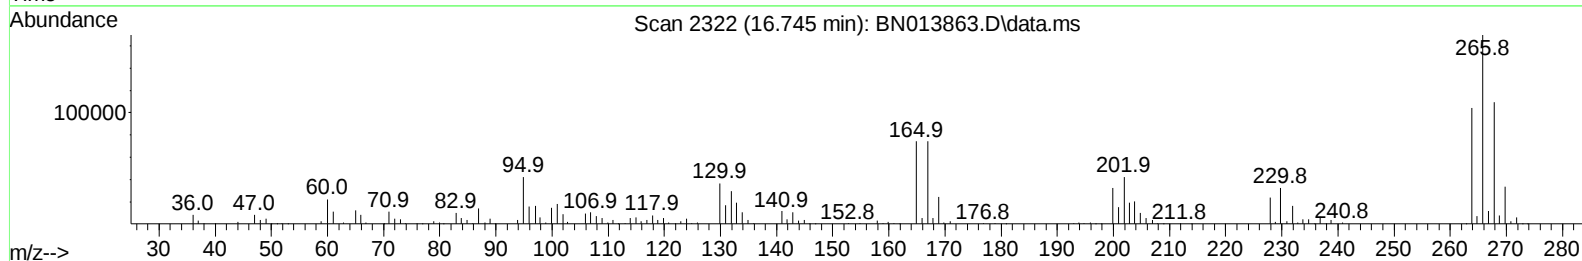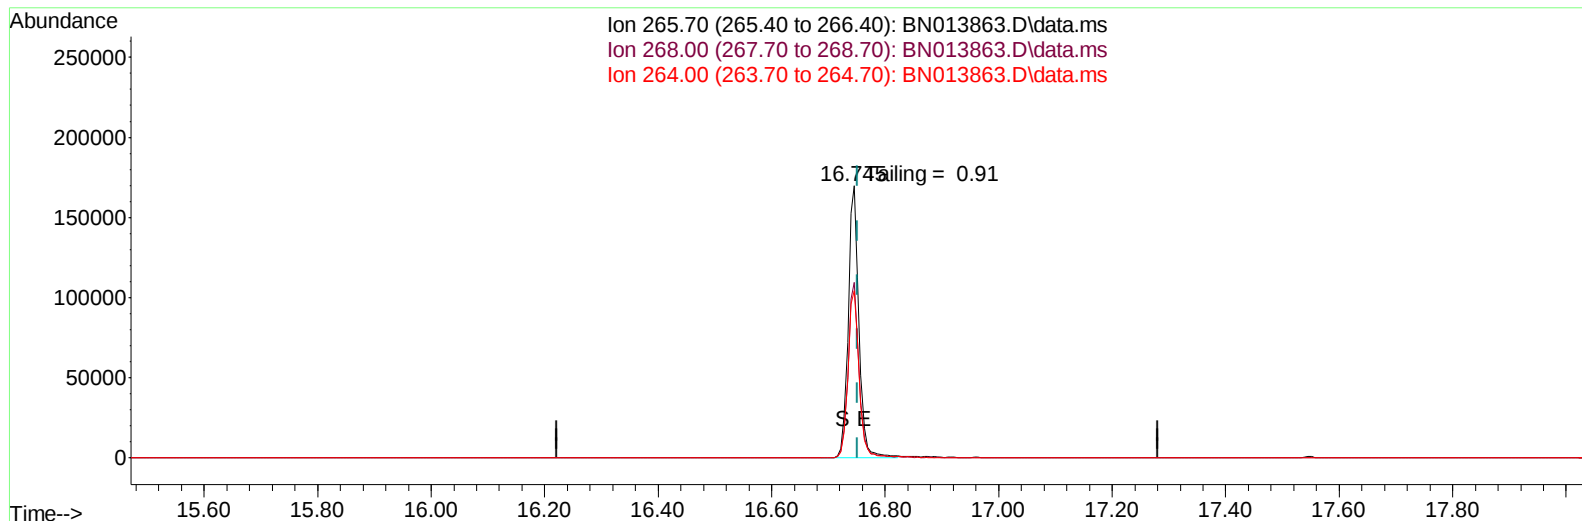

TIC: BN013863.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 20010.47 ng




response 224092

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.47
264.00	61.60	61.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
Data File : BN013863.D
Acq On : 08 Mar 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 10:14:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

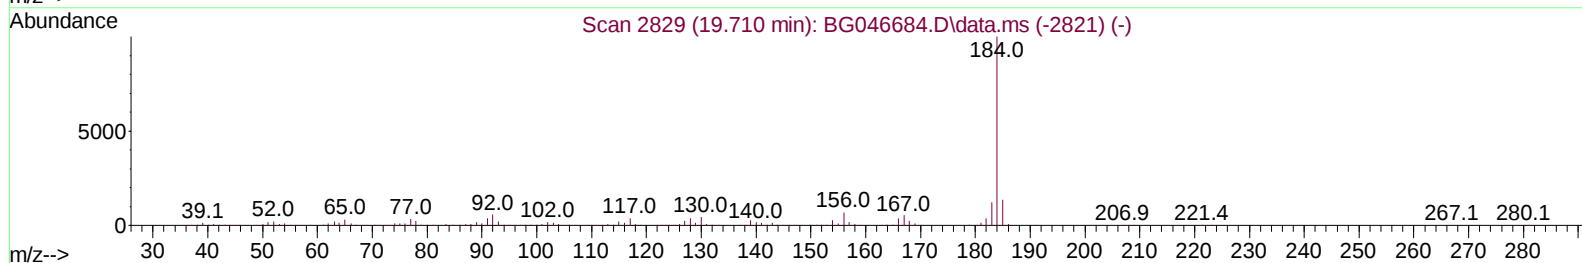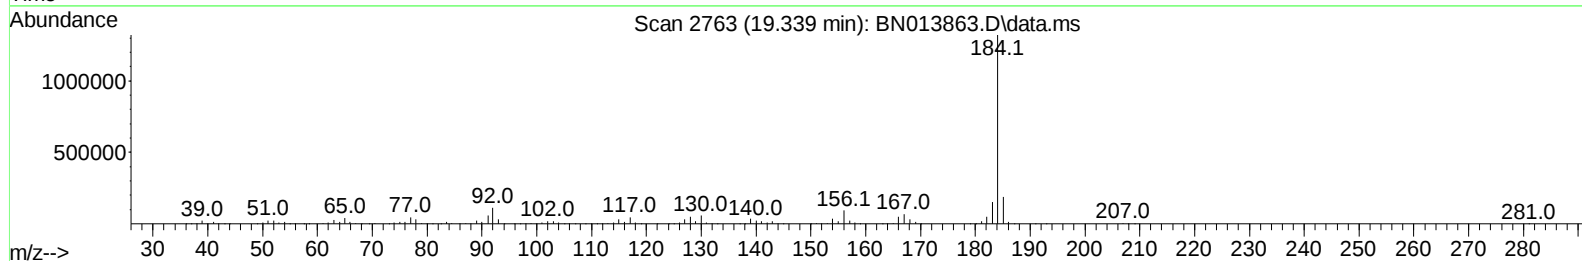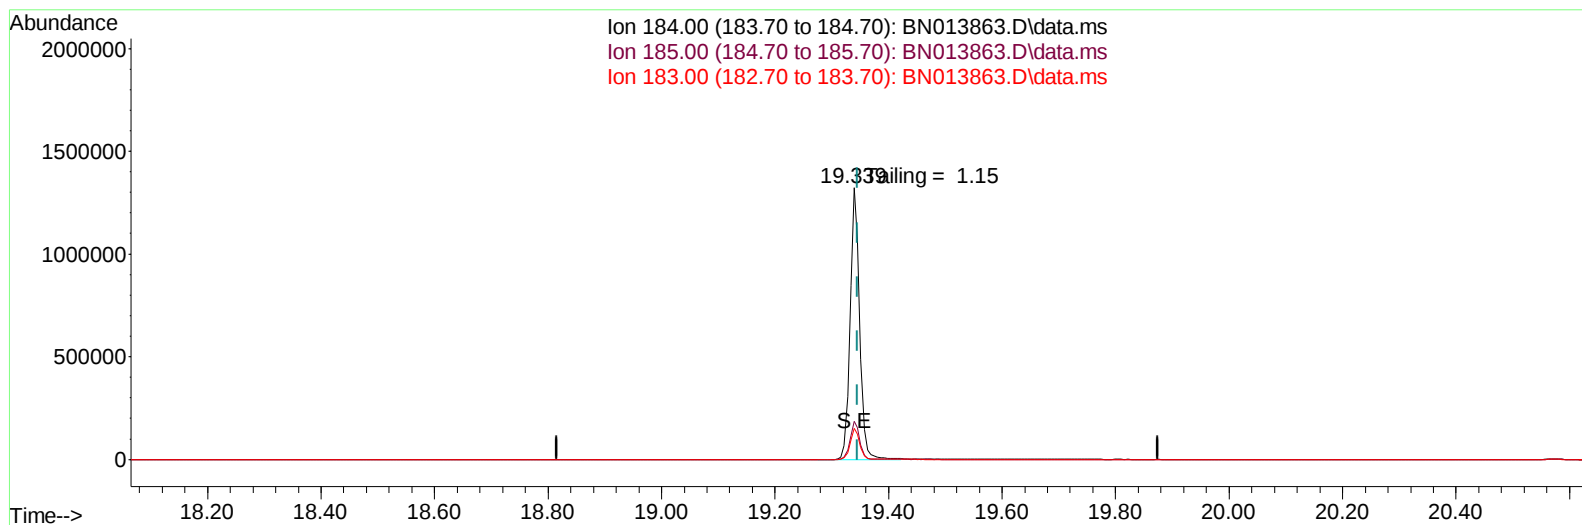

TIC: BN013863.D\data.ms

(77) Benzidine

19.339min (-0.006) 0.00 ng

response 1566478

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.11
183.00	13.20	11.57
0.00	0.00	0.00