DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
Data File : BN013867.D
Acq On : 08 Mar 2021 13:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 08 10:32:09 2021

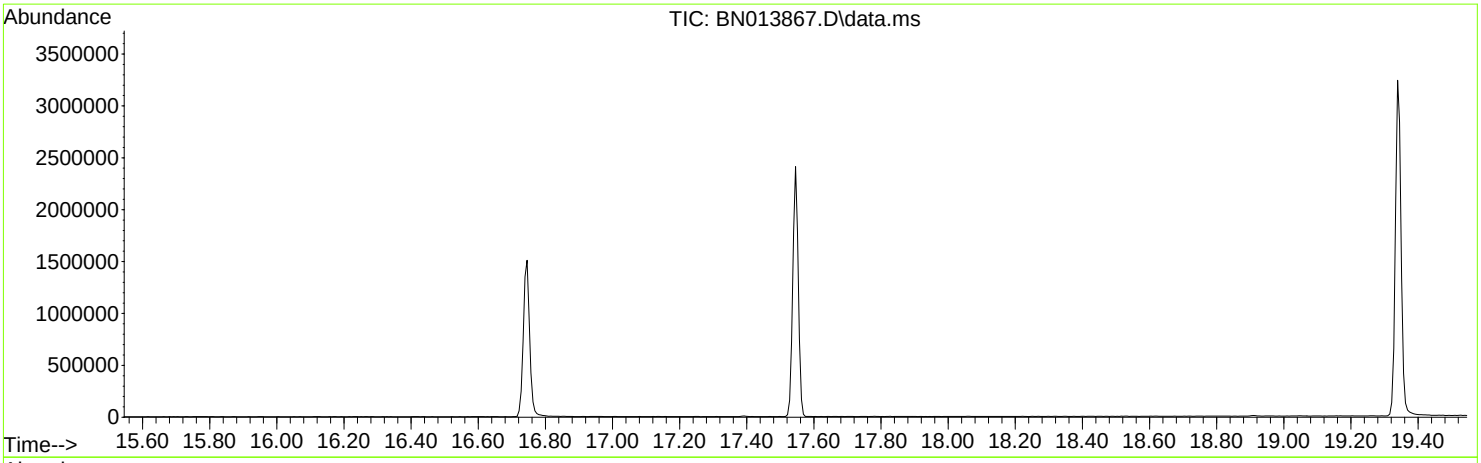

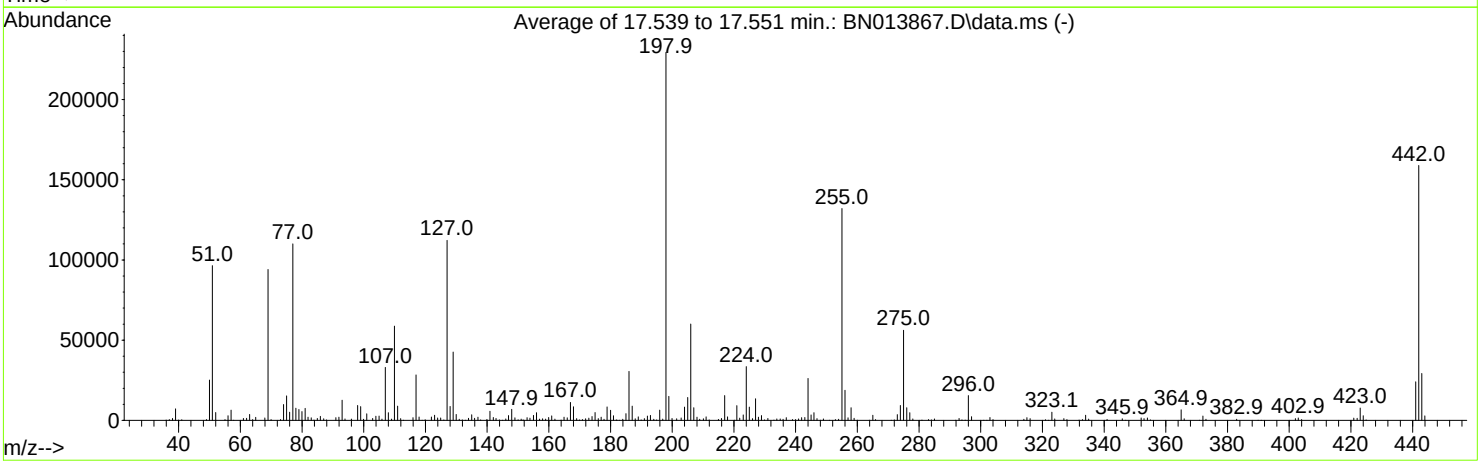

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	96439	PASS
68	69	0.00	2	1.6	1518	PASS
69	198	0.00	100	41.0	94123	PASS
70	69	0.00	2	0.5	499	PASS
127	198	10	80	48.9	112245	PASS
197	198	0.00	2	0.4	847	PASS
198	198	100	100	100.0	229355	PASS
199	198	5	9	6.5	14995	PASS
275	198	10	60	24.5	56171	PASS
365	198	1	100	2.9	6567	PASS
441	198	0.01	100	10.5	24025	PASS
442	442	50	100	100.0	158912	PASS
443	442	15	24	18.4	29261	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP

	DDT Breakdown	
Date	**Instrument Name**	**DFTPP Data File**
3/8/2021	**BNA_N**	**BN013867.D**
Compound Name	**Response**	**Retention Time**
DDT	**754510**	**20.574**
DDD	**3999**	**20.133**
DDE	**867**	**19.633**
SUM(DDD+DDE)	**SUM(DDT+DDD+DDE)**	**% Breakdown Of DDT**
4866	**759376**	**0.64**

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
Data File : BN013867.D
Acq On : 08 Mar 2021 13:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 15:27:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

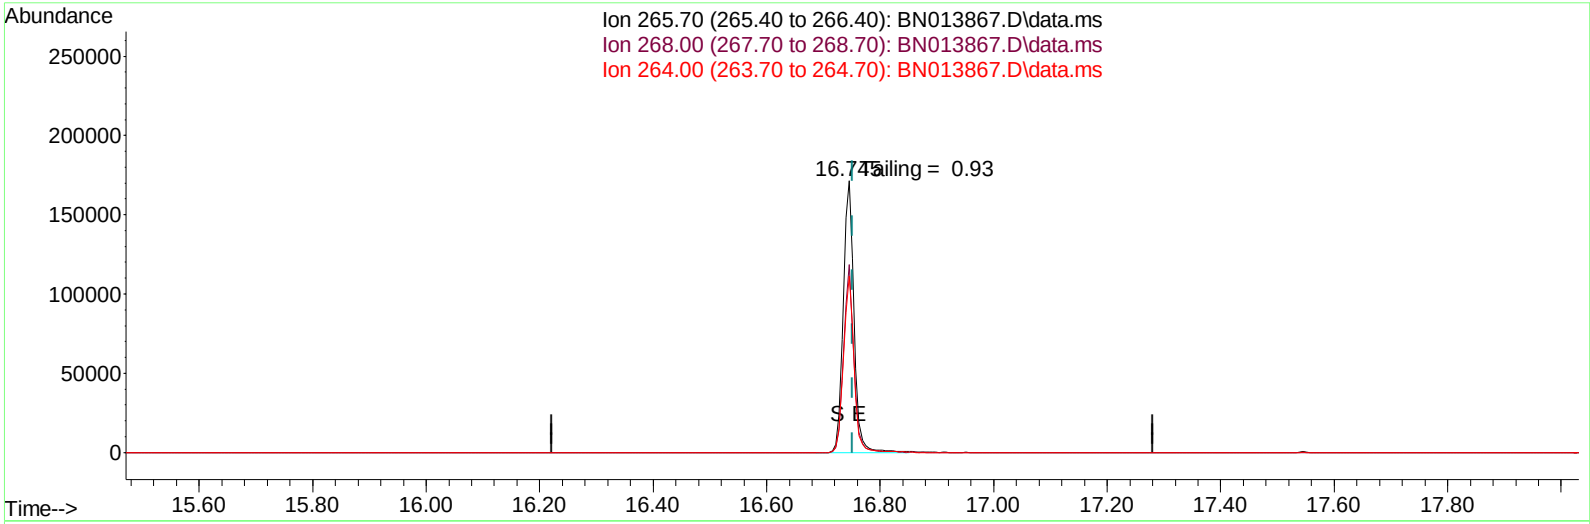

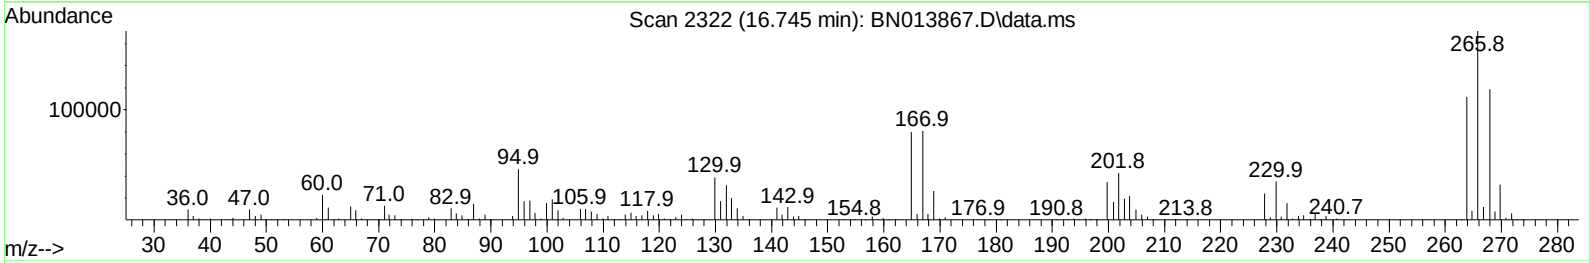

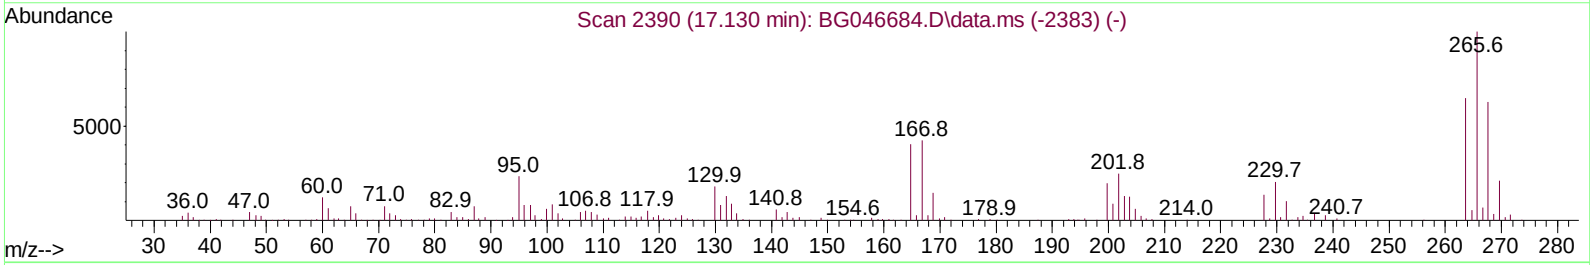

TIC: BN013867.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 20438.80 ng

response 226162

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.15
264.00	61.60	65.04
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030821\
Data File : BN013867.D
Acq On : 08 Mar 2021 13:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 15:27:49 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

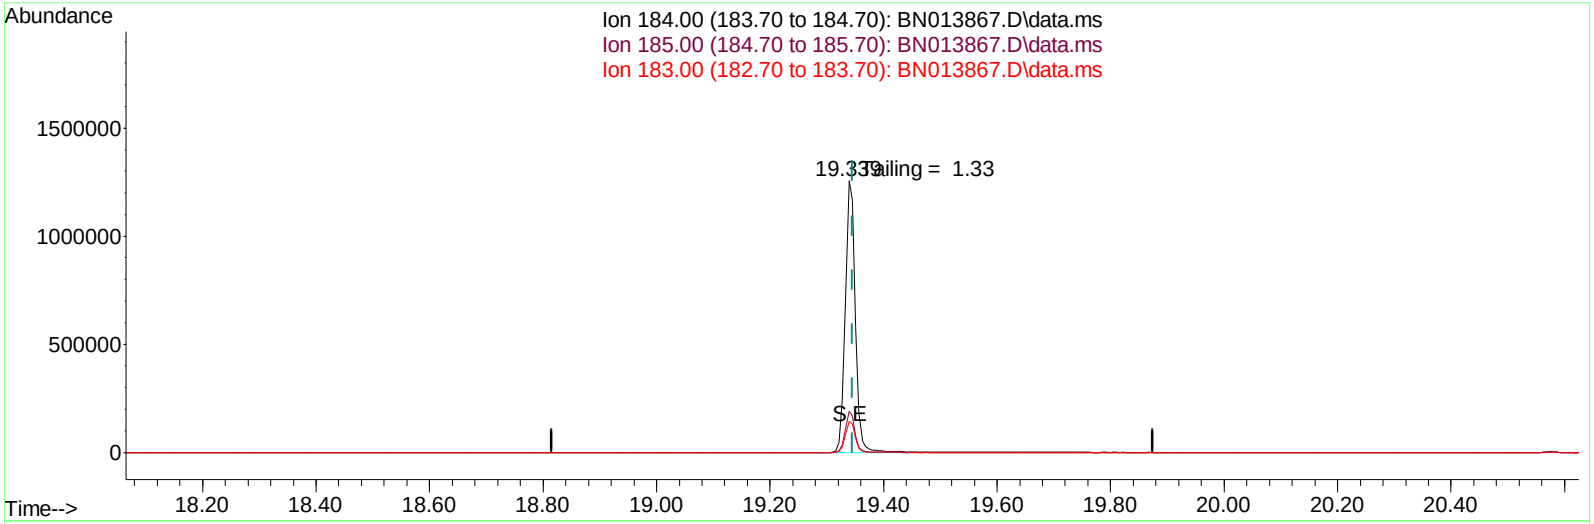

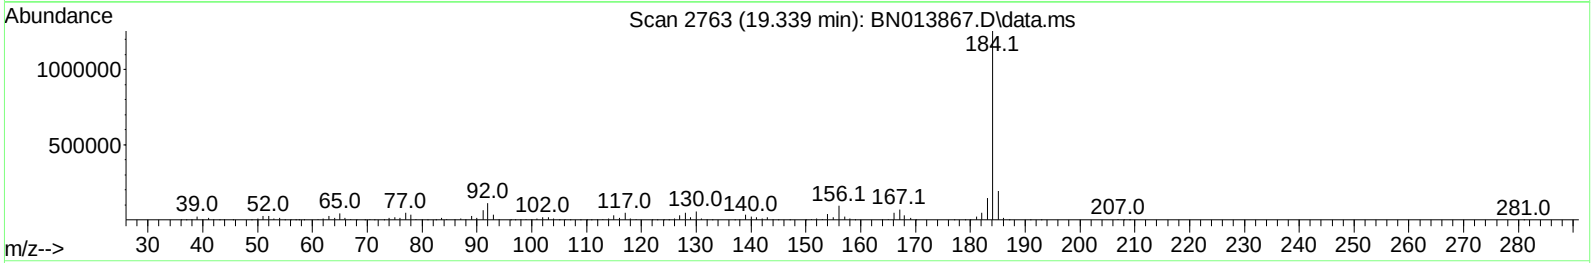

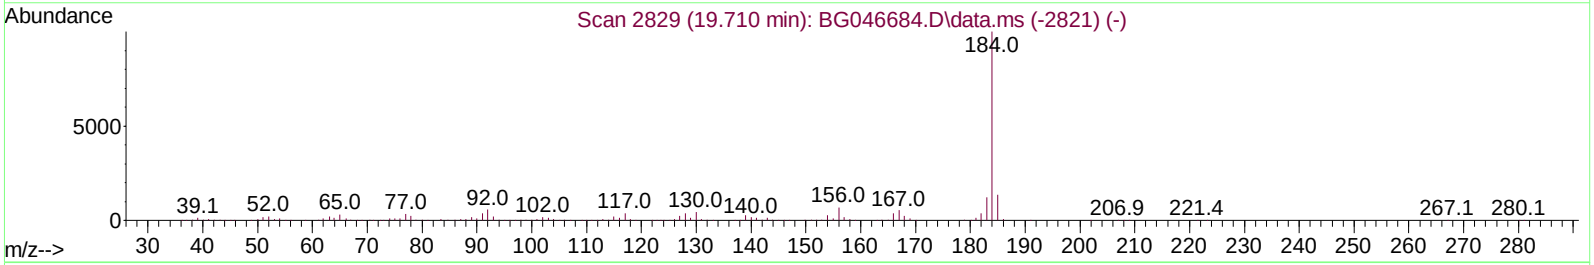

TIC: BN013867.D\data.ms

(77) Benzidine

19.339min (-0.006) 0.00 ng

response 1569237

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.21
183.00	13.20	11.45
0.00	0.00	0.00