




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018877.D
Acq On : 08 Mar 2022 18:56
Operator : CG/JU
Sample : N1775-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRX2

Manual IntegrationsAPPROVED

Quant Time: Mar 09 01:56:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 14:15:20 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/09/2022
Supervised By :Yogesh Patel 03/10/2022

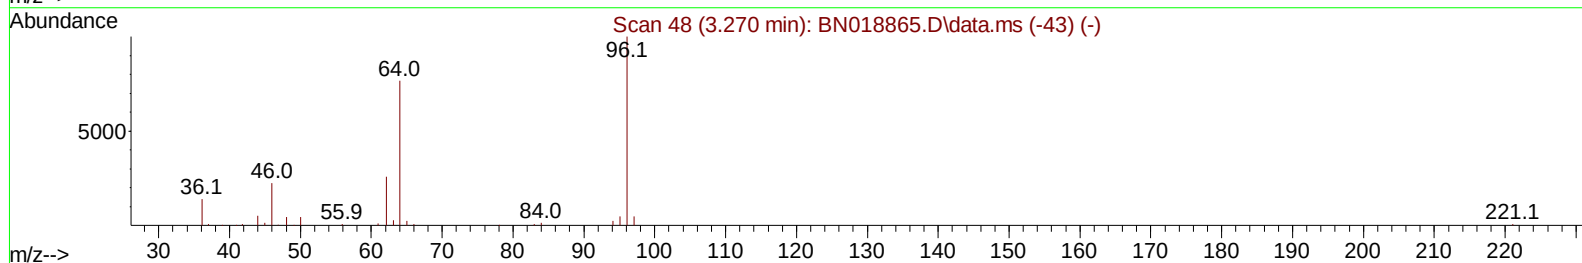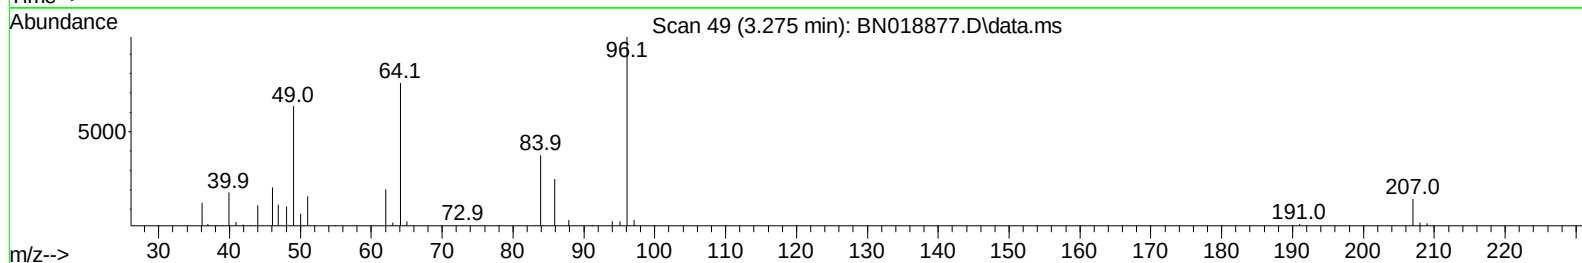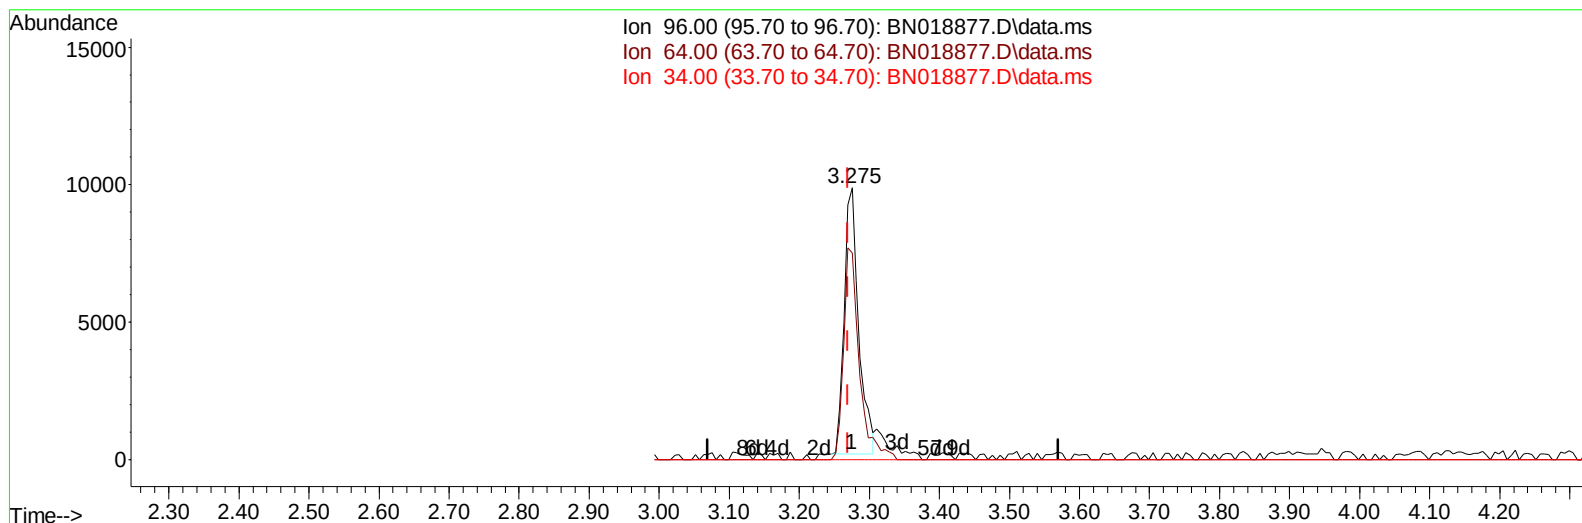

TIC: BN018877.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.275min (+ 0.005) 4.23 ng/uL

response 13907

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	76.11
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
 Data File : BN018877.D
 Acq On : 08 Mar 2022 18:56
 Operator : CG/JU
 Sample : N1775-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBRX2

Manual IntegrationsAPPROVED

Quant Time: Mar 09 01:56:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 14:15:20 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/09/2022
 Supervised By :Yogesh Patel 03/10/2022

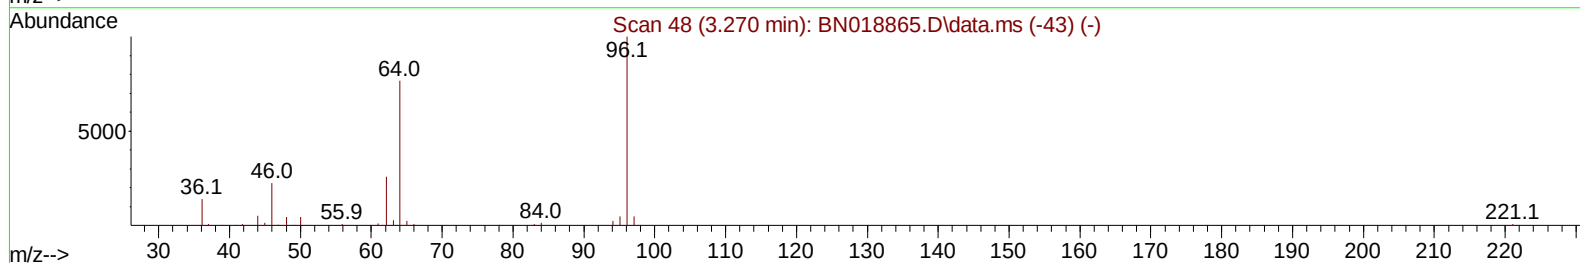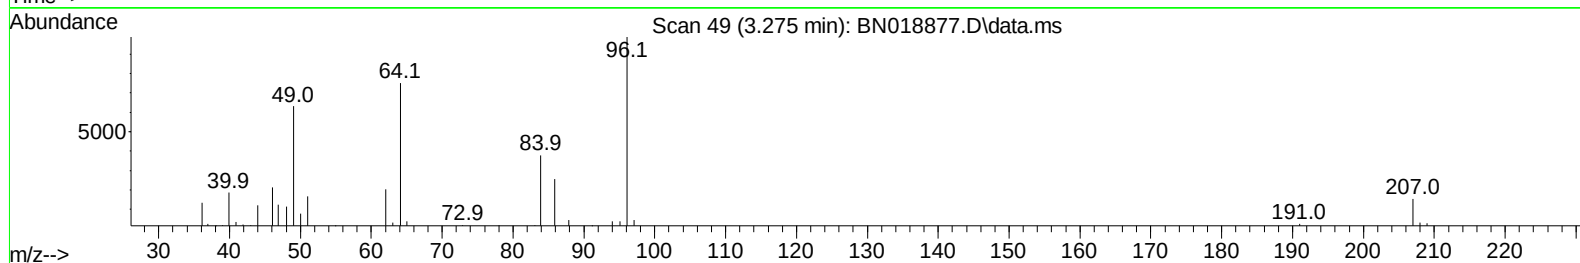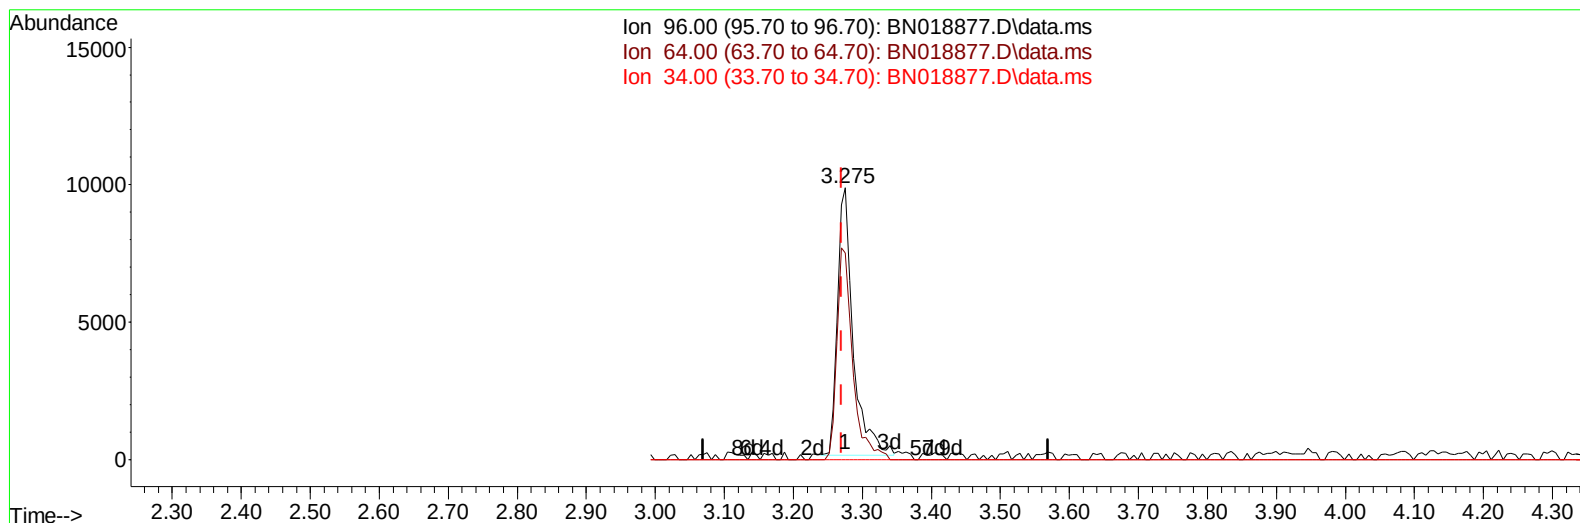

TIC: BN018877.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.275min (+ 0.005) 4.60 ng/uL m

response 15124

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	76.11
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
 Data File : BN018877.D
 Acq On : 08 Mar 2022 18:56
 Operator : CG/JU
 Sample : N1775-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBRX2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/09/2022
 Supervised By :Yogesh Patel 03/10/2022

Quant Time: Mar 09 01:56:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 14:15:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	131558	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	600032	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	423745	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	942539	20.000	ng/ul	0.00
79) Chrysene-d12	21.457	240	1066307	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	1172849	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	15124m	4.598	ng/uL	0.00
4) Pyridine-d5	3.699	84	71047	7.059	ng/ul	0.00
7) Phenol-d5	7.057	99	81563	6.350	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	253287	32.740	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	222619	24.186	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	157315	15.063	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	152382	33.062	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	71020	14.025	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	254745	26.299	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	396176	27.162	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1161119	36.191	ng/ul	0.00
49) Acenaphthylene-d8	14.233	160	1380159	34.560	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	11945	1.838	ng/ul	0.00
60) Fluorene-d10	15.528	176	1023876	36.715	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	7223	1.237	ng/ul	0.00
73) Anthracene-d10	17.375	188	1776799	39.413	ng/ul	0.00
81) Pyrene-d10	19.669	212	2152979	37.310	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	2426596	39.698	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018877.D
Acq On : 08 Mar 2022 18:56
Operator : CG/JU
Sample : N1775-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRX2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/09/2022
Supervised By :Yogesh Patel 03/10/2022

Quant Time: Mar 09 01:56:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 14:15:20 2022
Response via : Initial Calibration

