

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
 Data File : BN018870.D
 Acq On : 08 Mar 2022 14:40
 Operator : CG/JU
 Sample : PB143136BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	56	rVB	34724	53725	0.94%	0.106%
2	3.693	116	120	147	rBV	499839	838797	14.64%	1.654%
3	4.046	176	180	185	rVB	11422	15384	0.27%	0.030%
4	7.058	686	692	703	rBV	673160	1053034	18.38%	2.076%
5	7.228	713	721	732	rBV	526526	831028	14.51%	1.639%
6	7.434	749	756	766	rBV	655663	1033874	18.05%	2.039%
7	7.905	830	836	844	rBV	591012	952249	16.62%	1.878%
8	8.610	949	956	964	rBV	818392	1331043	23.24%	2.625%
9	9.063	1026	1033	1044	rBV	666605	1062620	18.55%	2.095%
10	9.793	1149	1157	1168	rBV	538072	898821	15.69%	1.772%
11	10.328	1241	1248	1259	rBV	838686	1364919	23.83%	2.691%
12	10.716	1306	1314	1322	rBV	914362	1517584	26.49%	2.992%
13	10.840	1328	1335	1345	rBV	900198	1501625	26.21%	2.961%
14	12.304	1578	1584	1590	rBV2	13679	22101	0.39%	0.044%
15	13.945	1856	1863	1875	rBV	1718355	2299856	40.15%	4.535%
16	14.234	1905	1912	1924	rBV	1843572	2659641	46.43%	5.244%
17	14.539	1957	1964	1973	rBV	1499771	2246260	39.21%	4.429%
18	14.716	1987	1994	2010	rBV	837208	1219087	21.28%	2.404%
19	15.345	2098	2101	2106	rBV4	6146	8692	0.15%	0.017%
20	15.528	2126	2132	2145	rBV	2328019	3387279	59.13%	6.679%
21	15.639	2145	2151	2163	rBV	850010	1125211	19.64%	2.219%
22	15.769	2168	2173	2179	rVB2	13305	17522	0.31%	0.035%
23	17.063	2386	2393	2398	rBV3	8261	17814	0.31%	0.035%
24	17.280	2423	2430	2439	rBV	1980961	2795390	48.80%	5.512%
25	17.375	2439	2446	2461	rVV2	2632748	3846580	67.15%	7.585%
26	17.651	2488	2493	2496	rBV5	3535	5889	0.10%	0.012%
27	18.245	2590	2594	2598	rVB3	4749	6144	0.11%	0.012%
28	19.233	2757	2762	2766	rBV2	34769	46769	0.82%	0.092%
29	19.304	2769	2774	2778	rBV	33376	46329	0.81%	0.091%
30	19.669	2829	2836	2847	rBV	3491656	4795588	83.72%	9.456%
31	19.969	2884	2887	2891	rBV5	3488	7127	0.12%	0.014%
32	20.663	3002	3005	3011	rVB2	28627	31066	0.54%	0.061%
33	21.457	3134	3140	3152	rBV	2710561	3558564	62.12%	7.017%
34	22.563	3326	3328	3333	rVB2	33469	38911	0.68%	0.077%
35	23.115	3418	3422	3428	rBV2	60099	93275	1.63%	0.184%
36	23.692	3512	3520	3528	rBV	2816920	5728403	100.00%	11.296%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018870.D
Acq On : 08 Mar 2022 14:40
Operator : CG/JU
Sample : PB143136BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK136

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Title : SVOA CALIBRATION

37	23.851	3539	3547	3559	rVB2	1890925	3896192	68.02%	7.683%
38	24.462	3647	3651	3658	rVB2	64281	122867	2.14%	0.242%
39	26.292	3957	3962	3974	rVB7	74271	235734	4.12%	0.465%


Sum of corrected areas: 50712994

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018870.D
Acq On : 08 Mar 2022 14:40
Operator : CG/JU
Sample : PB143136BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

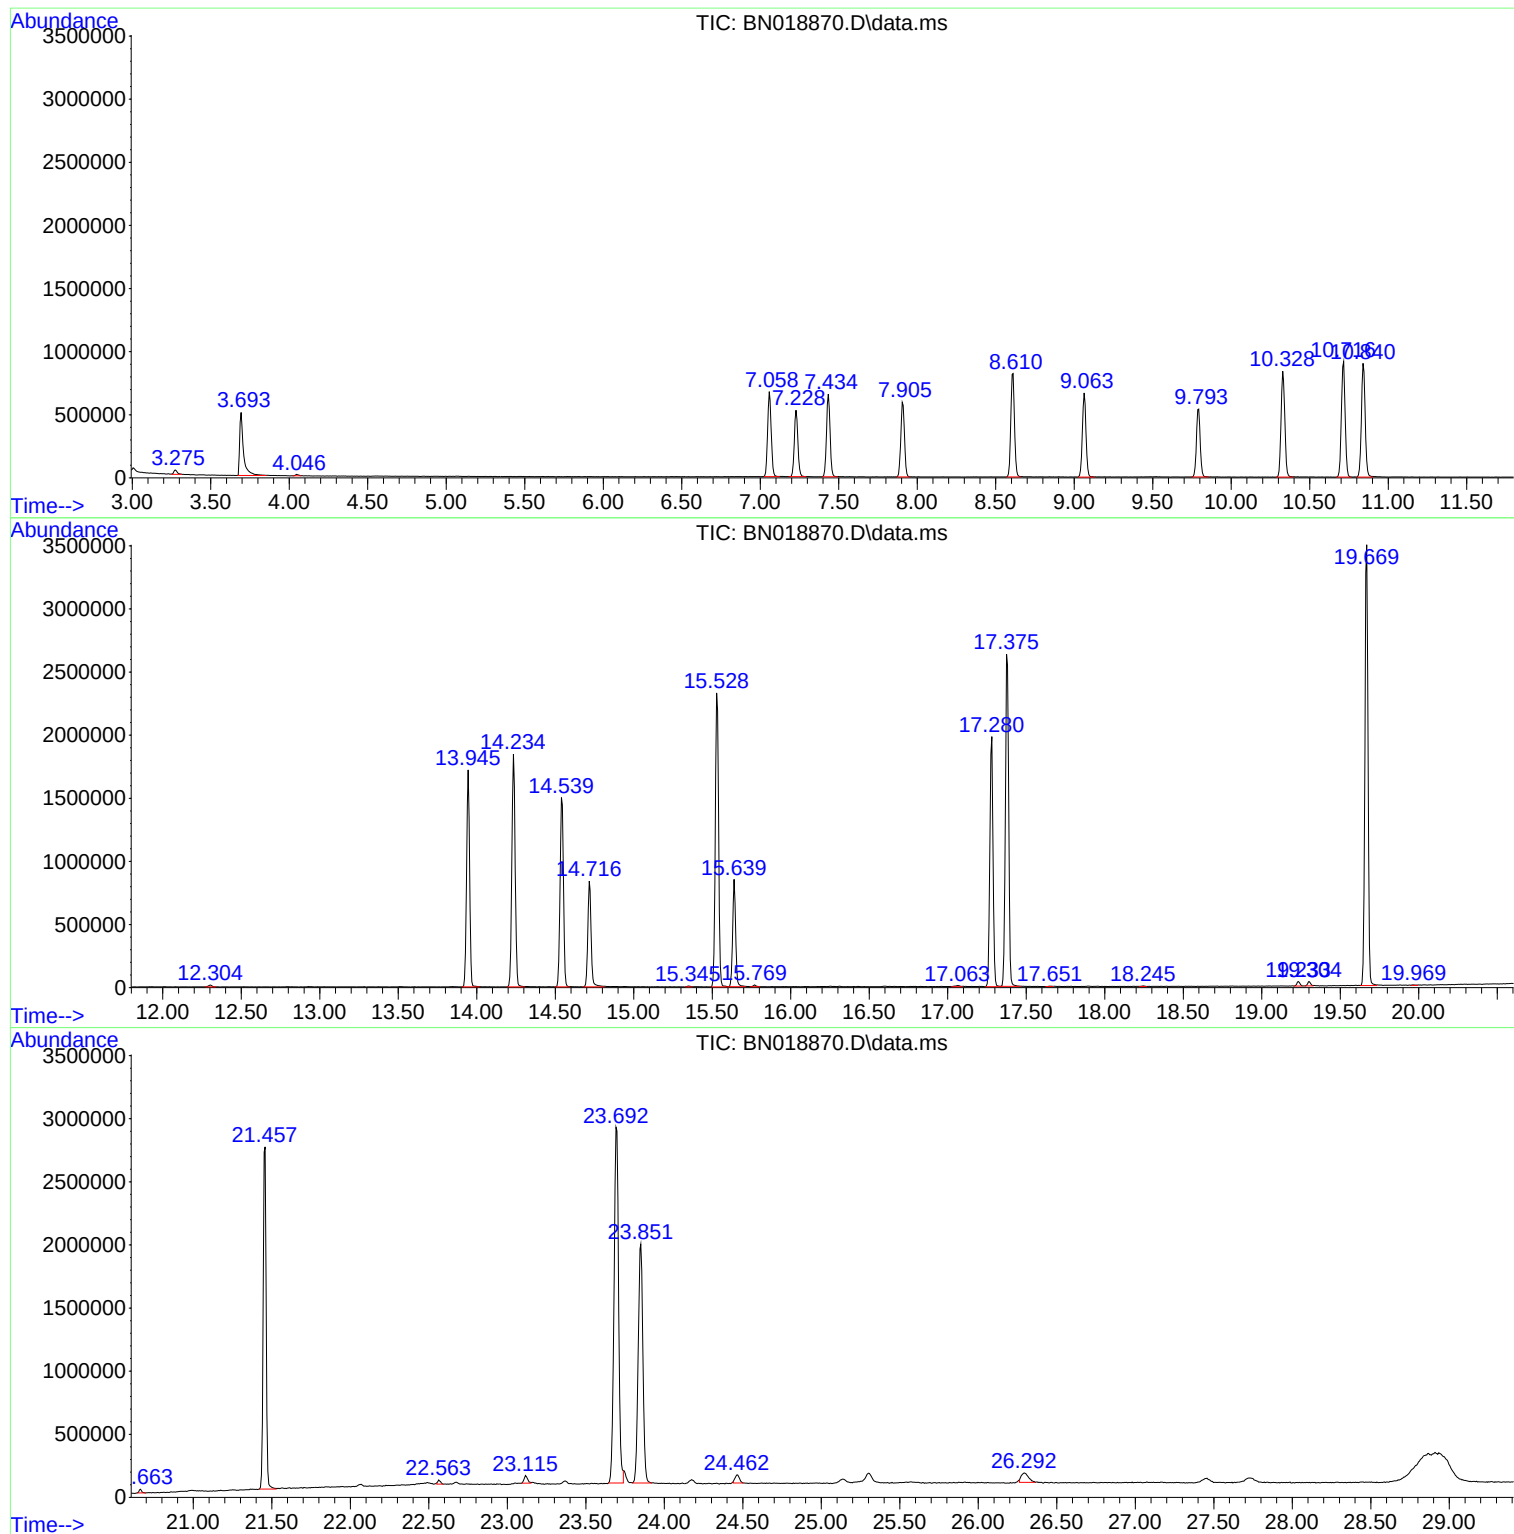

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018870.D
Acq On : 08 Mar 2022 14:40
Operator : CG/JU
Sample : PB143136BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018870.D
Acq On : 08 Mar 2022 14:40
Operator : CG/JU
Sample : PB143136BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc