

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
 Data File : BN018874.D
 Acq On : 08 Mar 2022 17:06
 Operator : CG/JU
 Sample : N1733-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBRU0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	44	48	58	rVB	25682	38113	0.61%	0.089%
2	3.699	118	121	135	rBV	67784	129932	2.08%	0.304%
3	4.046	176	180	187	rVB2	6720	10352	0.17%	0.024%
4	4.981	331	339	345	rBV4	9088	15619	0.25%	0.037%
5	7.058	686	692	702	rVB	147274	234813	3.76%	0.550%
6	7.228	715	721	731	rBV	481198	757158	12.11%	1.773%
7	7.434	750	756	769	rBV	475219	744955	11.91%	1.744%
8	7.905	829	836	844	rBV	425623	676637	10.82%	1.584%
9	8.605	945	955	964	rBV	412132	662846	10.60%	1.552%
10	9.063	1025	1033	1048	rBV	587946	933197	14.92%	2.185%
11	9.516	1104	1110	1119	rVB	14037	24008	0.38%	0.056%
12	9.793	1149	1157	1165	rBV	457155	746948	11.95%	1.749%
13	10.328	1241	1248	1260	rBV	711200	1144708	18.31%	2.680%
14	10.716	1306	1314	1321	rBV	647019	1087302	17.39%	2.546%
15	10.840	1328	1335	1347	rBV	650468	1077518	17.23%	2.523%
16	11.540	1449	1454	1461	rBV4	3196	7254	0.12%	0.017%
17	12.146	1553	1557	1563	rVB4	5263	7551	0.12%	0.018%
18	12.299	1578	1583	1589	rVB	13367	20360	0.33%	0.048%
19	13.381	1761	1767	1773	rBV2	17425	27156	0.43%	0.064%
20	13.946	1856	1863	1869	rBV	1583832	2102510	33.62%	4.923%
21	14.234	1901	1912	1924	rBV	1782882	2499933	39.98%	5.854%
22	14.445	1943	1948	1952	rVB4	8722	11226	0.18%	0.026%
23	14.540	1956	1964	1972	rBV	1088010	1586739	25.38%	3.715%
24	14.716	1987	1994	2007	rBV	153169	235229	3.76%	0.551%
25	15.275	2084	2089	2093	rVB	5504	7918	0.13%	0.019%
26	15.345	2093	2101	2105	rVV2	15728	25795	0.41%	0.060%
27	15.392	2105	2109	2115	rVB5	5935	9338	0.15%	0.022%
28	15.528	2126	2132	2144	rBV	2292054	3289384	52.61%	7.702%
29	15.640	2144	2151	2164	rVV	799408	1047386	16.75%	2.453%
30	15.769	2169	2173	2177	rVB2	10809	15887	0.25%	0.037%
31	16.251	2252	2255	2260	rBV4	5786	10117	0.16%	0.024%
32	16.604	2307	2315	2316	rBV7	4295	7232	0.12%	0.017%
33	17.045	2386	2390	2392	rBV3	7658	11706	0.19%	0.027%
34	17.281	2423	2430	2439	rBV	1403515	2012471	32.18%	4.712%
35	17.375	2439	2446	2460	rVV	2835707	4114801	65.81%	9.635%
36	17.657	2489	2494	2497	rBV6	3251	6347	0.10%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
 Data File : BN018874.D
 Acq On : 08 Mar 2022 17:06
 Operator : CG/JU
 Sample : N1733-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBRU0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

37	17.898	2532	2535	2540	rVB6	3765	6347	0.10%	0.015%
38	17.951	2540	2544	2548	rBV6	6022	9739	0.16%	0.023%
39	18.175	2577	2582	2590	rBV2	25135	43193	0.69%	0.101%
40	18.245	2590	2594	2601	rVB	9025	13777	0.22%	0.032%
41	18.604	2651	2655	2658	rBV3	14992	17559	0.28%	0.041%
42	19.033	2722	2728	2732	rBV8	4231	7879	0.13%	0.018%
43	19.233	2757	2762	2768	rBV2	34486	49362	0.79%	0.116%
44	19.304	2769	2774	2777	rBV	33681	45656	0.73%	0.107%
45	19.451	2795	2799	2804	rBV6	5202	8024	0.13%	0.019%
46	19.604	2820	2825	2829	rBV5	5300	8033	0.13%	0.019%
47	19.669	2829	2836	2848	rVV	3764486	5080450	81.25%	11.896%
48	19.892	2870	2874	2877	rBV3	6791	10051	0.16%	0.024%
49	20.186	2920	2924	2928	rBV6	4557	8792	0.14%	0.021%
50	20.663	3002	3005	3008	rBV3	17953	17199	0.28%	0.040%
51	21.163	3085	3090	3095	rBV2	177095	229820	3.68%	0.538%
52	21.457	3134	3140	3148	rBV	1938451	2530034	40.46%	5.924%
53	23.122	3419	3423	3428	rVB	59735	85333	1.36%	0.200%
54	23.698	3513	3521	3536	rVB2	3031634	6252849	100.00%	14.641%
55	23.851	3539	3547	3558	rVB2	1414403	2817929	45.07%	6.598%
56	24.468	3647	3652	3657	rVB2	65594	124380	1.99%	0.291%




Sum of corrected areas: 42706852

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018874.D
Acq On : 08 Mar 2022 17:06
Operator : CG/JU
Sample : N1733-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRU0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

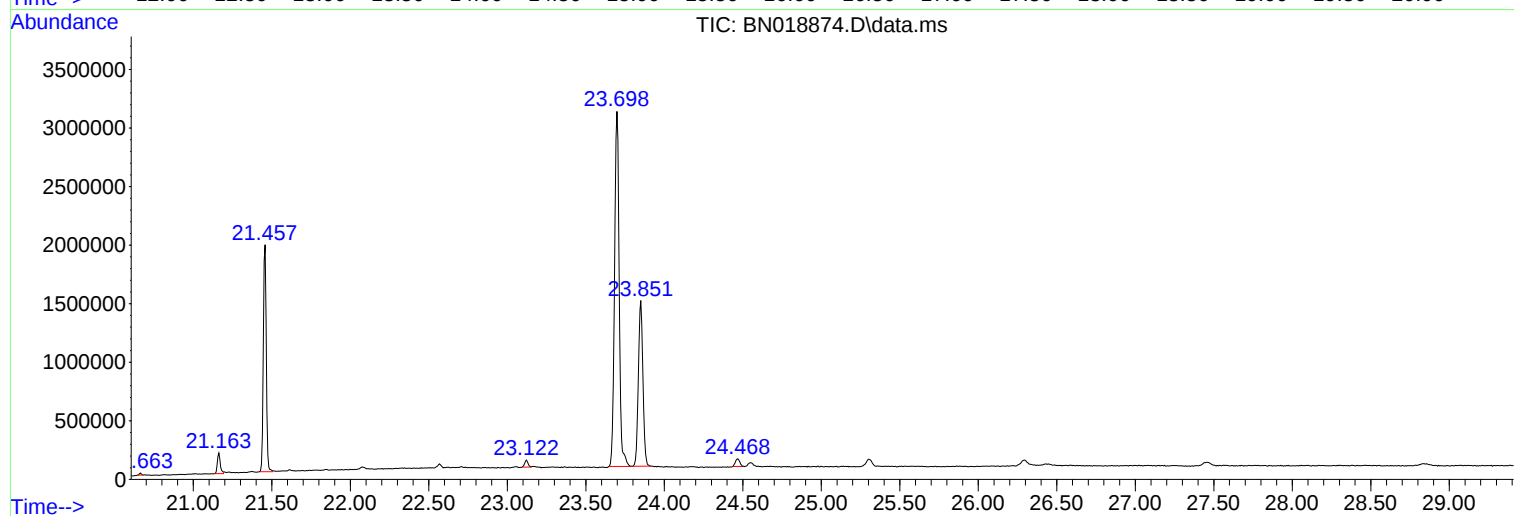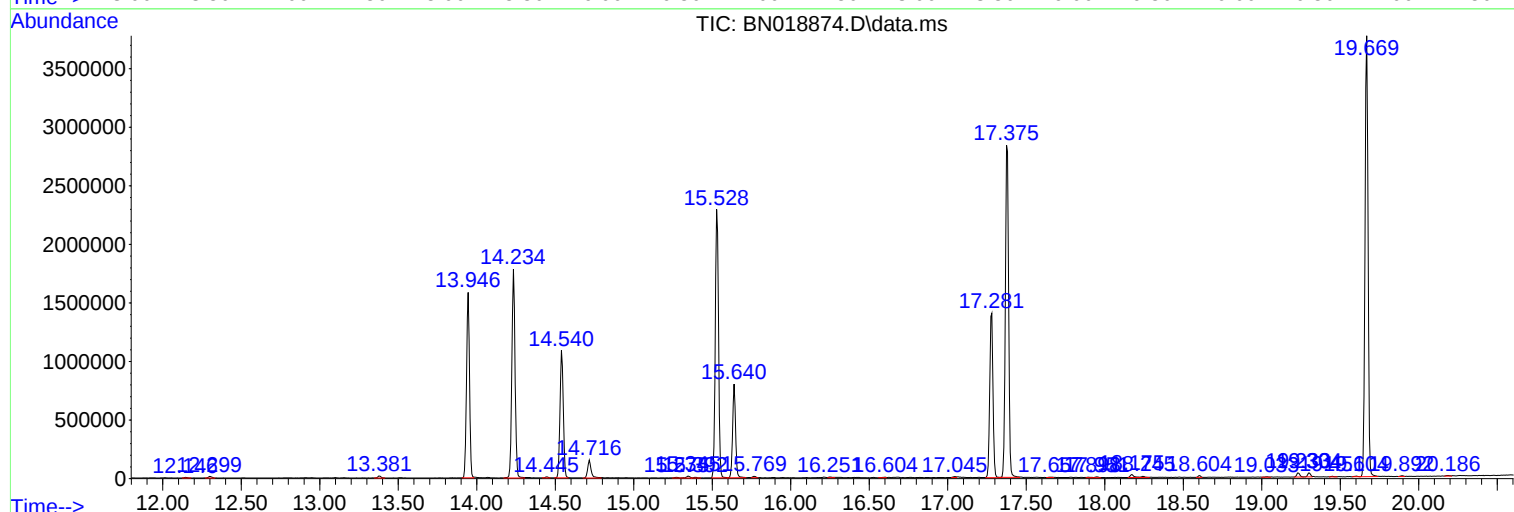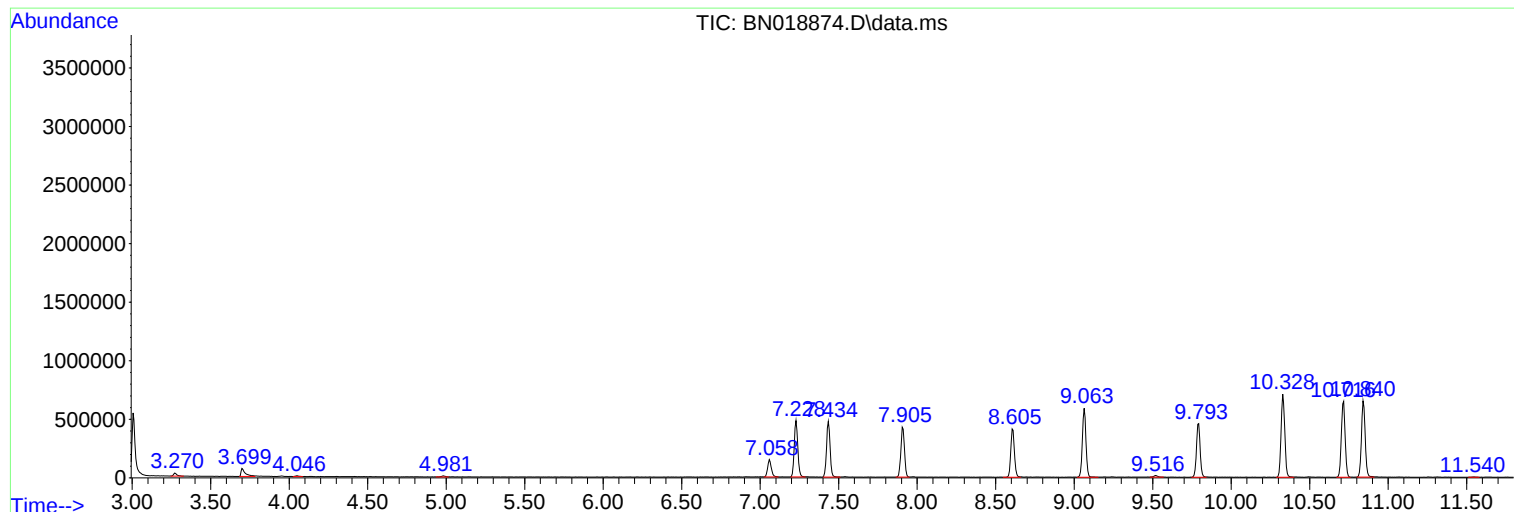

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018874.D
Acq On : 08 Mar 2022 17:06
Operator : CG/JU
Sample : N1733-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRU0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018874.D
Acq On : 08 Mar 2022 17:06
Operator : CG/JU
Sample : N1733-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRU0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc