

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
 Data File : BN018876.D
 Acq On : 08 Mar 2022 18:19
 Operator : CG/JU
 Sample : N1733-27
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBRU5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	44	48	60	rVB	32844	54228	0.73%	0.095%
2	3.552	93	96	103	rBV	11993	18148	0.24%	0.032%
3	3.693	116	120	141	rBV	408557	712520	9.59%	1.254%
4	4.046	176	180	188	rVB3	7035	12074	0.16%	0.021%
5	4.981	335	339	345	rBV4	7109	11988	0.16%	0.021%
6	7.058	685	692	704	rBV	728806	1161978	15.65%	2.044%
7	7.228	713	721	730	rBV	581412	911428	12.27%	1.604%
8	7.293	730	732	739	rVB	8431	12535	0.17%	0.022%
9	7.434	749	756	768	rVB	682411	1063730	14.32%	1.872%
10	7.905	829	836	844	rBV	434535	694746	9.35%	1.222%
11	7.969	844	847	852	rVB2	8660	11605	0.16%	0.020%
12	8.610	947	956	966	rBV	962716	1555043	20.94%	2.736%
13	9.063	1026	1033	1043	rBV	762744	1214227	16.35%	2.136%
14	9.234	1058	1062	1067	rBV5	7285	10889	0.15%	0.019%
15	9.522	1105	1111	1118	rVB	35070	53760	0.72%	0.095%
16	9.793	1147	1157	1173	rBV	609007	1013146	13.64%	1.783%
17	10.328	1241	1248	1258	rBV	996101	1618711	21.80%	2.848%
18	10.493	1270	1276	1280	rBV4	7331	13690	0.18%	0.024%
19	10.716	1306	1314	1321	rBV	662521	1124277	15.14%	1.978%
20	10.840	1326	1335	1354	rBV	1075202	1801791	24.26%	3.170%
21	11.640	1468	1471	1480	rBV6	3383	7468	0.10%	0.013%
22	11.746	1484	1489	1496	rVB6	4725	8456	0.11%	0.015%
23	12.146	1550	1557	1563	rBV	28093	41652	0.56%	0.073%
24	12.299	1578	1583	1589	rVB2	19268	30949	0.42%	0.054%
25	12.951	1690	1694	1698	rVB4	7746	11439	0.15%	0.020%
26	13.040	1704	1709	1714	rVV6	5805	9842	0.13%	0.017%
27	13.093	1714	1718	1724	rVB4	9482	15625	0.21%	0.027%
28	13.381	1762	1767	1775	rVB2	60655	83383	1.12%	0.147%
29	13.946	1851	1863	1869	rBV	2137722	2916567	39.27%	5.132%
30	14.069	1881	1884	1890	rVB5	5828	9818	0.13%	0.017%
31	14.234	1900	1912	1923	rBV	2398300	3475688	46.80%	6.115%
32	14.445	1944	1948	1953	rVB	25998	32018	0.43%	0.056%
33	14.540	1957	1964	1974	rBV	1146451	1667753	22.46%	2.934%
34	14.716	1987	1994	2005	rBV	1102007	1544774	20.80%	2.718%
35	14.945	2029	2033	2041	rBV8	9635	13694	0.18%	0.024%
36	15.345	2094	2101	2105	rBV7	6793	13082	0.18%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
 Data File : BN018876.D
 Acq On : 08 Mar 2022 18:19
 Operator : CG/JU
 Sample : N1733-27
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBRU5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

37	15.392	2105	2109	2115	rVB2	17676	22232	0.30%	0.039%
38	15.528	2125	2132	2145	rVB	3035166	4493926	60.51%	7.907%
39	15.640	2145	2151	2164	rBV	1049801	1373462	18.49%	2.417%
40	15.769	2168	2173	2177	rBV3	17372	25500	0.34%	0.045%
41	15.945	2199	2203	2210	rVV8	6475	11947	0.16%	0.021%
42	16.169	2236	2241	2244	rBV7	5258	8757	0.12%	0.015%
43	16.210	2244	2248	2251	rVV6	7908	12559	0.17%	0.022%
44	16.251	2251	2255	2258	rVV2	14532	21363	0.29%	0.038%
45	16.322	2262	2267	2270	rVB7	6223	10384	0.14%	0.018%
46	16.428	2279	2285	2289	rVB7	5707	8694	0.12%	0.015%
47	16.522	2297	2301	2305	rVB3	7105	9516	0.13%	0.017%
48	16.681	2325	2328	2332	rVB4	9746	12011	0.16%	0.021%
49	17.045	2384	2390	2396	rBV6	9595	24870	0.33%	0.044%
50	17.281	2423	2430	2439	rVV	1464861	2103470	28.32%	3.701%
51	17.381	2439	2447	2458	rVV2	3407759	5073031	68.31%	8.926%
52	17.469	2458	2462	2466	rVB5	20305	29087	0.39%	0.051%
53	17.651	2489	2493	2499	rBV6	7165	14477	0.19%	0.025%
54	17.951	2541	2544	2548	rVB5	7235	10032	0.14%	0.018%
55	18.169	2577	2581	2588	rBV2	54089	85350	1.15%	0.150%
56	18.245	2592	2594	2600	rVB3	6074	8328	0.11%	0.015%
57	18.604	2651	2655	2661	rVB2	27912	35811	0.48%	0.063%
58	19.033	2725	2728	2731	rBV5	6508	8648	0.12%	0.015%
59	19.233	2757	2762	2766	rBV	53346	69407	0.93%	0.122%
60	19.304	2770	2774	2778	rBV	47820	67730	0.91%	0.119%
61	19.451	2794	2799	2802	rBV5	13602	20129	0.27%	0.035%
62	19.598	2821	2824	2829	rVB6	5845	8014	0.11%	0.014%
63	19.669	2829	2836	2849	rBV2	4750512	6248432	84.13%	10.994%
64	20.180	2919	2923	2927	rBV6	8504	14121	0.19%	0.025%
65	20.663	3002	3005	3008	rBV2	19705	19384	0.26%	0.034%
66	21.163	3086	3090	3099	rBV	298422	383501	5.16%	0.675%
67	21.457	3134	3140	3149	rBV	2164279	2652364	35.71%	4.667%
68	22.563	3324	3328	3334	rVB5	53705	86602	1.17%	0.152%
69	23.121	3419	3423	3429	rBV2	61424	91172	1.23%	0.160%
70	23.698	3512	3521	3537	rBV2	3512967	7426679	100.00%	13.067%
71	23.851	3539	3547	3562	rVB	1455837	2904608	39.11%	5.111%
72	24.468	3647	3652	3658	rVB	78050	156231	2.10%	0.275%
73	24.551	3661	3666	3674	rVB4	59804	129306	1.74%	0.228%
74	25.304	3789	3794	3809	rVB3	77681	200820	2.70%	0.353%

Sum of corrected areas: 56834677

Instrument :

BNA_N

ClientSampleId :




DBRU5

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018876.D
Acq On : 08 Mar 2022 18:19
Operator : CG/JU
Sample : N1733-27
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRU5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

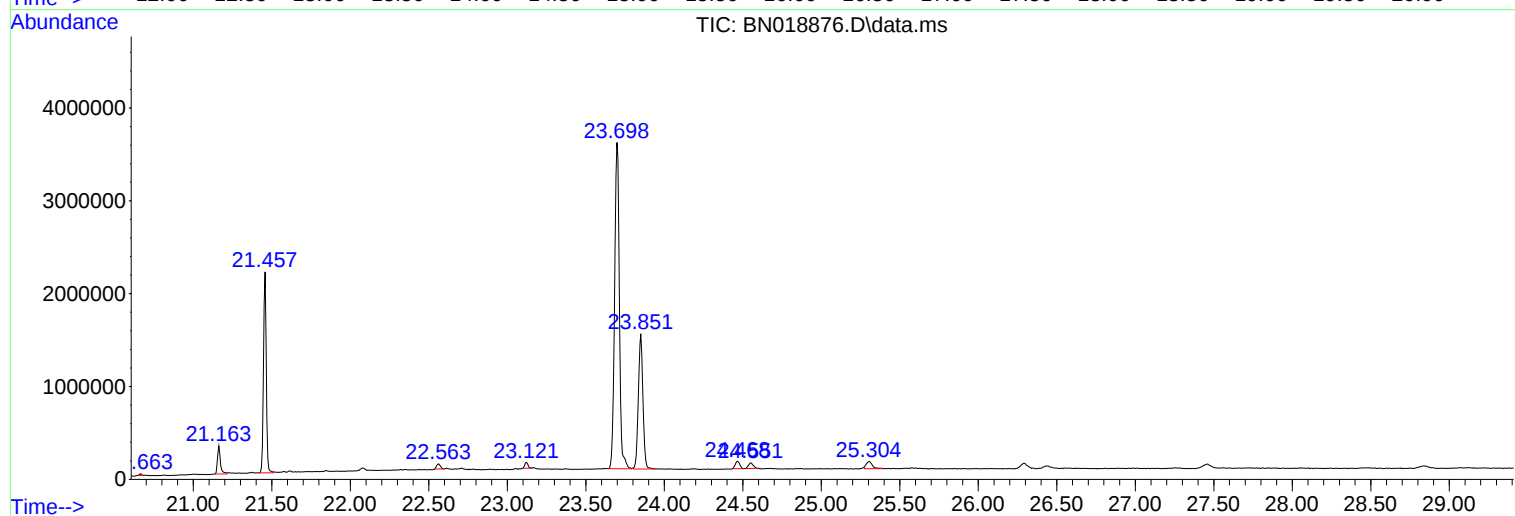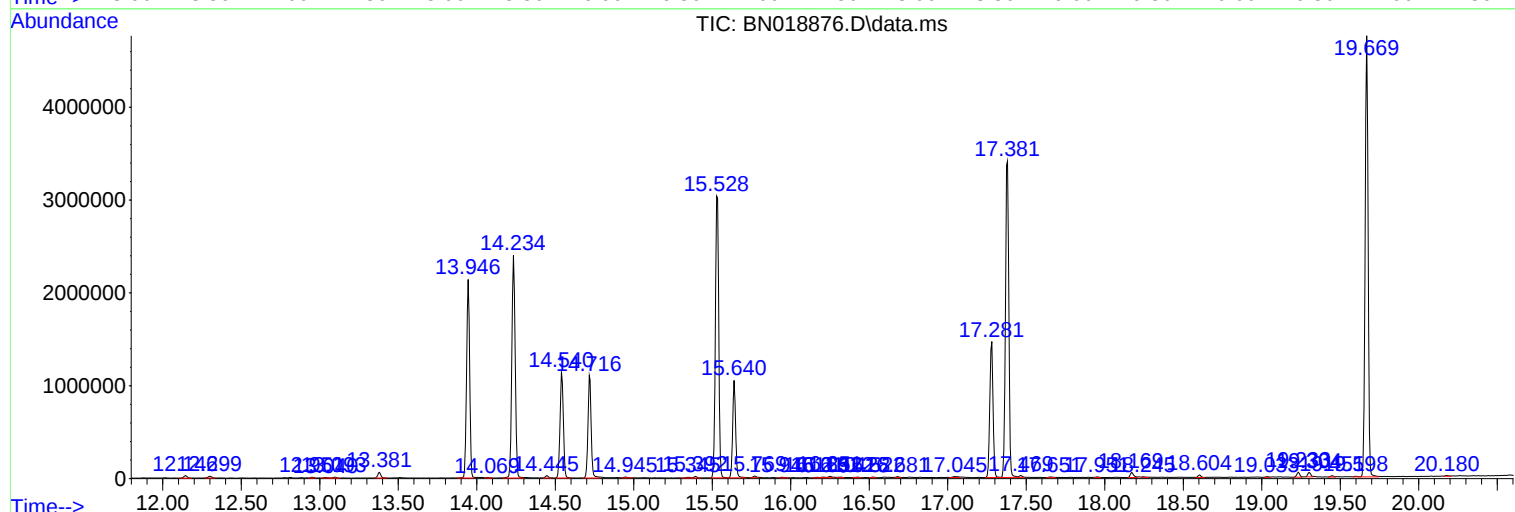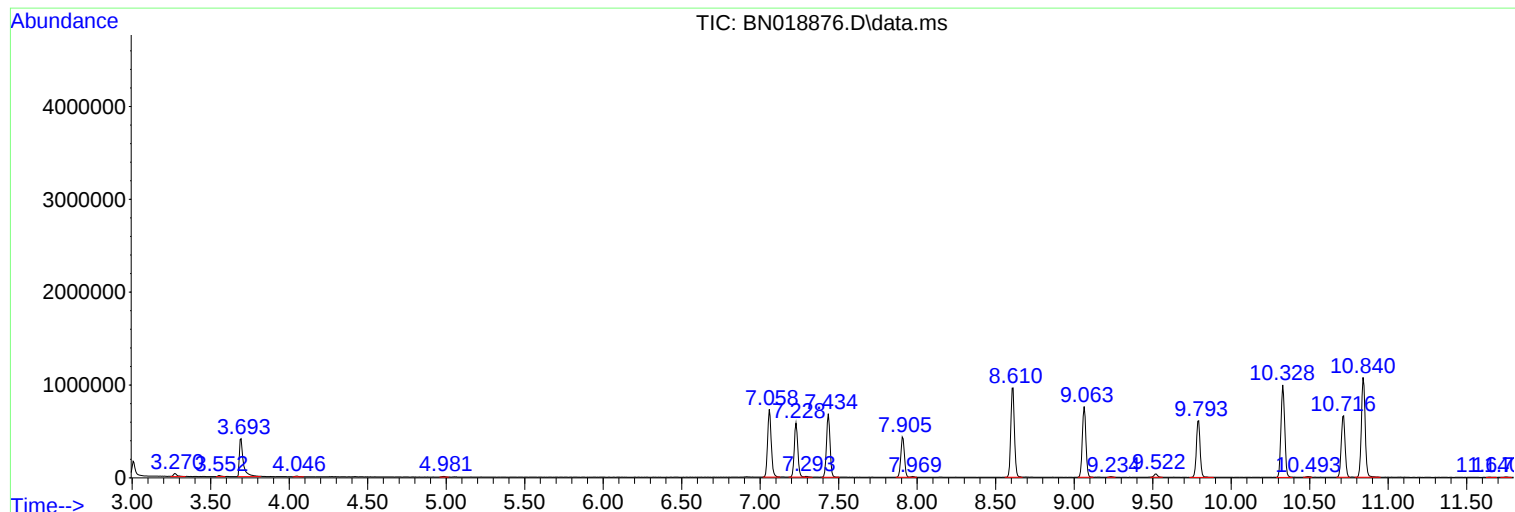

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018876.D
Acq On : 08 Mar 2022 18:19
Operator : CG/JU
Sample : N1733-27
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRU5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trifluoroacetoxy hexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.163	2.89 ng/ul	383501	Chrysene-d12	21.457

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
2			1-Tetracosene	336	C24H48	010192-32-2	94
3			1-Heneicosanol	312	C21H44O	015594-90-8	93
4			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	93
5			1-Hexacosene	364	C26H52	018835-33-1	91

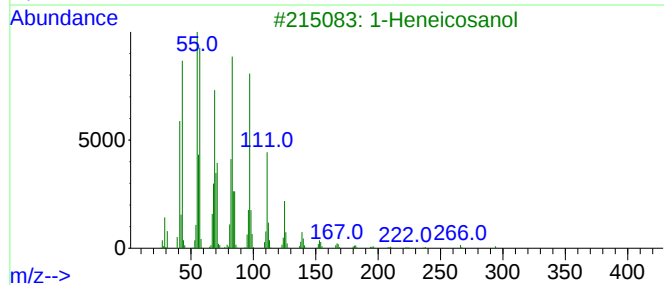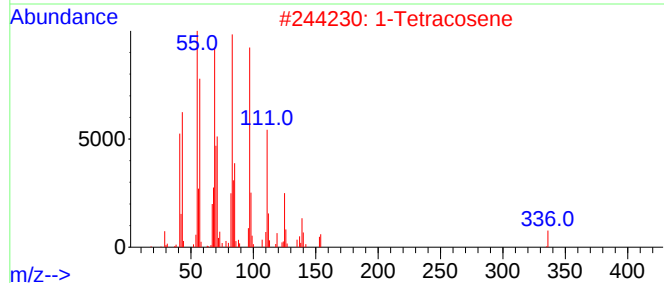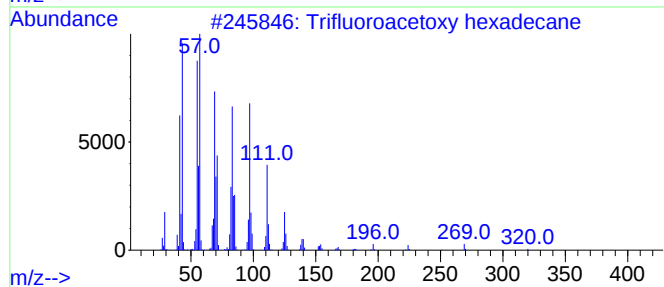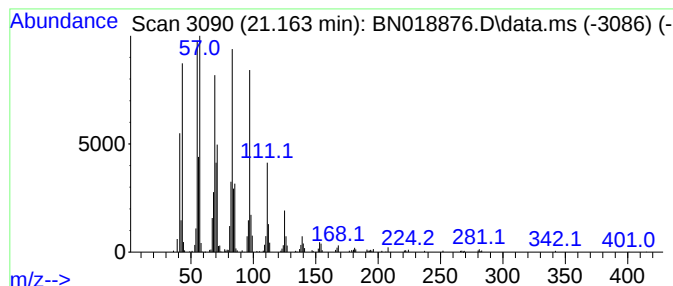

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030822\
Data File : BN018876.D
Acq On : 08 Mar 2022 18:19
Operator : CG/JU
Sample : N1733-27
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBRU5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trifluoroacetox...	21.163	2.9	ng/ul	383501	5	21.457	2652360	20.0