
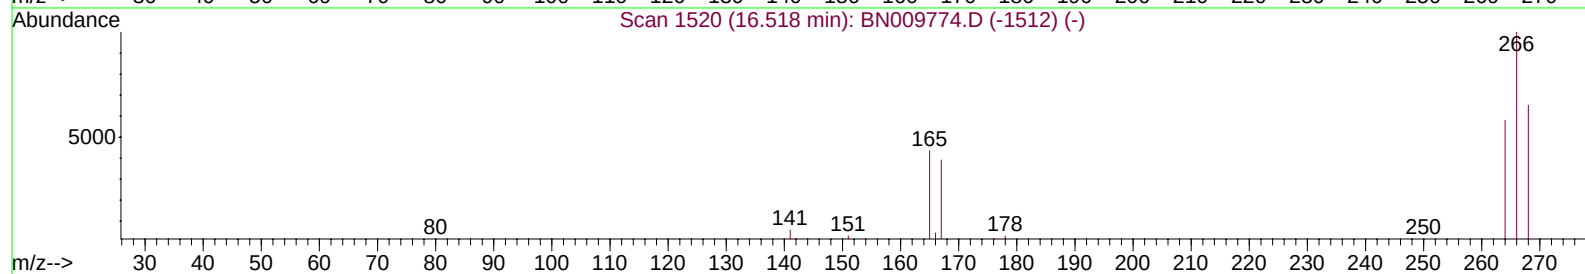
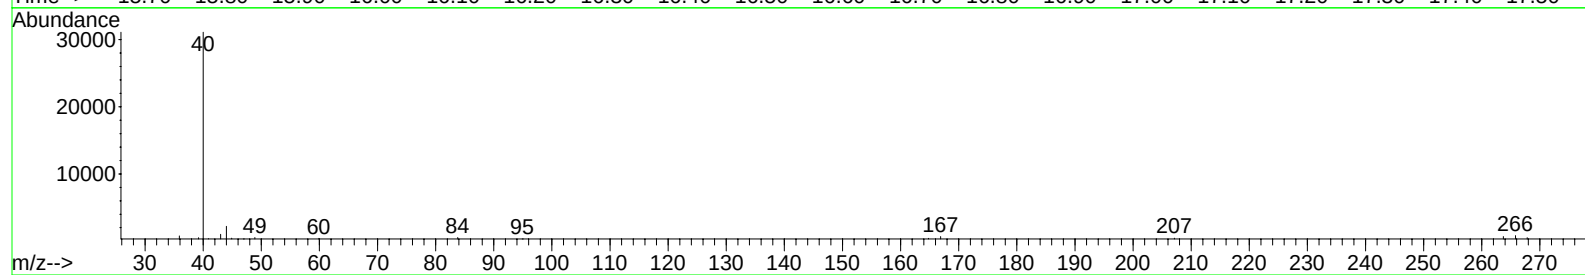


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN031020\
 Data File : BN010158.D
 Acq On : 10 Mar 2020 12:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 19:09:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 19 15:57:43 2020
 Response via : Initial Calibration

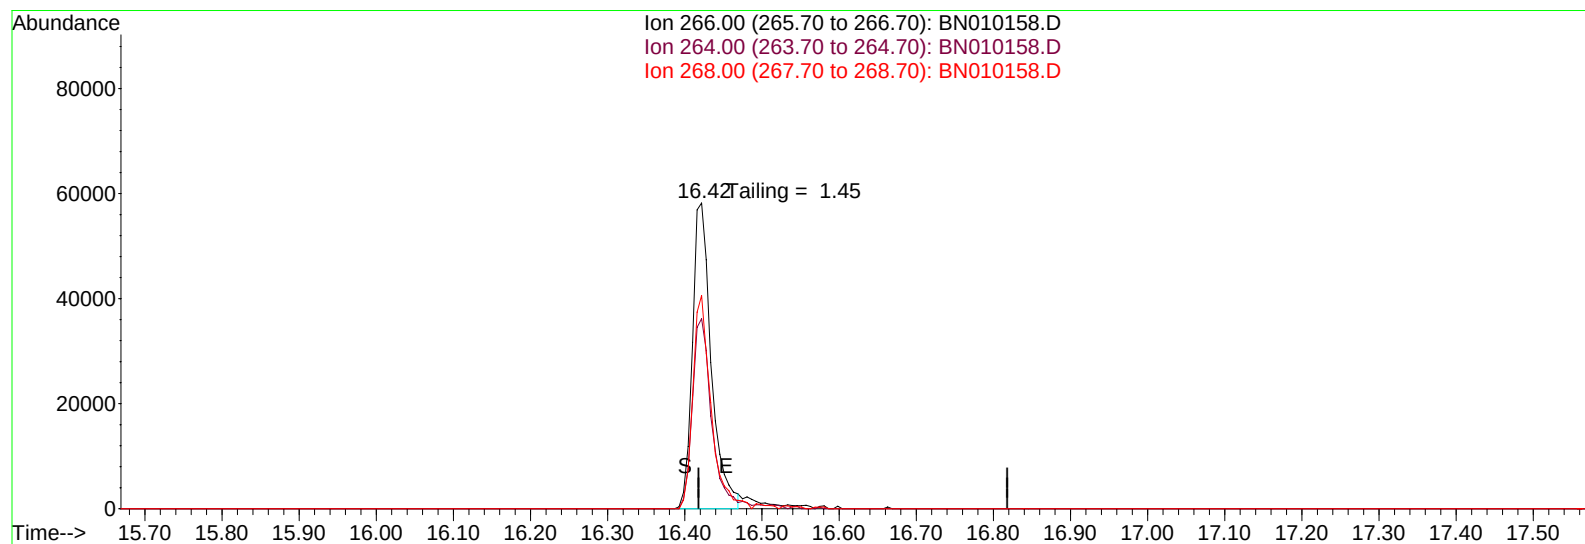

TIC: BN010158.D

(22) Pentachlorophenol

16.518min (-16.518) 0.00ng

response 0

Ion	Exp%	Act%
266.00	100	0.00
264.00	72.60	0.00#
268.00	82.10	0.00#
0.00	0.00	0.00