
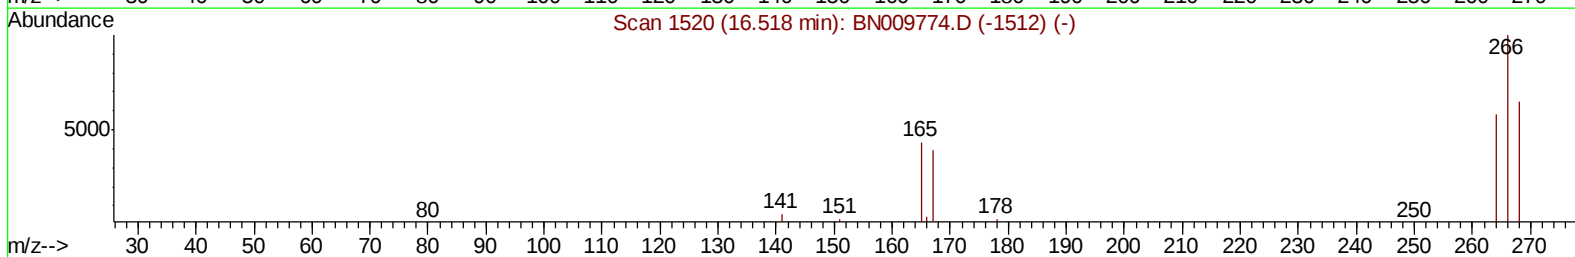
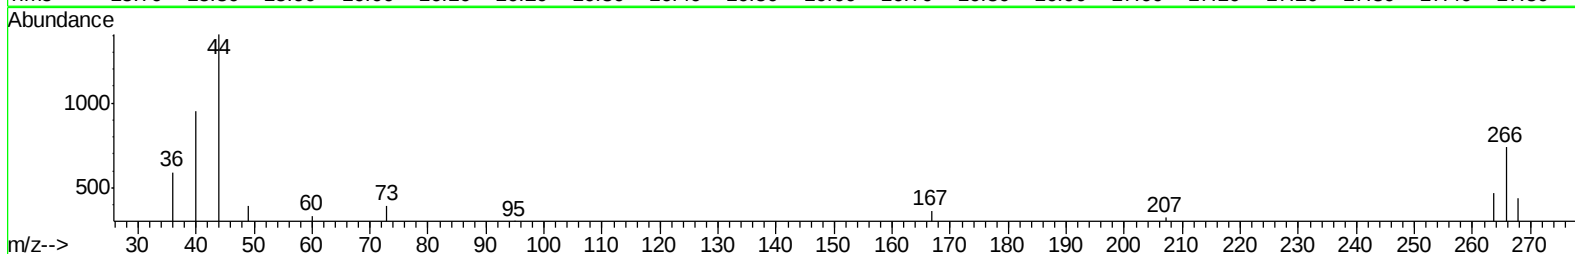


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031020\
Data File : BN010173.D
Acq On : 11 Mar 2020 02:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 07:03:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 19 15:57:43 2020
Response via : Initial Calibration

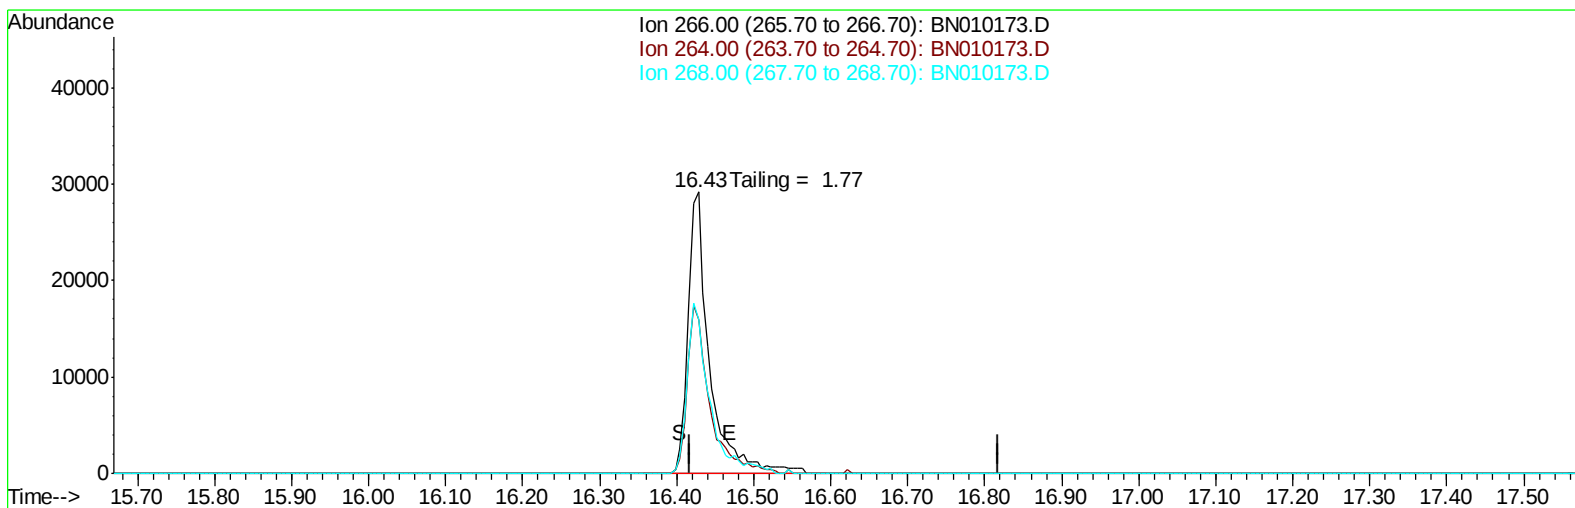

TIC: BN010173.D

(22) Pentachlorophenol

16.518min (-16.518) 0.00ng

response 0

Ion	Exp%	Act%
266.00	100	0.00
264.00	72.60	0.00#
268.00	82.10	0.00#
0.00	0.00	0.00