


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031020\
 Data File : BN010158.D
 Acq On : 10 Mar 2020 12:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 11 17:37:44 2020

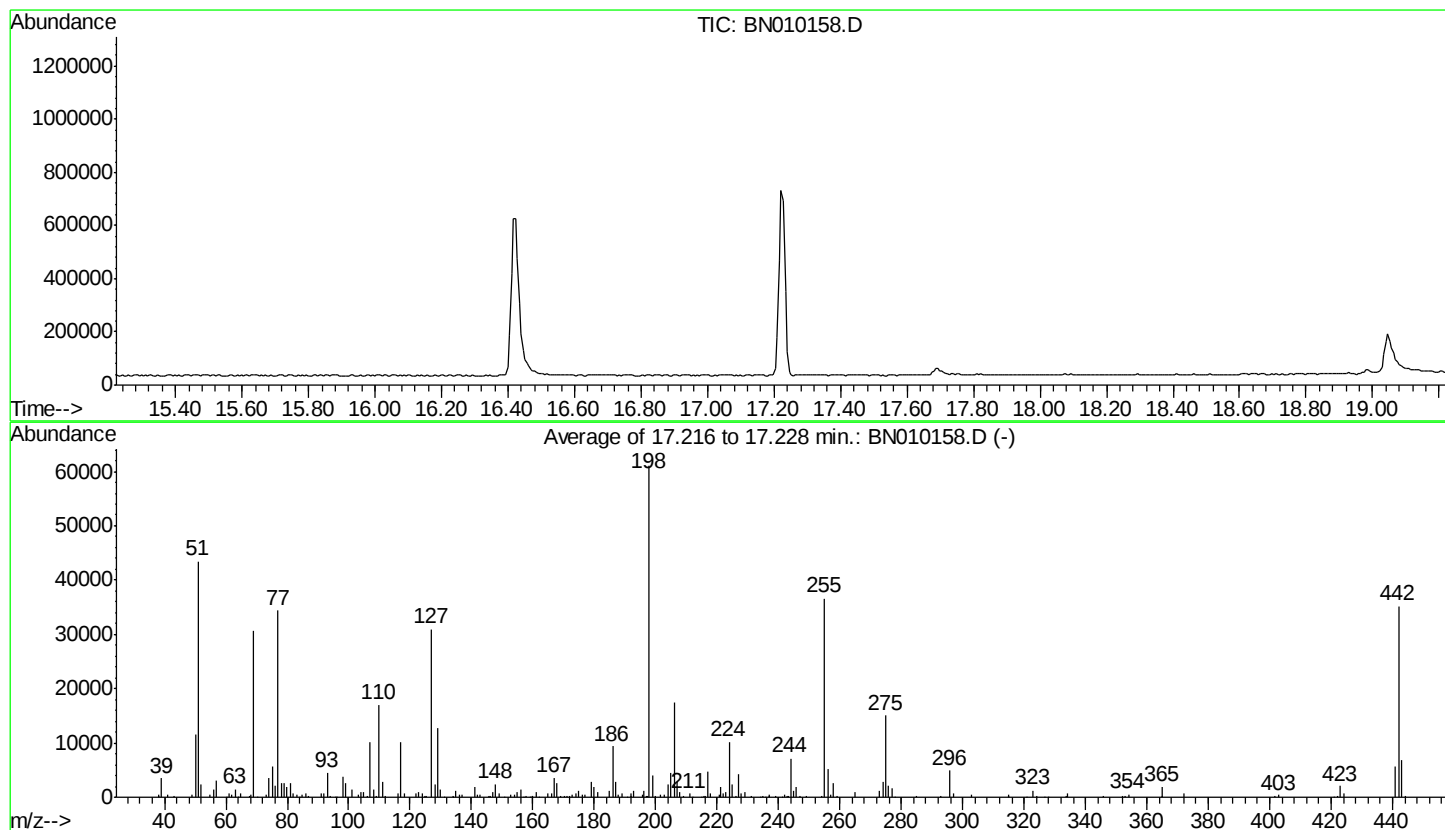

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.1	43445	PASS
68	69	0.00	2	1.6	503	PASS
69	198	0.00	100	50.1	30578	PASS
70	69	0.00	2	0.4	112	PASS
127	198	10	80	50.7	30989	PASS
197	198	0.00	2	0.3	168	PASS
198	198	100	100	100.0	61082	PASS
199	198	5	9	6.7	4081	PASS
275	198	10	60	24.6	15024	PASS
365	198	1	100	3.1	1889	PASS
441	198	0.01	100	9.2	5643	PASS
442	198	50	100	57.7	35215	PASS
443	442	15	24	19.2	6774	PASS