


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031020\
 Data File : BN010173.D
 Acq On : 11 Mar 2020 02:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 11 17:37:44 2020

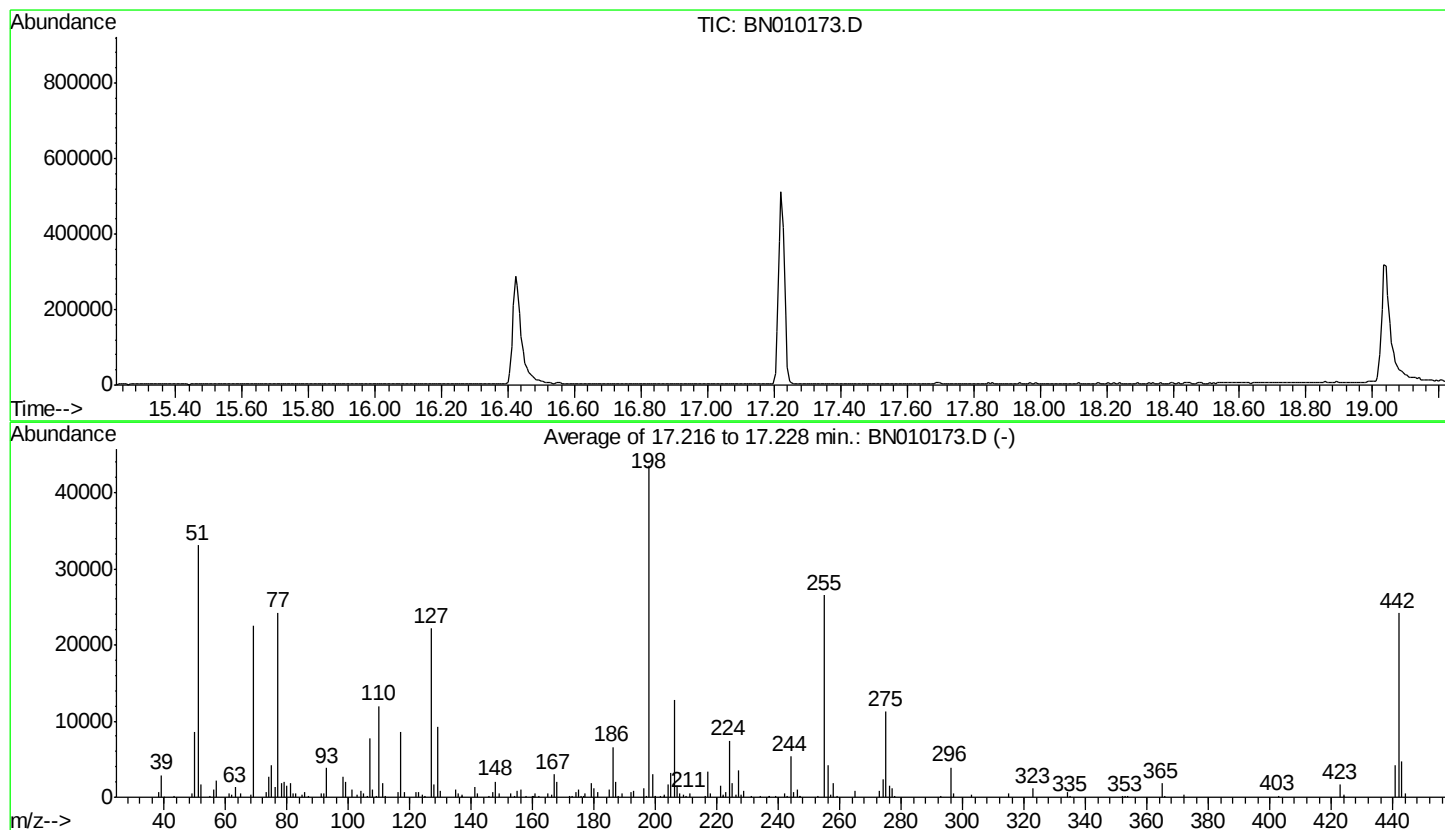

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	75.9	33085	PASS
68	69	0.00	2	1.9	423	PASS
69	198	0.00	100	51.9	22610	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	22168	PASS
197	198	0.00	2	0.2	108	PASS
198	198	100	100	100.0	43576	PASS
199	198	5	9	6.9	3026	PASS
275	198	10	60	25.8	11253	PASS
365	198	1	100	4.2	1830	PASS
441	198	0.01	100	9.5	4151	PASS
442	198	50	100	55.5	24197	PASS
443	442	15	24	19.6	4749	PASS