

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031319\
 Data File : BN004754.D
 Acq On : 14 Mar 2019 09:14
 Operator : JU/SJ
 Sample : K1959-01DL 2X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 14 16:13:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 13 03:05:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	31609	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	135706	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	78614	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	180933	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	180681	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	168889	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.88	99	7680	2.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	19055	13.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	27466	12.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	15538	6.84	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	16001	15.47	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.59	143	18426	15.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	31054	13.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	1154	0.43	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	106807	15.71	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	133241	16.28	ng/ul	0.00
52) 4-Nitrophenol-d4	14.60	143	921	0.73	ng/ul	0.02
58) Fluorene-d10	15.35	176	91676	15.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	12821	10.26	ng/ul	0.00
71) Anthracene-d10	17.20	188	145932	16.56	ng/ul	0.00
79) Pyrene-d10	19.51	212	166089	18.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	140361	15.48	ng/ul	0.00

Target Compounds


					Ovalue
20) Nitrobenzene	8.92	77	103437	48.698	ng/ul 98
32) Caprolactam	11.32	113	2754	3.689	ng/ul# 1
37) 1,2,4,5-Tetrachlorobenzene	12.53	216	3790	1.371	ng/ul 99
73) 1,2,3,4-Tetrachlorobenzene	13.15	216	18428	6.862	ng/uL 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031319\
Data File : BN004754.D
Acq On : 14 Mar 2019 09:14
Operator : JU/SJ
Sample : K1959-01DL 2X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 14 16:13:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 13 03:05:10 2019
Response via : Initial Calibration




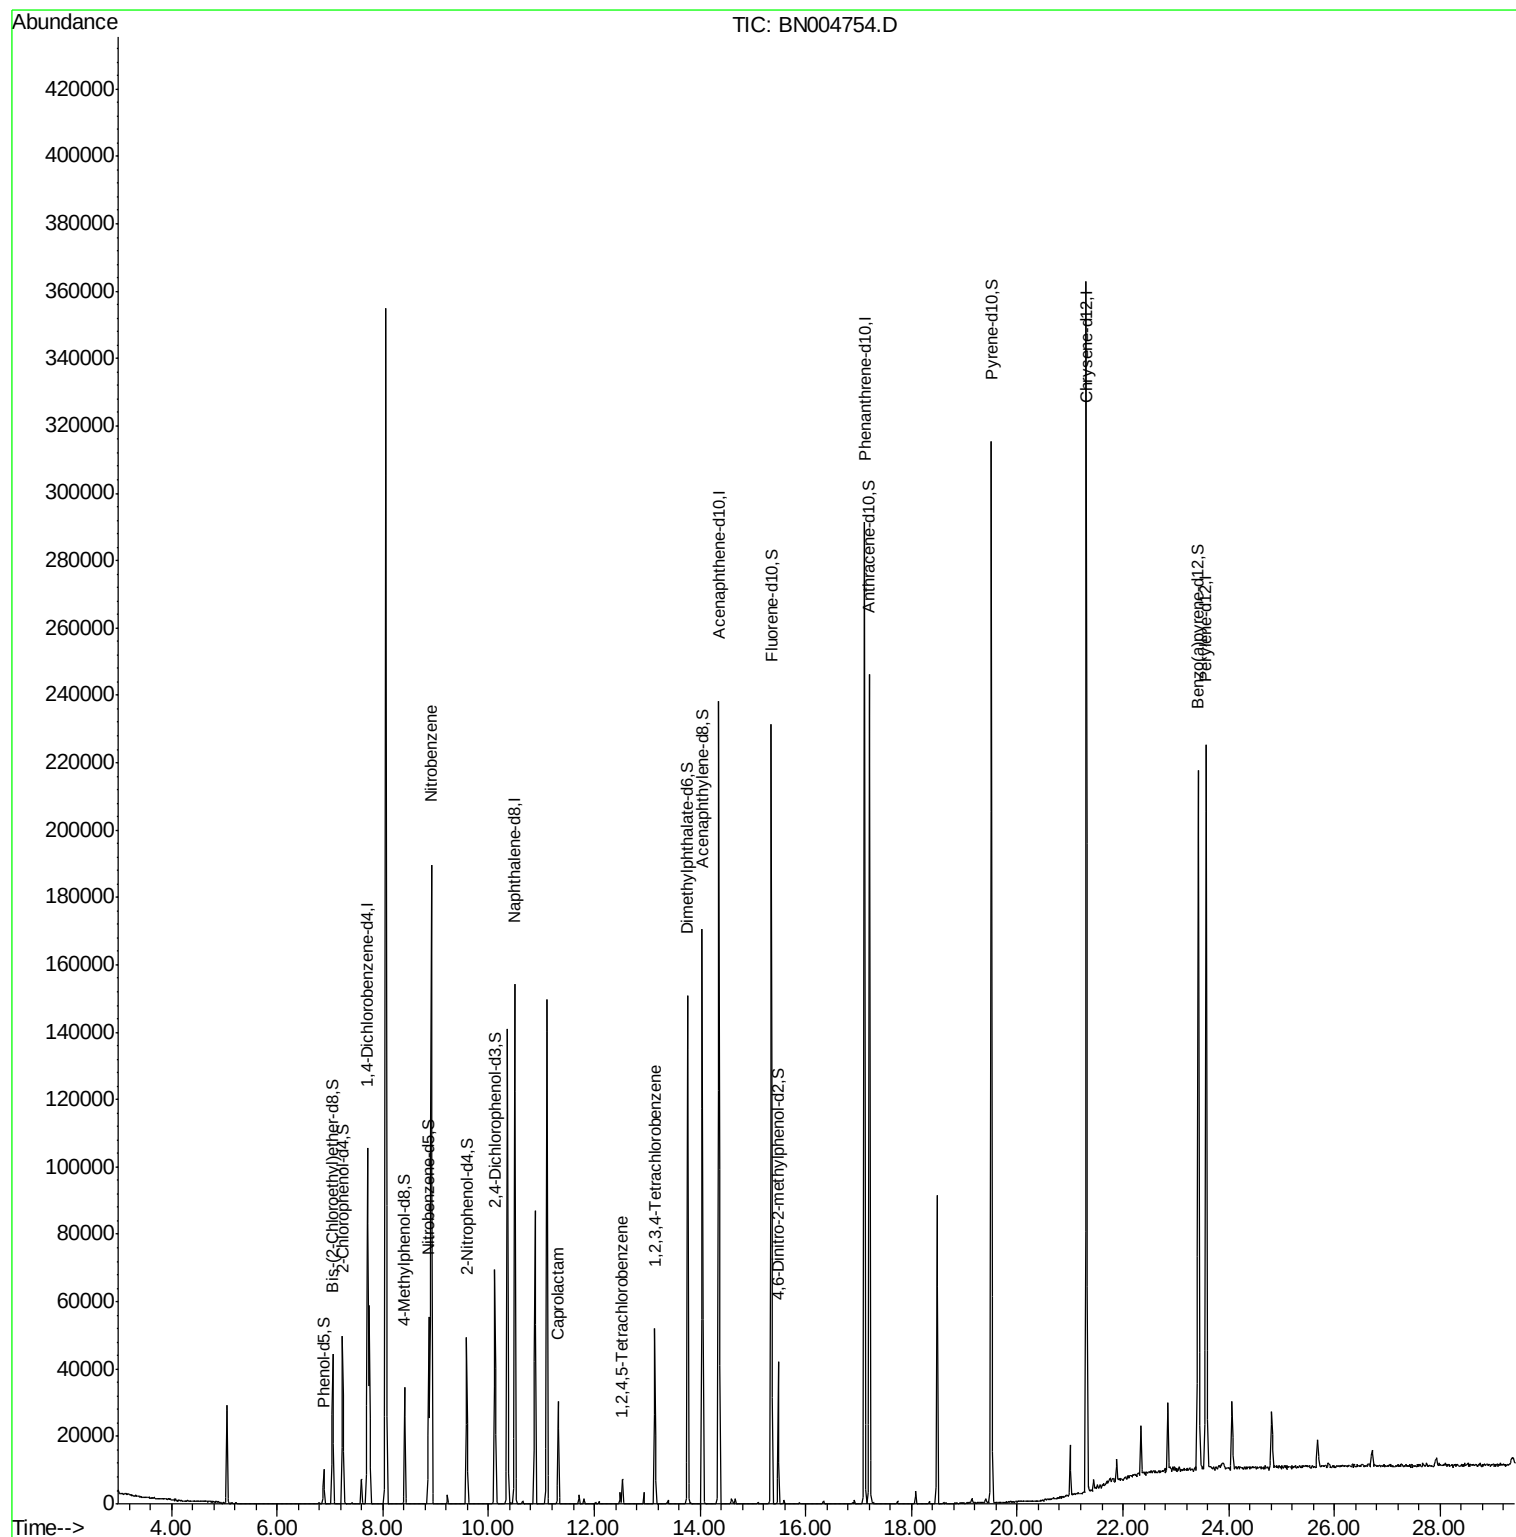


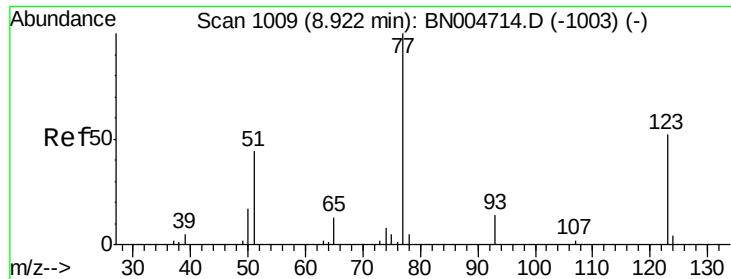

#20
Nitrobenzene
Concen: 48.698 ng/ul
RT: 8.92 min Scan# 1008
Delta R.T. -0.01 min
Lab File: BN004754.D
Acq: 14 Mar 2019 09:14




Instrument :
BNA_N
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
77	100		
123	53.8	41.6	62.4
65	13.3	10.2	15.4

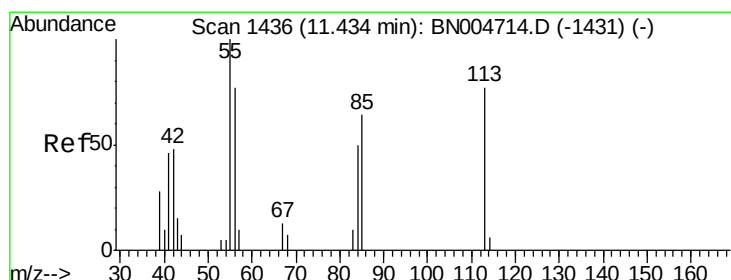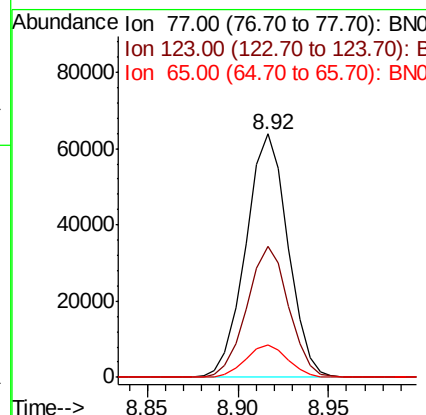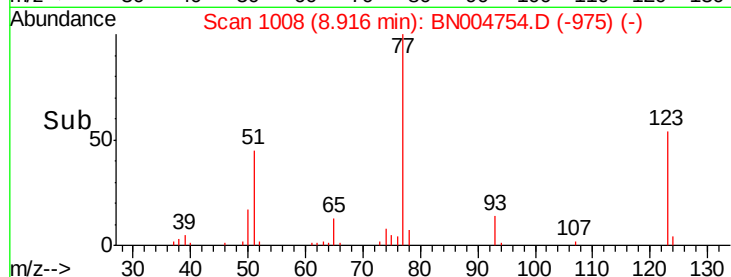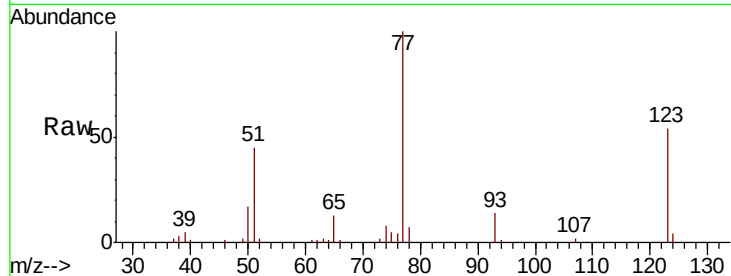

#32
Caprolactam
Concen: 3.689 ng/ul
RT: 11.32 min Scan# 1416
Delta R.T. -0.12 min
Lab File: BN004754.D
Acq: 14 Mar 2019 09:14

Tgt Ion	Ratio	Lower	Upper
113	100		
55	0.0	100.7	151.1#
56	0.0	76.1	114.1#


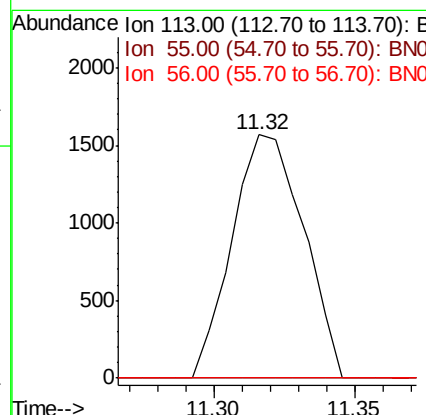
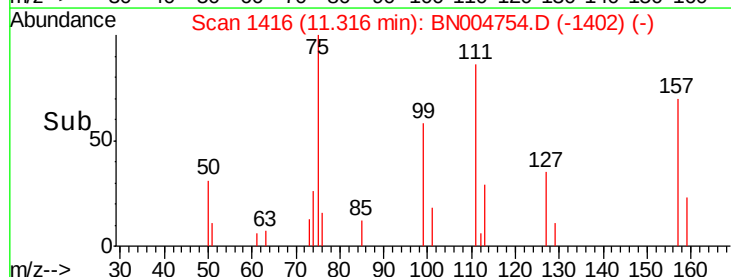
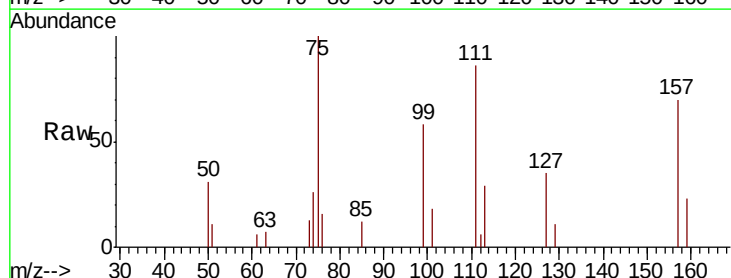


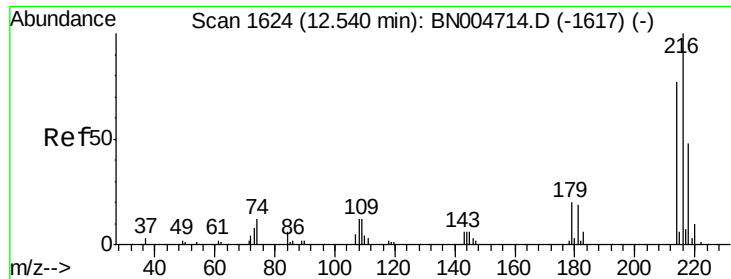

#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 1.371 ng/ul
 RT: 12.53 min Scan# 1623
 Delta R.T. -0.01 min
 Lab File: BN004754.D
 Acq: 14 Mar 2019 09:14

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:216	Resp:	3790
Ion	Ratio	Lower Upper
216	100	
214	75.6	60.9 91.3
179	20.3	16.2 24.4
108	14.2	11.5 17.3

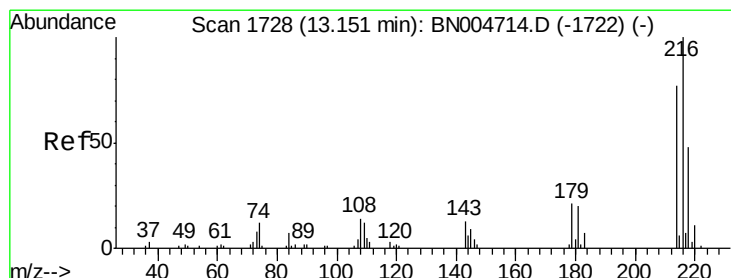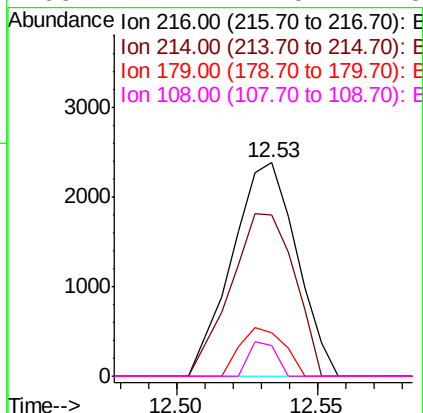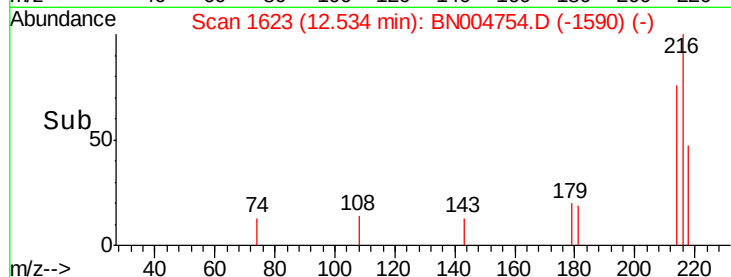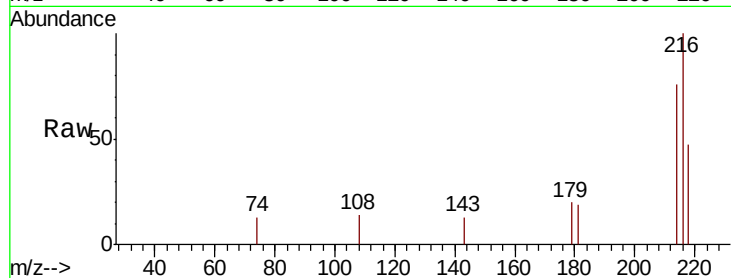

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 6.862 ng/uL
 RT: 13.15 min Scan# 1727
 Delta R.T. -0.01 min
 Lab File: BN004754.D
 Acq: 14 Mar 2019 09:14

Tgt Ion:216	Resp:	18428
Ion	Ratio	Lower Upper
216	100	
214	78.4	61.9 92.9
218	50.1	38.7 58.1

