


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031319\
Data File : BN004740.D
Acq On : 13 Mar 2019 20:40
Operator : JU/SJ
Sample : K1794-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 14 01:25:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 13 03:05:10 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
BF5P5

Manual Integrations
APPROVED

Sohil
3/14/2019 11:14:52 AM

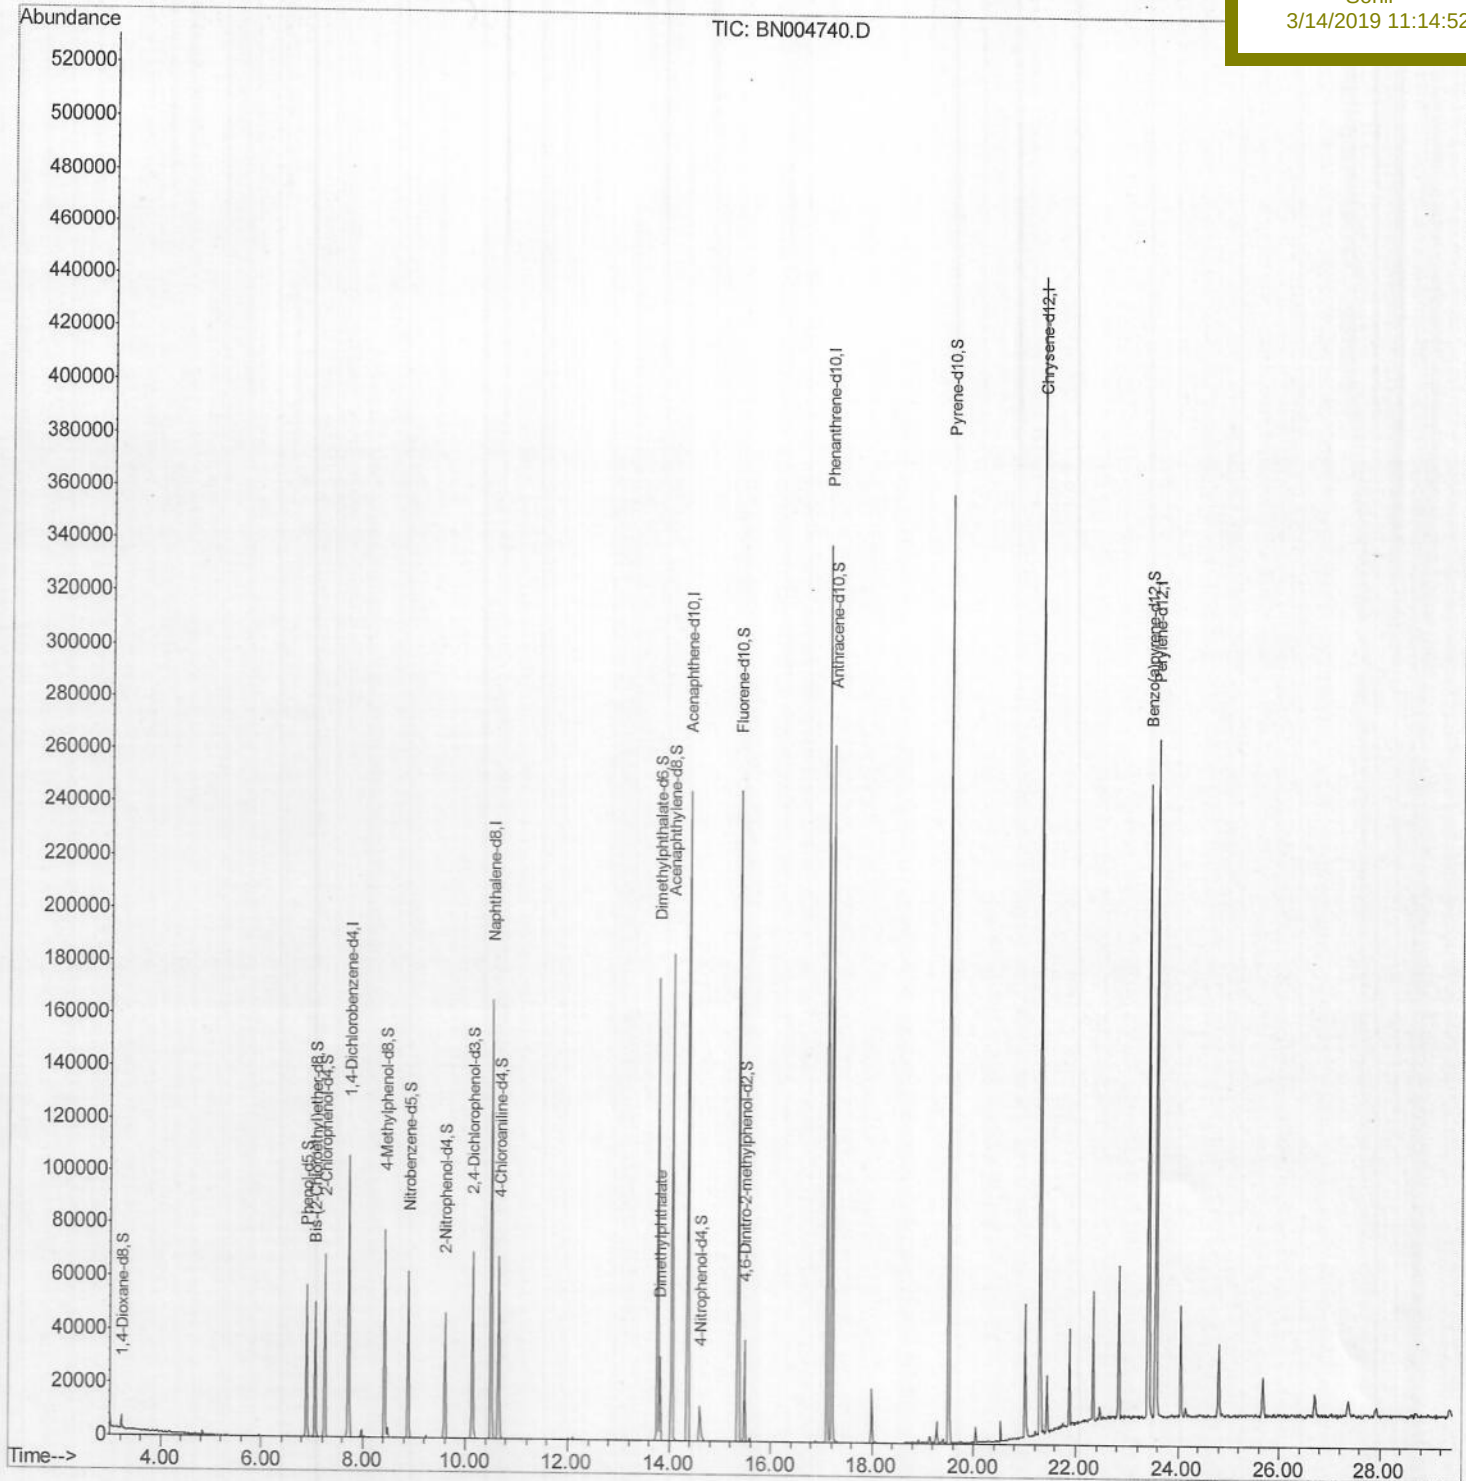

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031319\
 Data File : BN004740.D
 Acq On : 13 Mar 2019 20:40
 Operator : JU/SJ
 Sample : K1794-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 14 00:42:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 13 03:05:10 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 BF5P5

Manual Integrations
 APPROVED

Sohil
 3/14/2019 11:14:52 AM

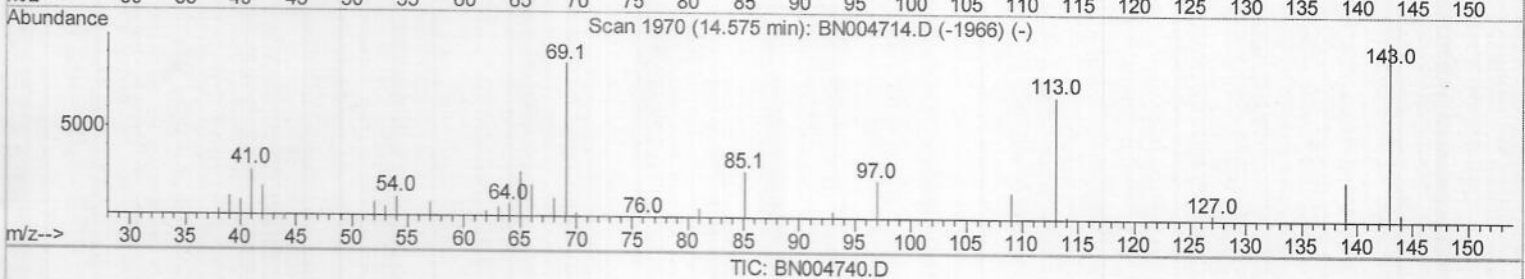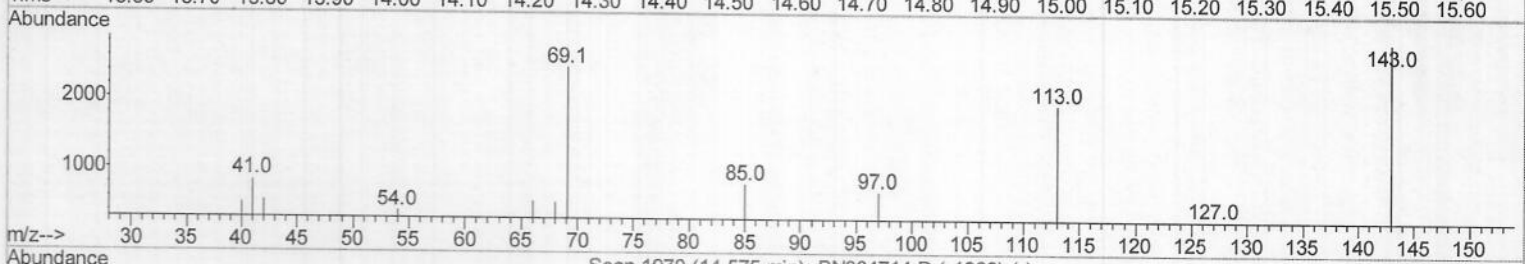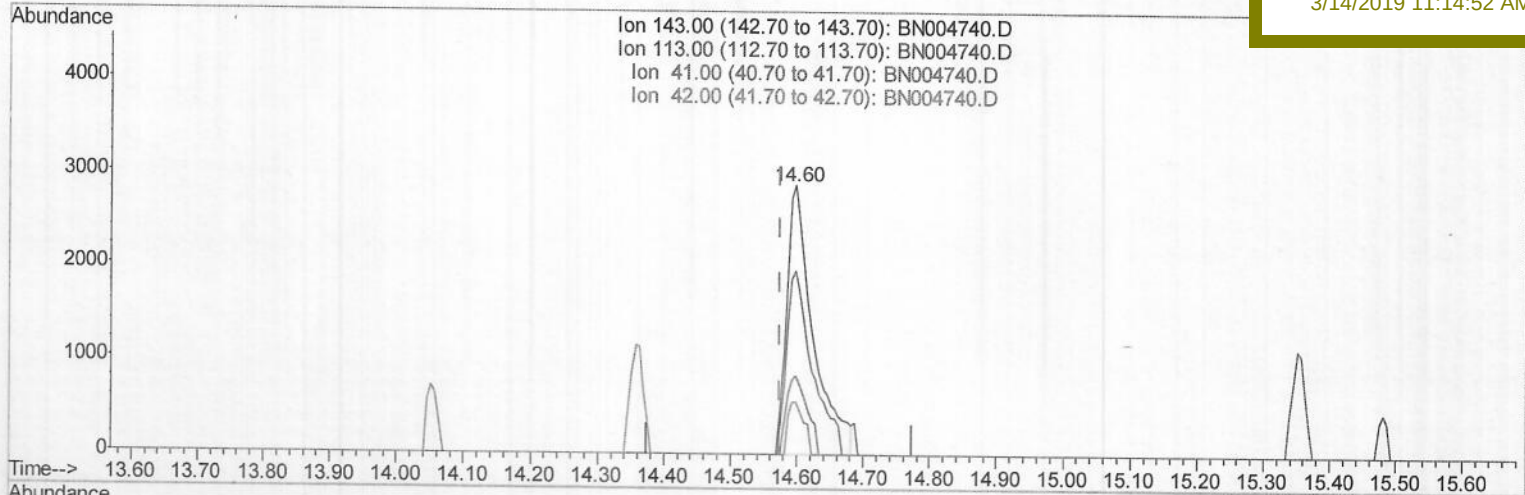

TIC: BN004740.D

(52) 4-Nitrophenol-d4 (S)
 14.598min (+0.024) 5.77ng/ul
 response 7874

Ion	Exp%	Act%
143.00	100	100
113.00	69.80	67.91
41.00	26.70	29.12
42.00	17.80	19.36

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031319\

Data File : BN004740.D

Acq On : 13 Mar 2019 20:40

Operator : JU/SJ

Sample : K1794-18

Misc :

ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 14 00:42:06 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 13 03:05:10 2019

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :




BF5P5

Manual Integrations

APPROVED

Sohil

3/14/2019 11:14:52 AM

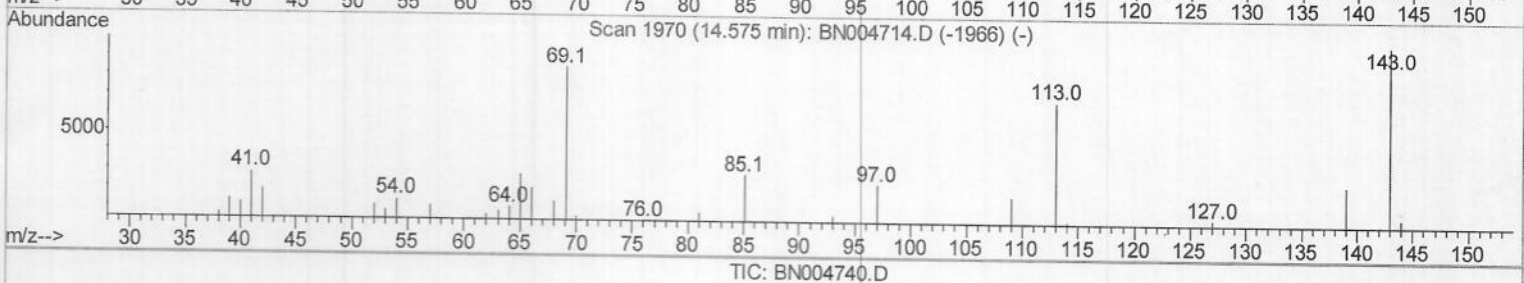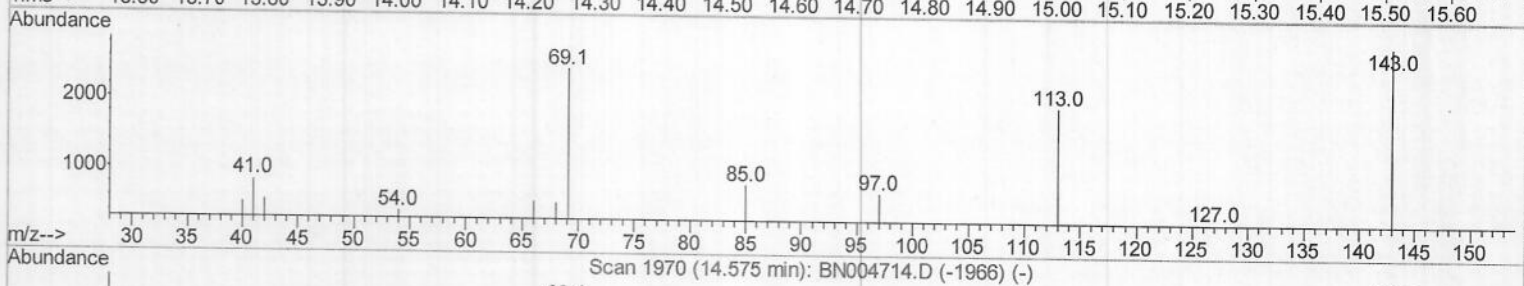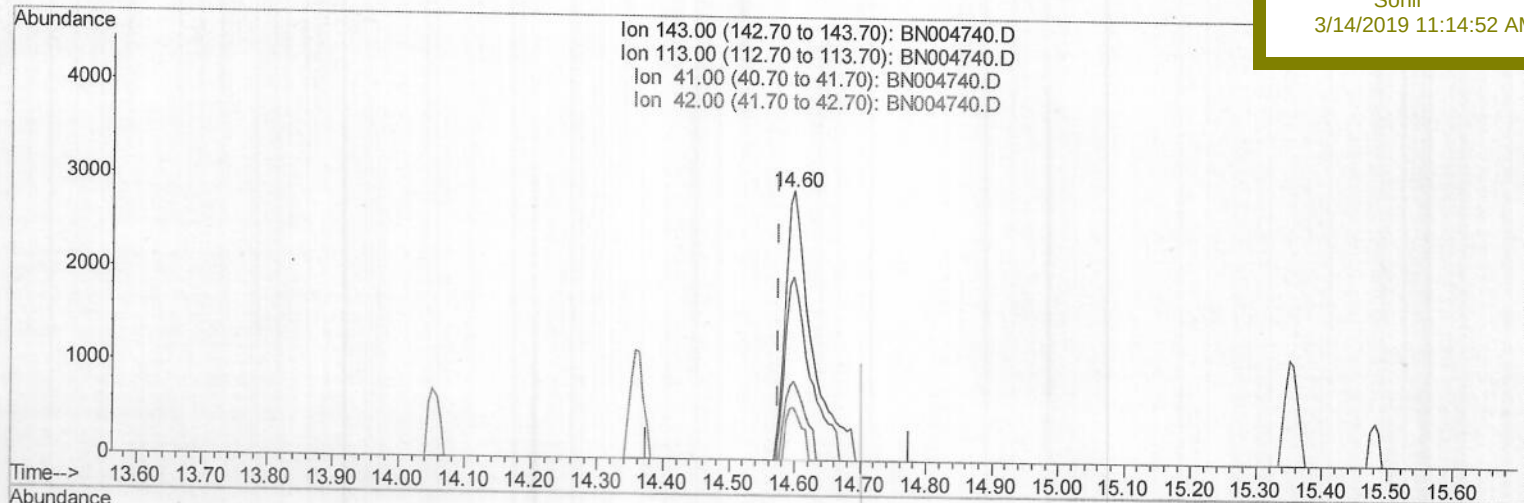

(52) 4-Nitrophenol-d4 (S)

14.598min (+0.024) 5.85ng/ul m

response 7994

Ion	Exp%	Act%
143.00	100	100
113.00	69.80	67.91
41.00	26.70	29.12
42.00	17.80	19.36

S7
03 114119

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031319\
 Data File : BN004740.D
 Acq On : 13 Mar 2019 20:40
 Operator : JU/SJ
 Sample : K1794-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5P5

Quant Time: Mar 14 01:25:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 13 03:05:10 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 3/14/2019 11:14:52 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	32325	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	141120	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	85104	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	198818	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	219666	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	202881	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	3110	5.43	ng/uL	0.00
5) Phenol-d5	6.89	99	36748	13.76	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.06	67	22105	15.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	35856	15.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	32748	14.10	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	17397	16.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	18881	15.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	33299	14.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	44142	15.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	124292	16.89	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	141067	15.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.60	143	7994m	5.85	ng/ul	0.02
58) Fluorene-d10	15.36	176	103834	16.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	11477	8.36	ng/ul	0.00
71) Anthracene-d10	17.20	188	162857	16.82	ng/ul	0.00
79) Pyrene-d10	19.51	212	187684	17.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	160846	14.76	ng/ul	-0.01

Target Compounds

45) Dimethylphthalate	13.82	163	22349	3.095	ng/ul	99
-----------------------	-------	-----	-------	-------	-------	----

(#) = qualifier out of range (m) = manual integration (+) = signals summed

ST
 03/14/19