

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031319\
 Data File : BN004731.D
 Acq On : 13 Mar 2019 15:23
 Operator : JU/SJ
 Sample : K1794-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5N6

Quant Time: Mar 14 00:41:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 13 03:05:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	39899	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	175820	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	107419	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	256965	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	305659	20.00	ng/ul	0.00
86) Perylene-d12	23.57	264	299602	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	5058	7.15	ng/uL	0.00
5) Phenol-d5	6.89	99	66854	20.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	36003	20.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	61170	21.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	58517	20.41	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	29562	22.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	33568	22.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	60561	20.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	84501	24.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	212554	22.88	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	258368	23.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	21698	12.59	ng/ul	0.01
58) Fluorene-d10	15.36	176	183776	23.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	26947	15.19	ng/ul	0.00
71) Anthracene-d10	17.21	188	304348	24.32	ng/ul	0.00
79) Pyrene-d10	19.51	212	357908	23.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.43	264	357005	22.19	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.92	94	3398	1.013	ng/ul 92
45) Dimethylphthalate	13.82	163	36556	4.011	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031319\
Data File : BN004731.D
Acq On : 13 Mar 2019 15:23
Operator : JU/SJ
Sample : K1794-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5N6

Quant Time: Mar 14 00:41:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 13 03:05:10 2019
Response via : Initial Calibration

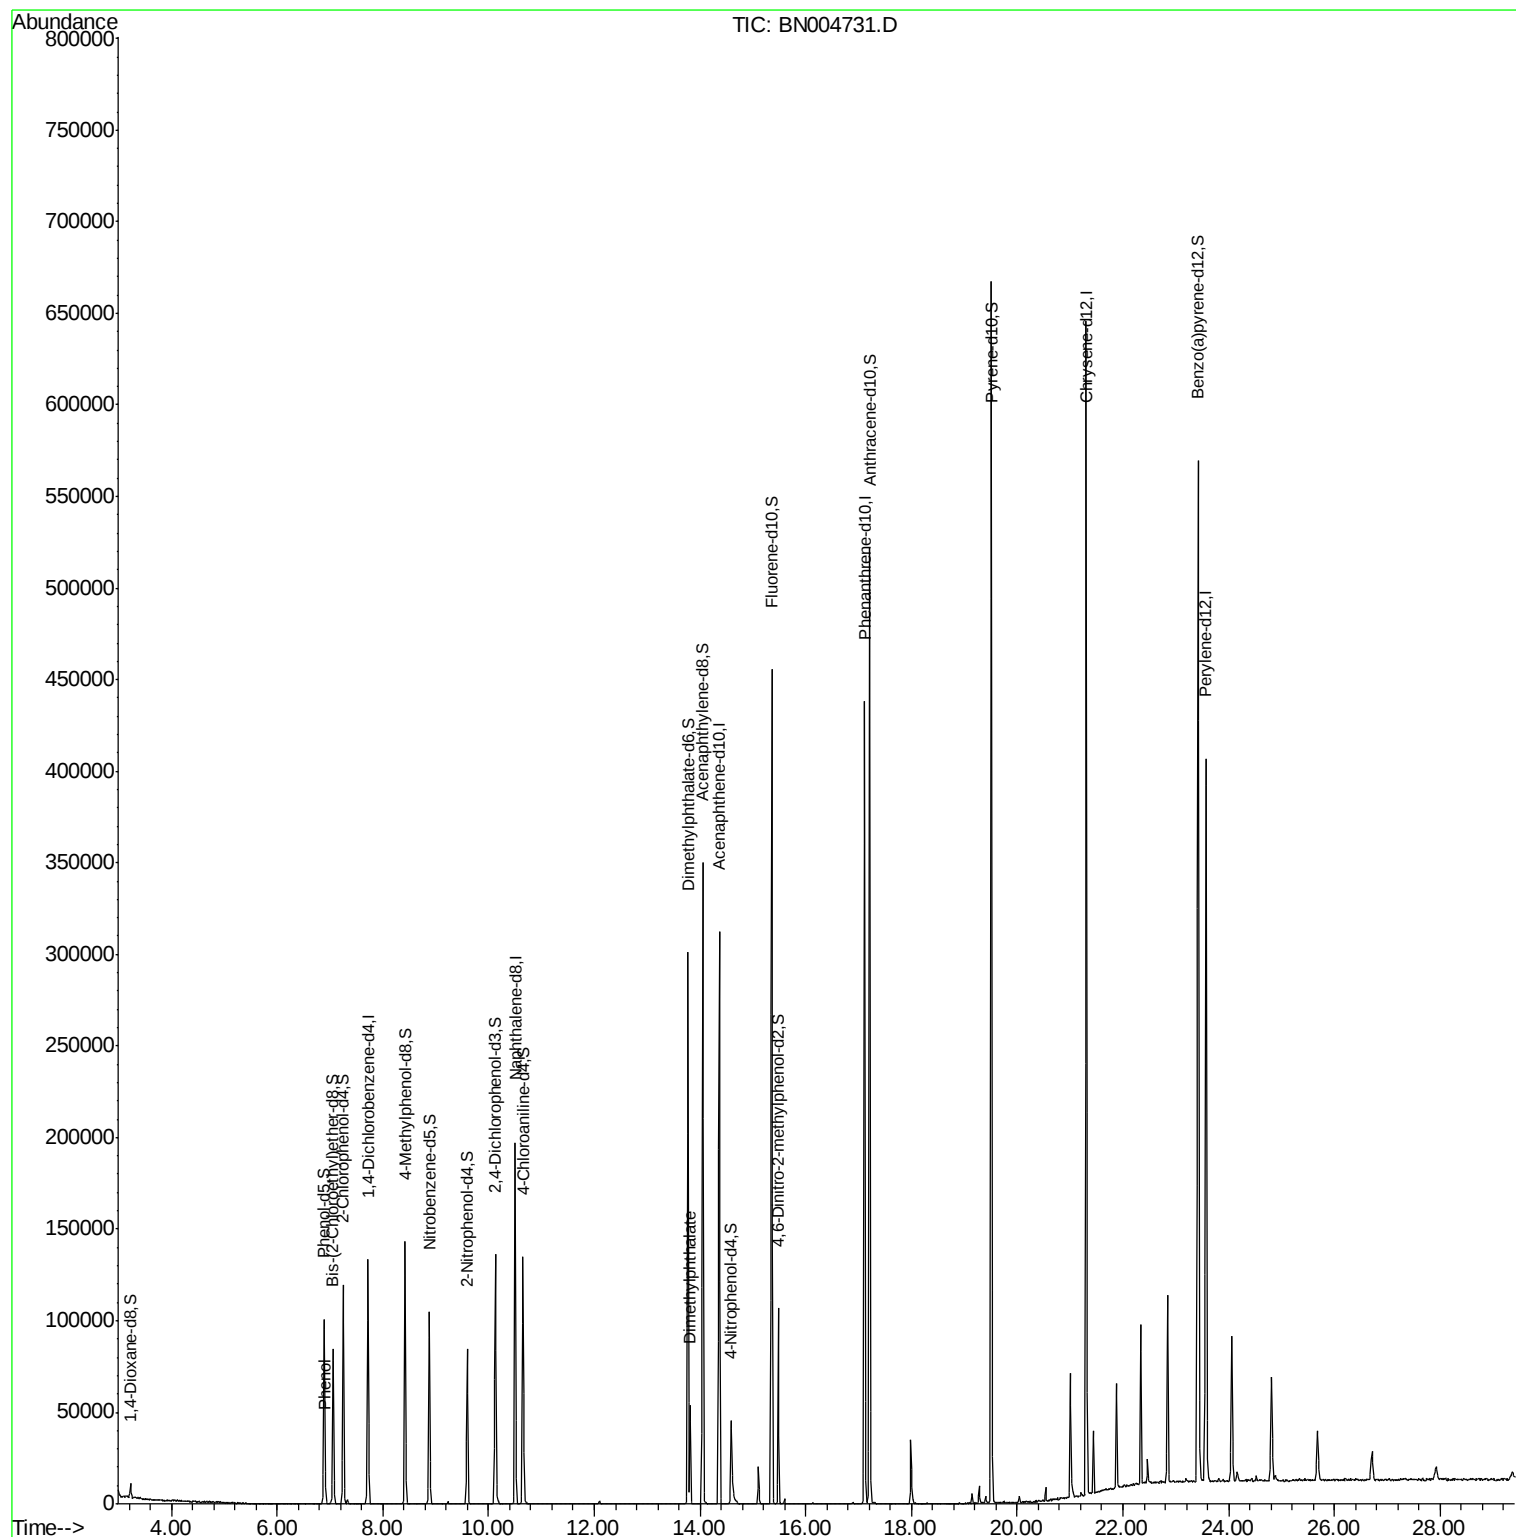

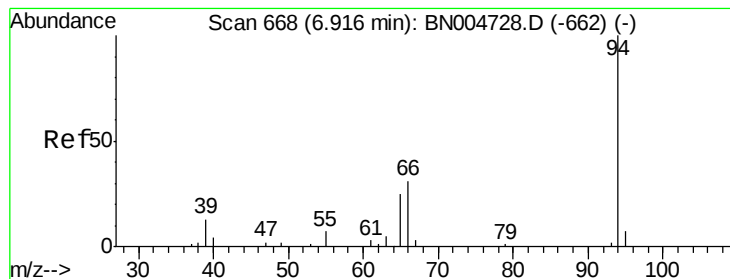

#6

Phenol

Concen: 1.013 ng/ul

RT: 6.92 min Scan# 668

Delta R.T. 0.01 min

Lab File: BN004731.D

Acq: 13 Mar 2019 15:23

Instrument :

BNA_N

ClientSampleId :

BF5N6


Tot Ion: 94 Resp: 3398

Ion Ratio Lower Upper

94 100

65 27.4 20.2 30.4

66 41.2 28.2 42.2



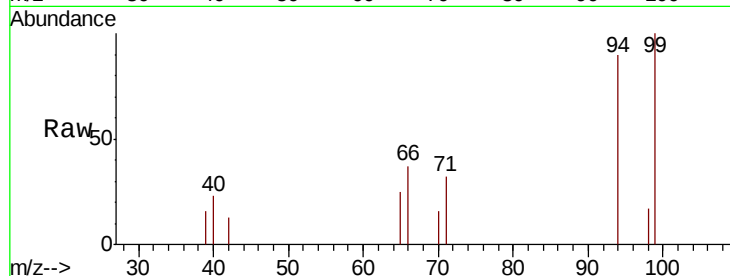


Abundance

Ion 94.00 (93.70 to 94.70): BN004728.D (-662) (-)

Ion 65.00 (64.70 to 65.70): BN004728.D (-662) (-)

Ion 66.00 (65.70 to 66.70): BN004728.D (-662) (-)

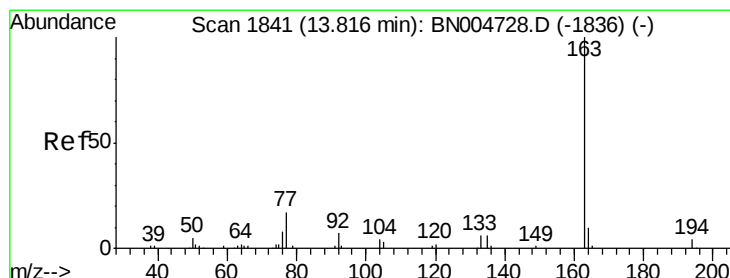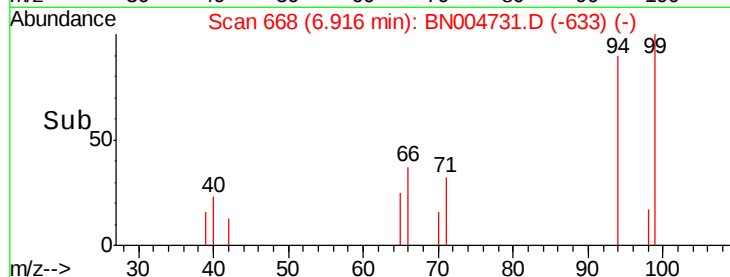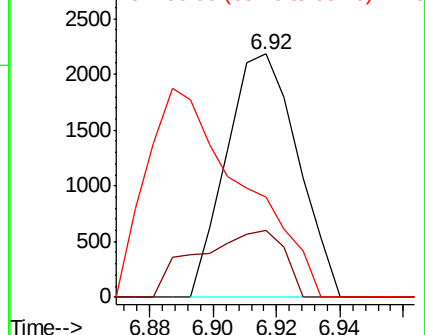

#45

Dimethylphthalate

Concen: 4.011 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. 0.00 min

Lab File: BN004731.D

Acq: 13 Mar 2019 15:23


Tgt Ion: 163 Resp: 36556

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.5 7.9 11.9

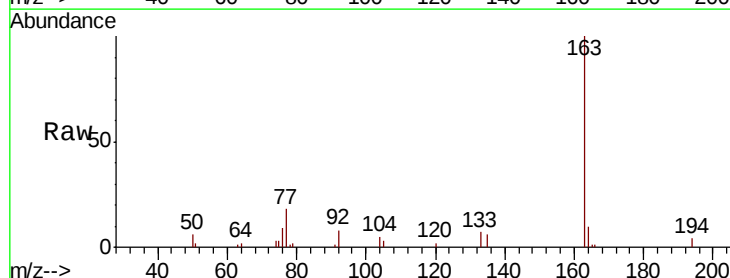

Abundance

Ion 163.00 (162.70 to 163.70): BN004728.D (-1836) (-)

Ion 194.00 (193.70 to 194.70): BN004728.D (-1836) (-)

Ion 164.00 (163.70 to 164.70): BN004728.D (-1836) (-)

