

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031319\
 Data File : BN004750.D
 Acq On : 14 Mar 2019 03:11
 Operator : JU/SJ
 Sample : K1794-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5N5

Quant Time: Mar 14 04:49:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 14 03:49:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	40621	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	174352	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	99353	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	218444	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	194408	20.00	ng/ul	-0.01
86) Perylene-d12	23.56	264	188187	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	4105	5.70	ng/uL	0.00
5) Phenol-d5	6.89	99	53997	16.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	31832	18.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	52361	17.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	42655	14.61	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	26148	19.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	29971	19.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	50496	17.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	63720	18.46	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	176407	20.53	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	202786	19.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	14659	9.19	ng/ul	0.02
58) Fluorene-d10	15.36	176	144436	19.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.48	200	19627	13.01	ng/ul	0.00
71) Anthracene-d10	17.21	188	223918	21.04	ng/ul	0.00
79) Pyrene-d10	19.51	212	232677	24.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	192426	19.04	ng/ul	-0.02


Target Compounds					Ovalue
45) Dimethylphthalate	13.82	163	29292	3.475	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031319\
Data File : BN004750.D
Acq On : 14 Mar 2019 03:11
Operator : JU/SJ
Sample : K1794-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5N5

Quant Time: Mar 14 04:49:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 14 03:49:57 2019
Response via : Initial Calibration

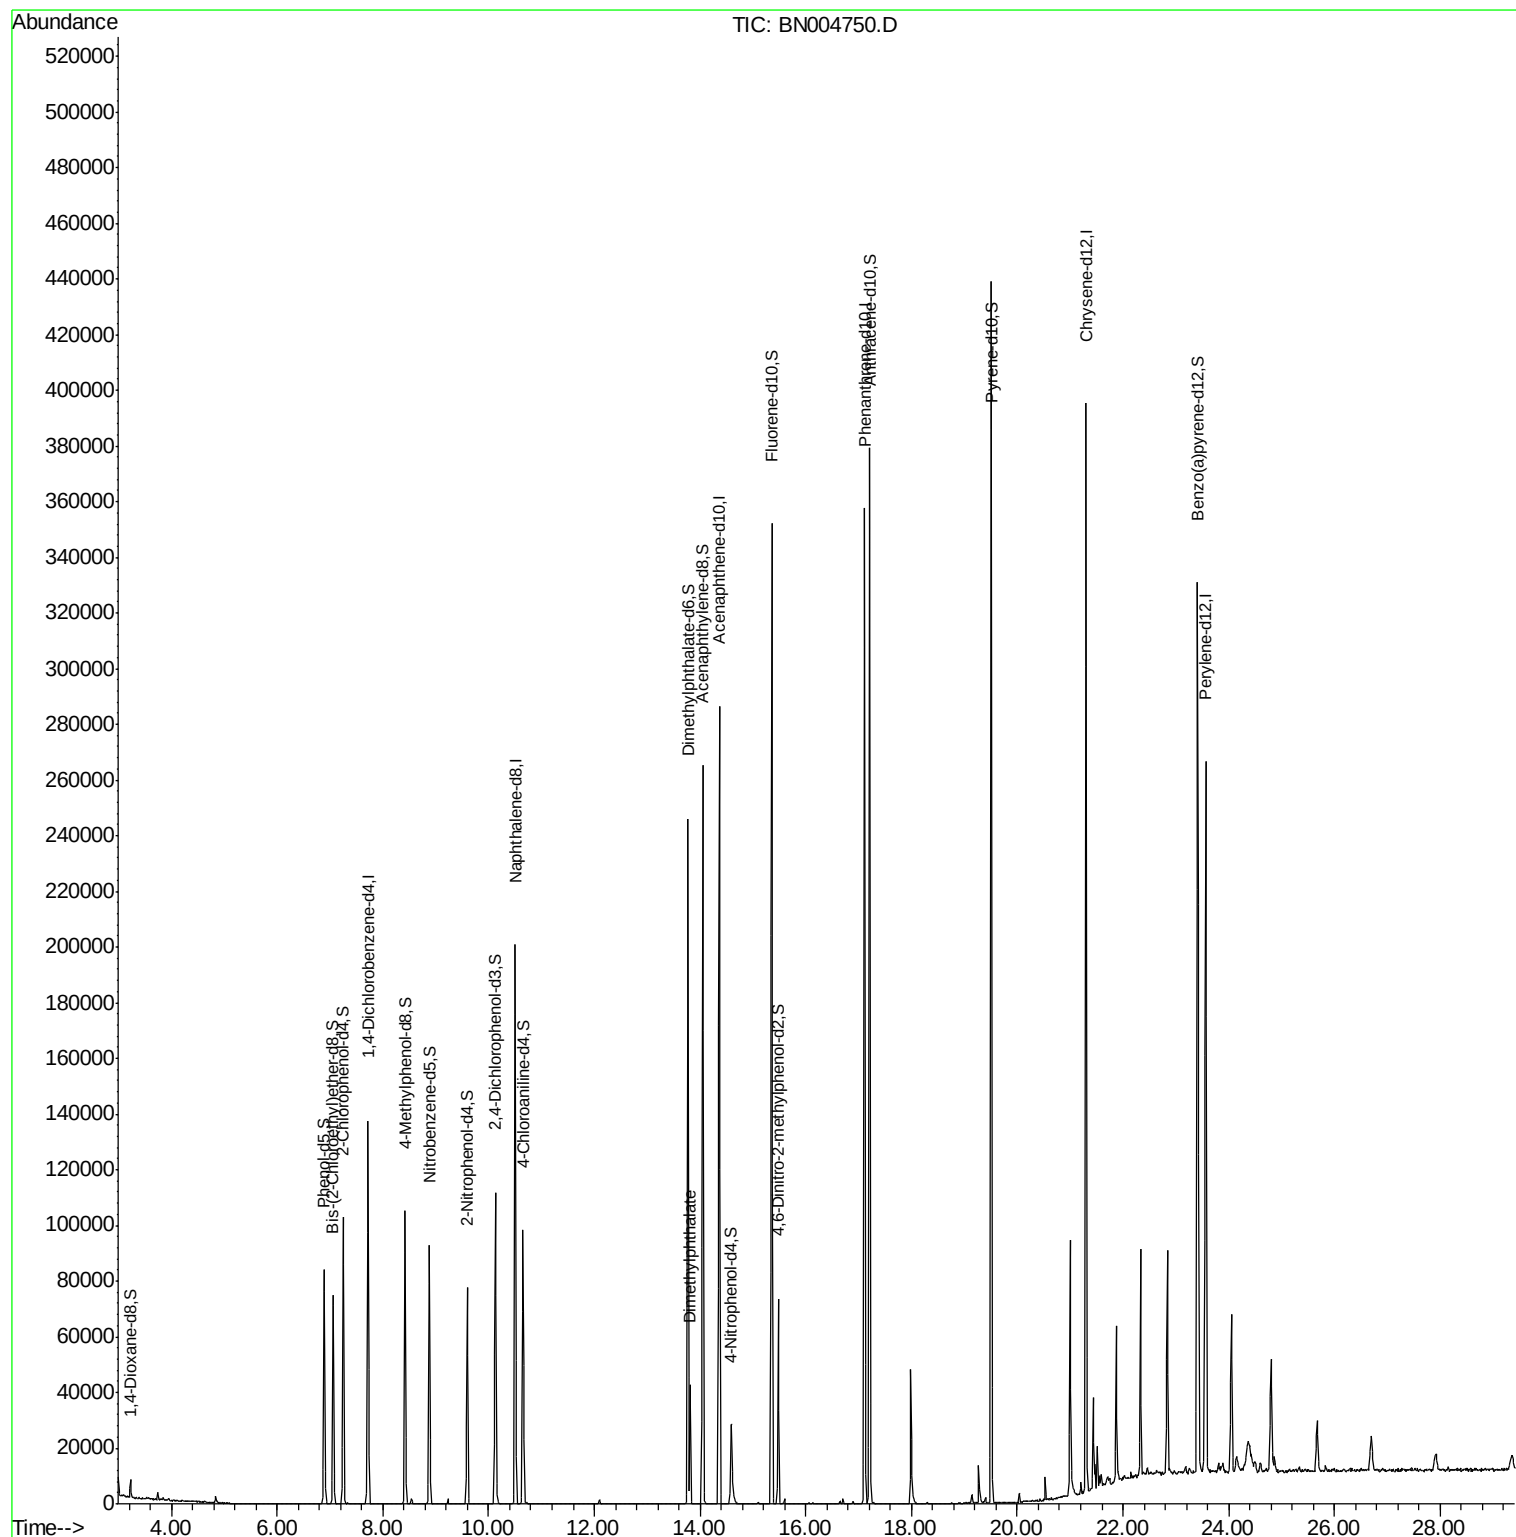

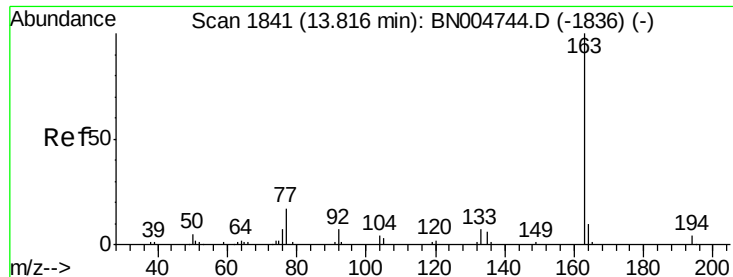

#45

Dimethylphthalate

Concen: 3.475 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. -0.00 min

Lab File: BN004750.D

Acq: 14 Mar 2019 03:11

Instrument :

BNA_N

ClientSampleId :

BF5N5


Tot Ion:163 Resp: 29292

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 10.0 7.9 11.9

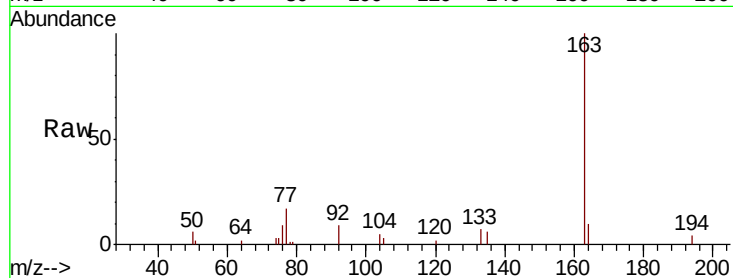

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

