
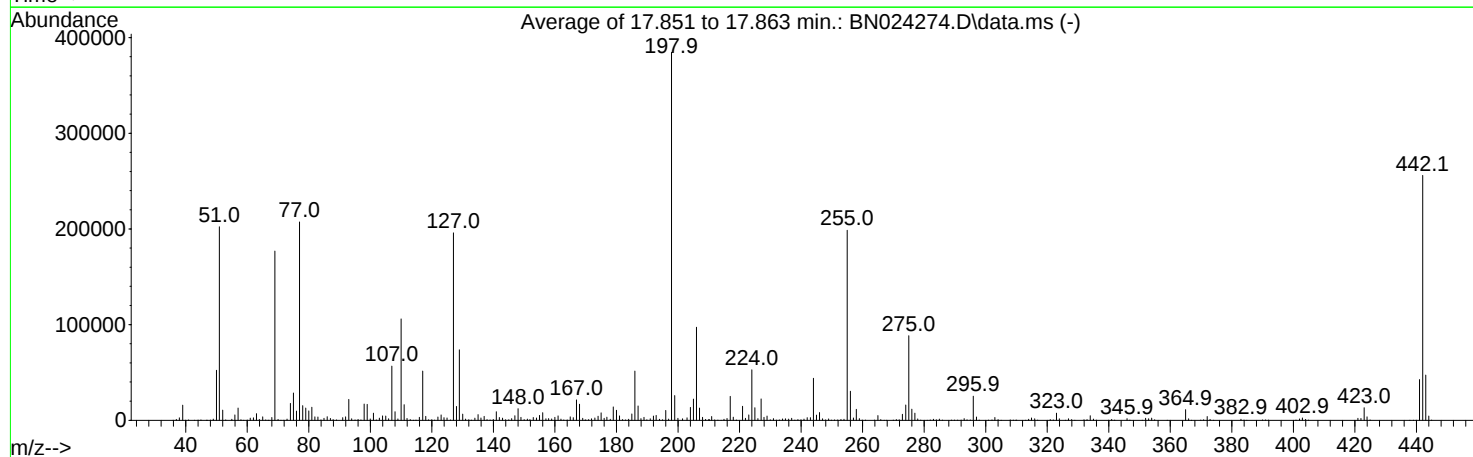


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031423\
Data File : BN024274.D
Acq On : 14 Mar 2023 10:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 15 01:49:05 2023

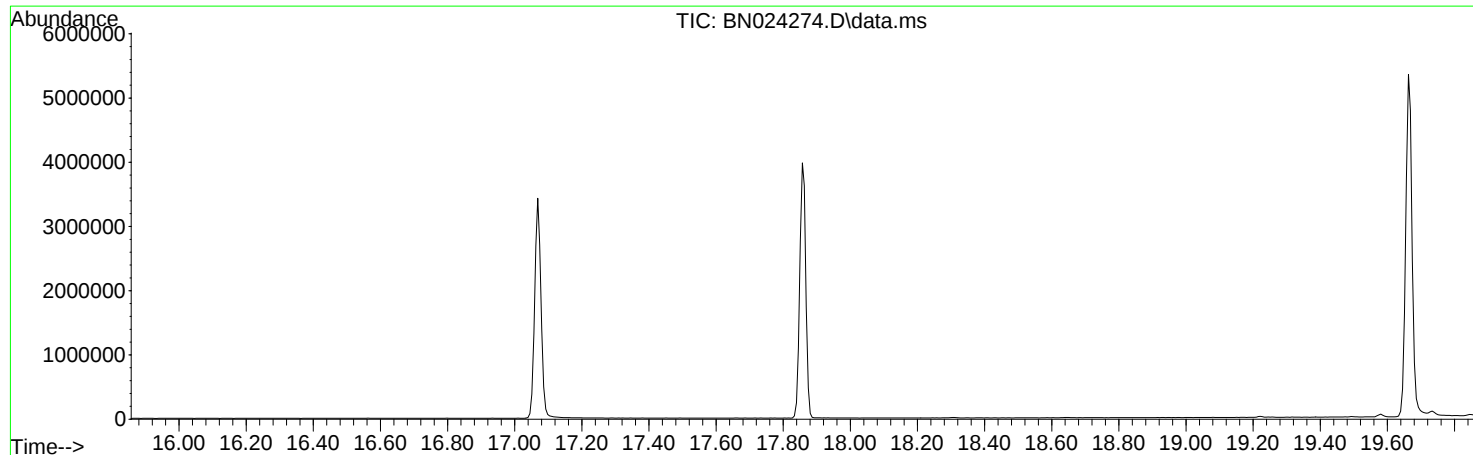




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	202243	PASS
68	69	0.00	2	1.6	2907	PASS
69	198	0.00	100	46.0	176896	PASS
70	69	0.00	2	0.5	900	PASS
127	198	10	80	51.0	195989	PASS
197	198	0.00	2	0.3	1212	PASS
198	198	100	100	100.0	384469	PASS
199	198	5	9	6.7	25877	PASS
275	198	10	60	23.0	88312	PASS
365	198	1	100	2.9	11184	PASS
441	198	0.01	100	11.1	42552	PASS
442	442	50	100	100.0	255936	PASS
443	442	15	24	18.5	47325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031423\
Data File : BN024274.D
Acq On : 14 Mar 2023 10:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 06:06:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 15 06:06:29 2023
Response via : Initial Calibration

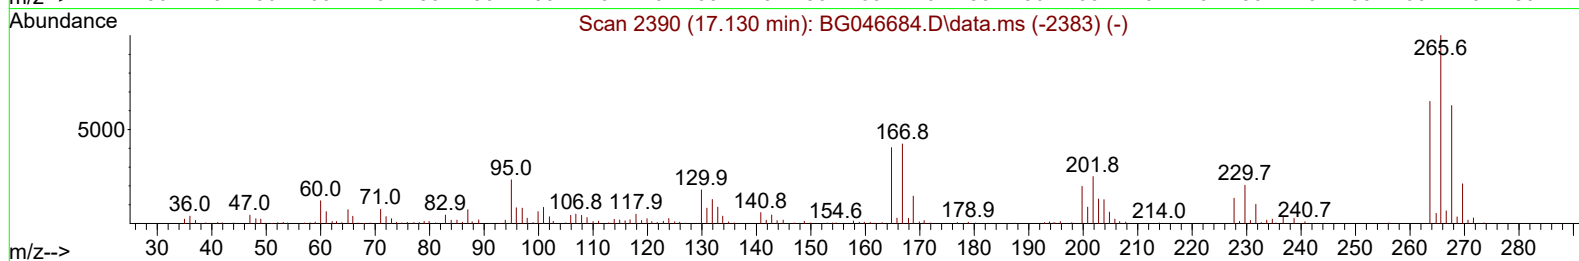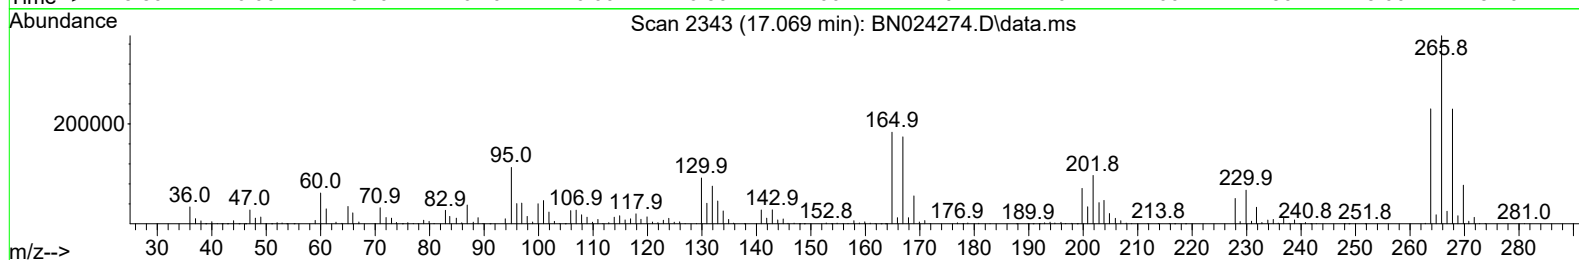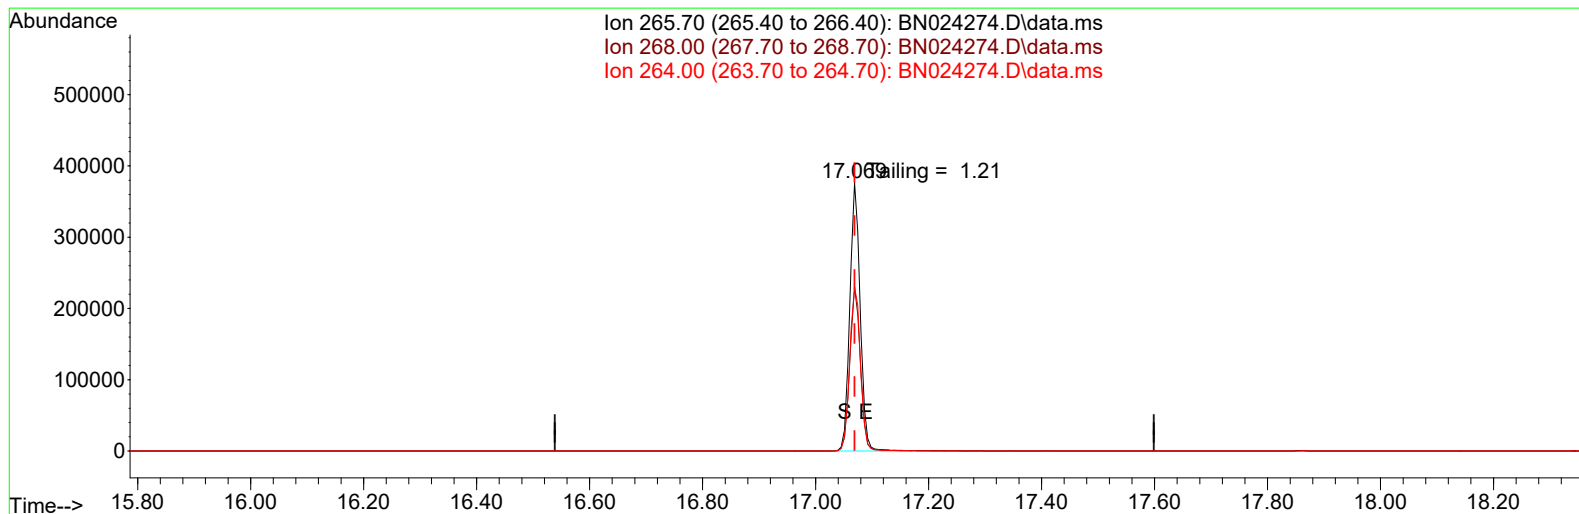

TIC: BN024274.D\data.ms

(70) Pentachlorophenol (C)

17.069min (0.000) 27269.59 ng




response 483865

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.01
264.00	61.60	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031423\
Data File : BN024274.D
Acq On : 14 Mar 2023 10:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 06:06:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 15 06:06:29 2023
Response via : Initial Calibration

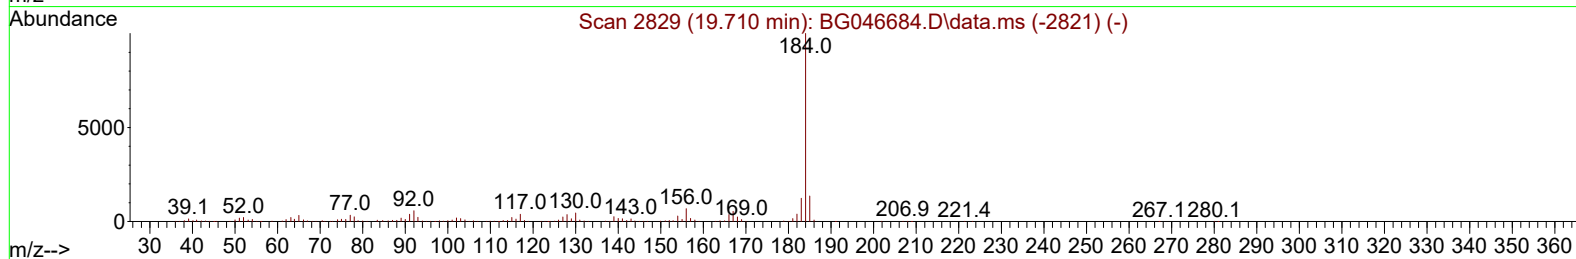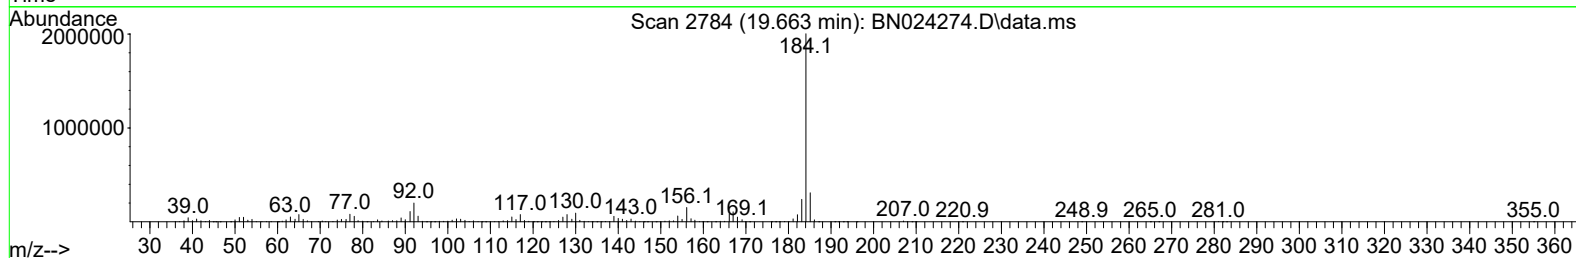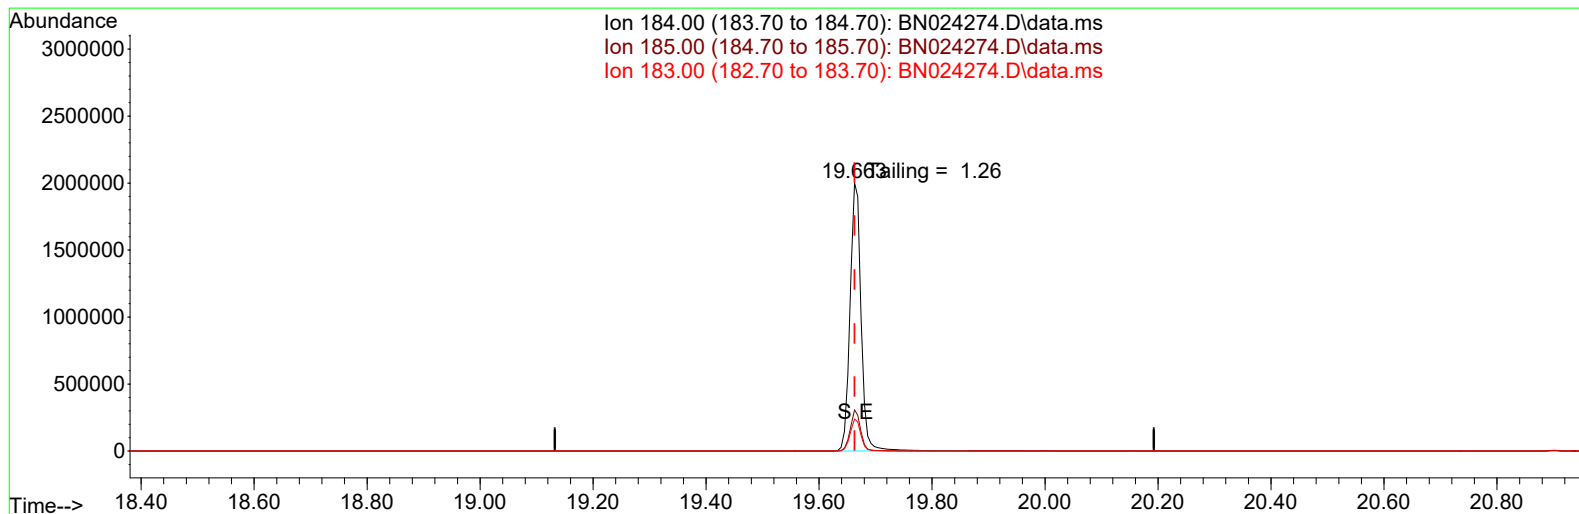

TIC: BN024274.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 2731183

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.39
183.00	13.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2023	BNA_N	<u>BN024274.D</u>
Compound Name	Response	Retention Time
DDT	1252150	20.904
DDD	29516	20.457
DDE	760	19.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30276	1282426	2.36

Instrument :
BNA_N
ClientSampleId :
DFTPP