

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031519\
 Data File : BN004774.D
 Acq On : 15 Mar 2019 16:48
 Operator : JU/SJ
 Sample : K1919-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 15 22:35:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 15 04:01:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	24797	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	110353	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.35	164	70962	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.10	188	174757	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	233669	20.00	ng/ul	-0.01
86) Perylene-d12	23.56	264	268422	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	1669	3.80	ng/uL	0.00
5) Phenol-d5	6.88	99	8098	3.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	21212	19.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	30845	17.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	17491	9.81	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	18476	21.96	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.59	143	21255	22.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	35376	19.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	216	0.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	149575	24.38	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	170728	23.12	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	2360	2.07	ng/ul	0.00
58) Fluorene-d10	15.35	176	131966	25.31	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.47	200	24180	20.04	ng/ul	0.00
71) Anthracene-d10	17.20	188	228390	26.83	ng/ul	-0.01
79) Pyrene-d10	19.50	212	276362	24.21	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.42	264	347981	24.14	ng/ul	-0.02


Target Compounds				Ovalue
6) Phenol	6.90	94	4188	2.008 ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031519\
Data File : BN004774.D
Acq On : 15 Mar 2019 16:48
Operator : JU/SJ
Sample : K1919-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 15 22:35:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 15 04:01:10 2019
Response via : Initial Calibration

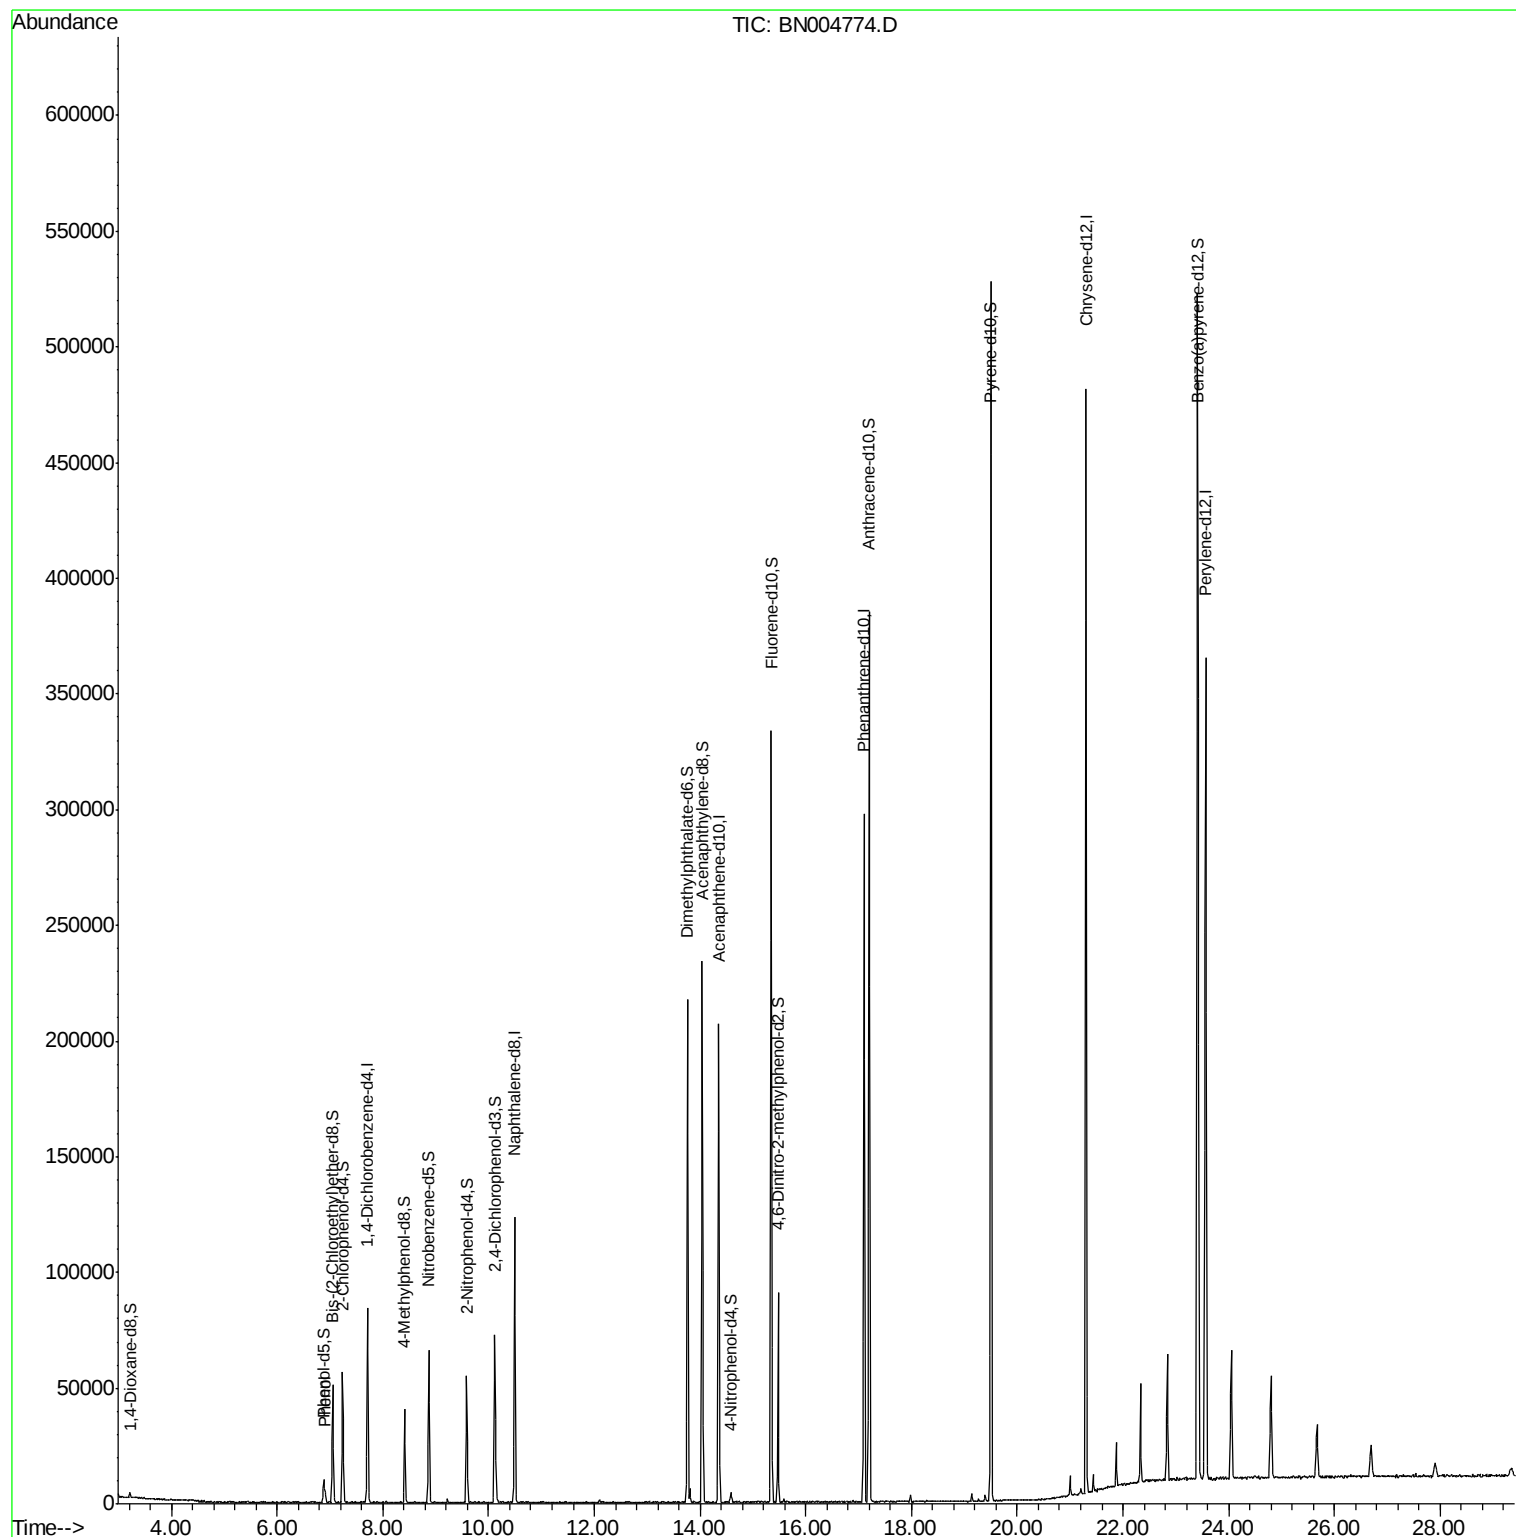

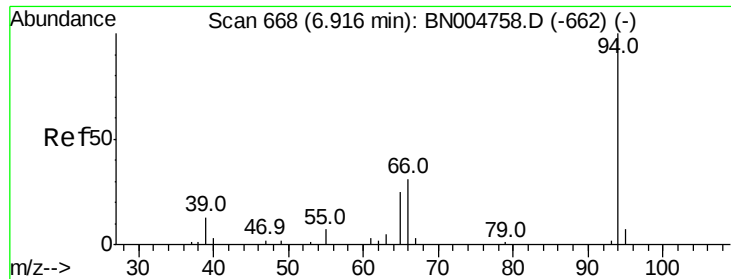

#6

Phenol

Concen: 2.008 ng/ul

RT: 6.90 min Scan# 666

Delta R.T. -0.01 min

Lab File: BN004774.D

Acq: 15 Mar 2019 16:48

Instrument :

BNA_N

ClientSampleId :


Tot Ion: 94 Resp: 4188

Ion Ratio Lower Upper

94 100

65 25.2 20.2 30.4

66 35.3 28.2 42.2

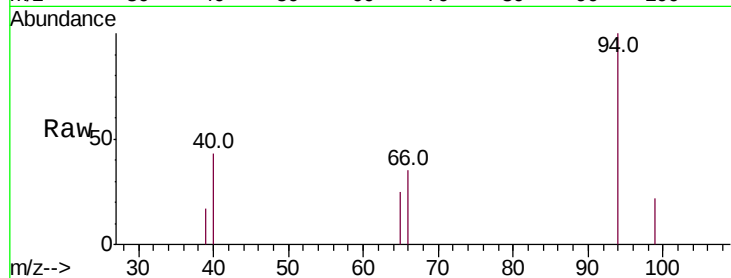

Abundance Ion 94.00 (93.70 to 94.70): BNC

Ion 65.00 (64.70 to 65.70): BNC

Ion 66.00 (65.70 to 66.70): BNC

