

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031519\
 Data File : BN004770.D
 Acq On : 15 Mar 2019 14:27
 Operator : JU/SJ
 Sample : K1919-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C09G8

Quant Time: Mar 15 22:34:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 15 04:01:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	20449	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	91597	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.35	164	59560	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.10	188	148220	20.00	ng/ul	-0.01
78) Chrysene-d12	21.30	240	196735	20.00	ng/ul	-0.01
86) Perylene-d12	23.56	264	224666	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	1998	5.51	ng/uL	0.00
5) Phenol-d5	6.88	99	10636	6.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	25422	28.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	36502	24.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	21803	14.84	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	21572	30.89	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.59	143	25231	31.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	42537	28.14	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	13.76	166	165521	32.14	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	195719	31.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	3439	3.60	ng/ul	0.00
58) Fluorene-d10	15.35	176	144546	33.02	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.47	200	27163	26.55	ng/ul	0.00
71) Anthracene-d10	17.20	188	244389	33.85	ng/ul	-0.01
79) Pyrene-d10	19.50	212	297270	30.92	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.42	264	376645	31.22	ng/ul	-0.02


Target Compounds					Qvalue	
6) Phenol	6.90	94	2566	1.492	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031519\
Data File : BN004770.D
Acq On : 15 Mar 2019 14:27
Operator : JU/SJ
Sample : K1919-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C09G8

Quant Time: Mar 15 22:34:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 15 04:01:10 2019
Response via : Initial Calibration

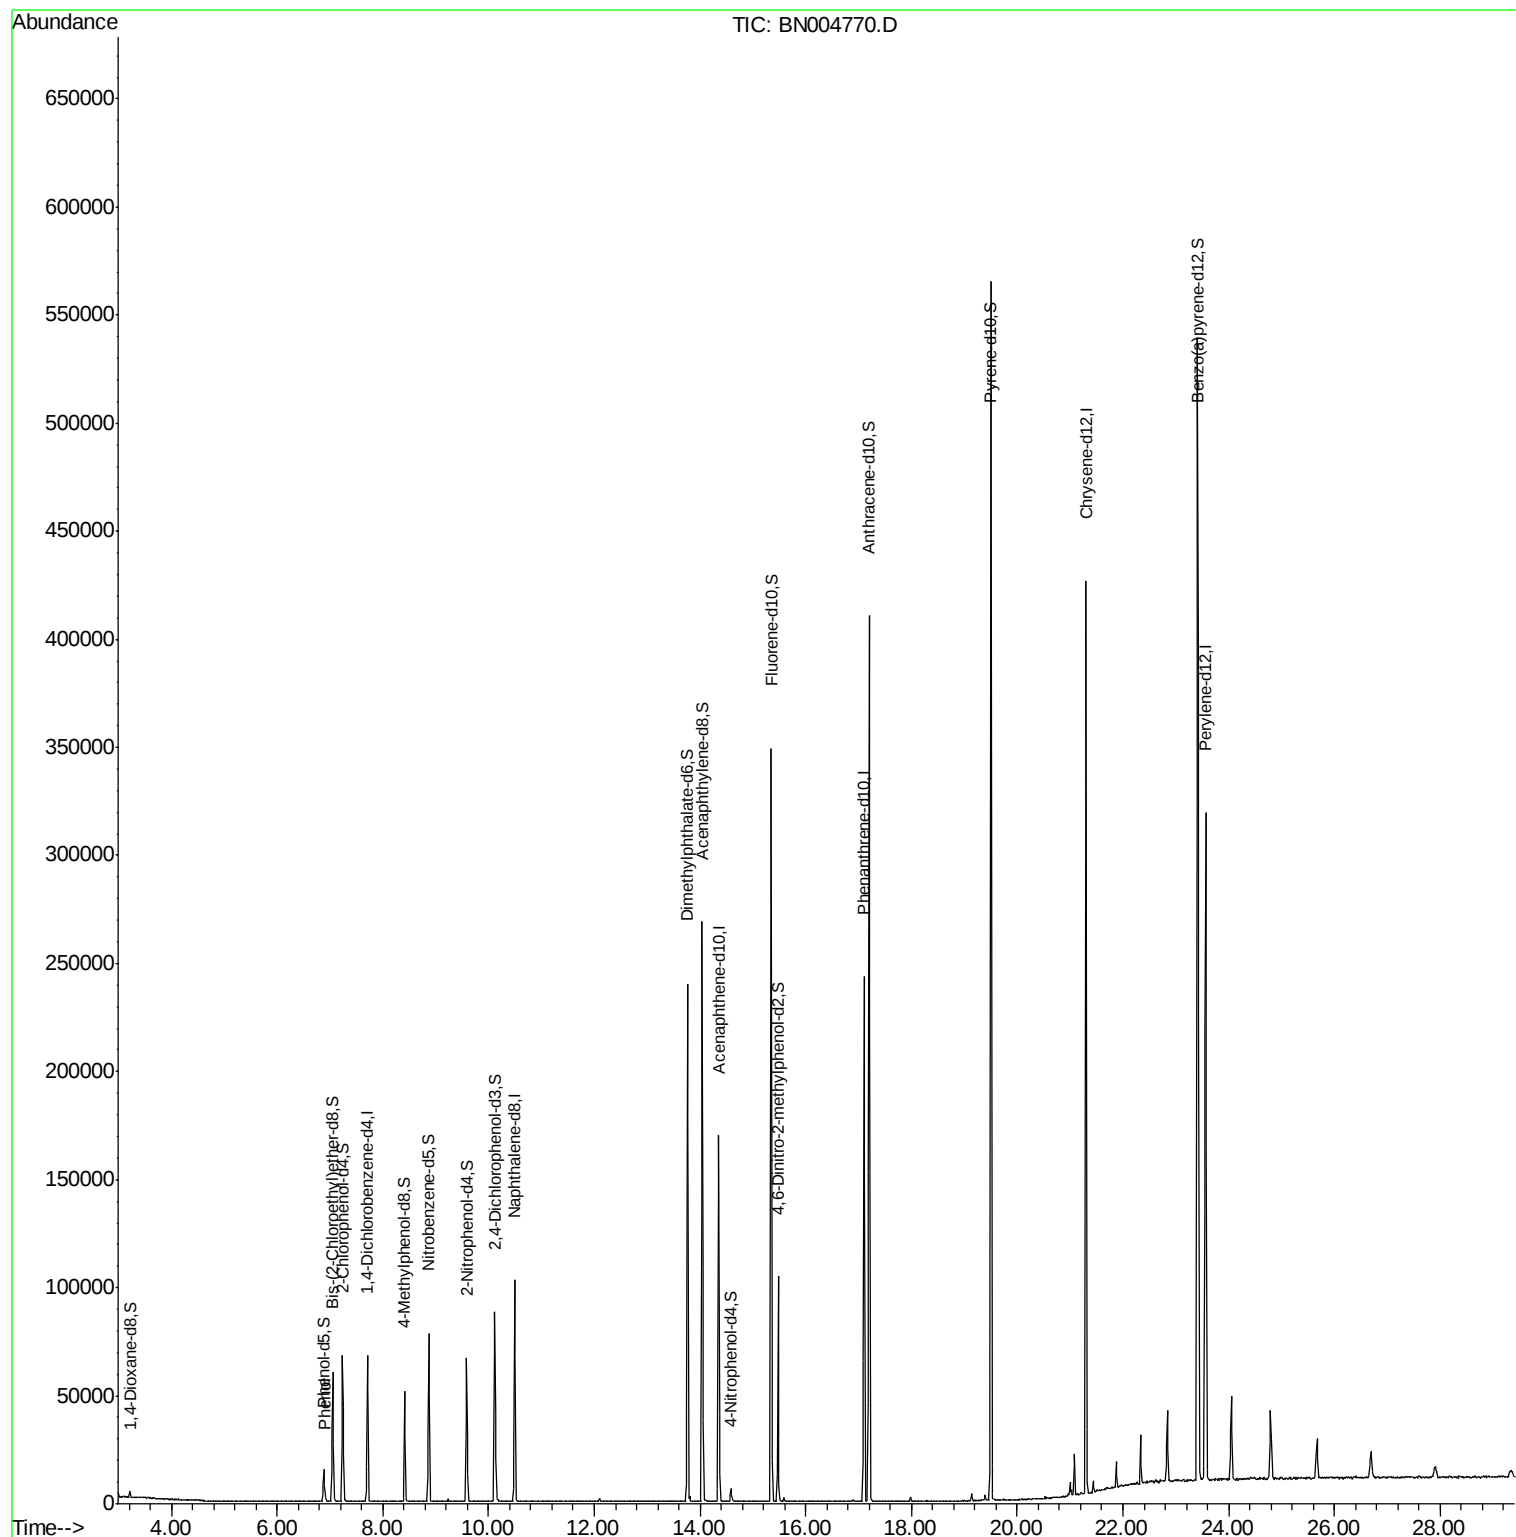

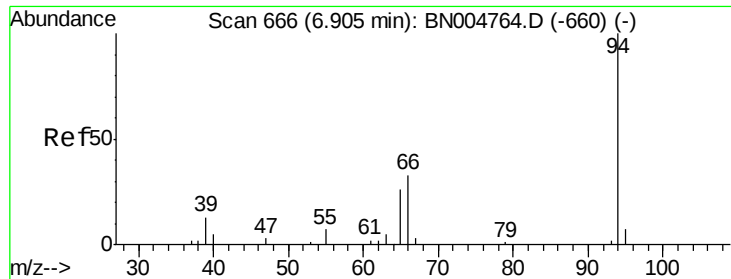

#6

Phenol

Concen: 1.492 ng/ul

RT: 6.90 min Scan# 666

Delta R.T. -0.01 min

Lab File: BN004770.D


Acq: 15 Mar 2019 14:27

Instrument :

BNA_N

ClientSampleId :

C09G8

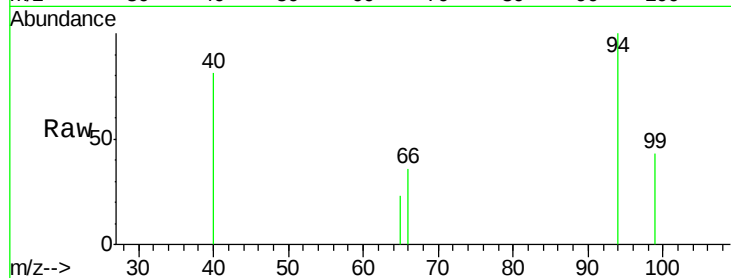


Tgt Ion: 94 Resp: 2566

Ion Ratio Lower Upper

94 100

65 22.9 20.2 30.4

66 35.5 28.2 42.2

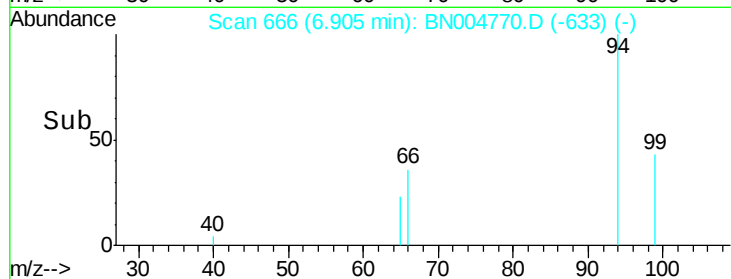

Abundance Ion 94.00 (93.70 to 94.70): BNC

Ion 65.00 (64.70 to 65.70): BNC

Ion 66.00 (65.70 to 66.70): BNC

