
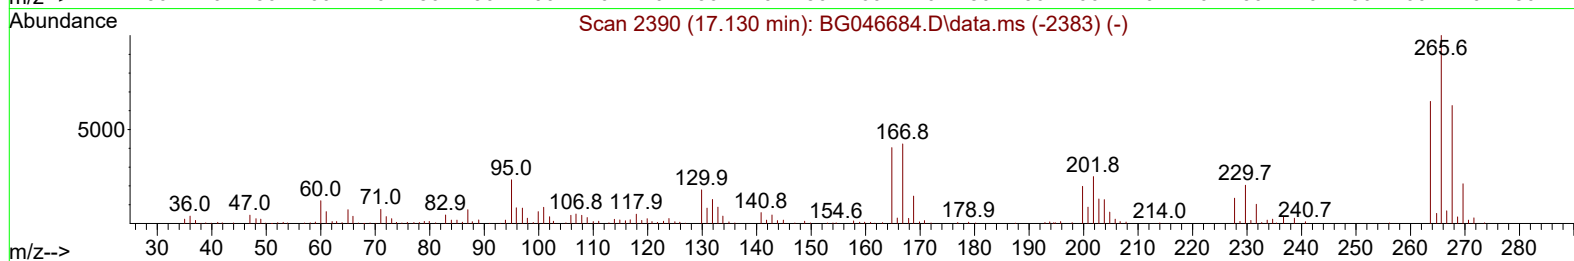
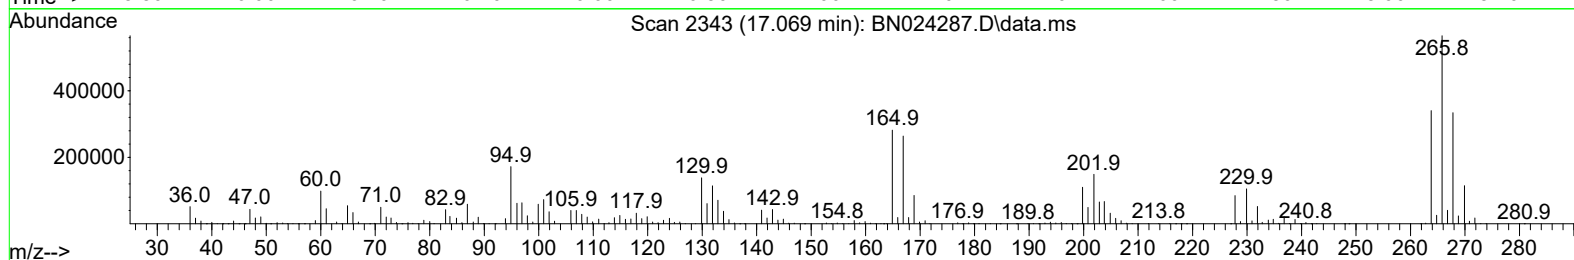


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031523\
Data File : BN024287.D
Acq On : 15 Mar 2023 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 01:58:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 16 01:58:07 2023
Response via : Initial Calibration

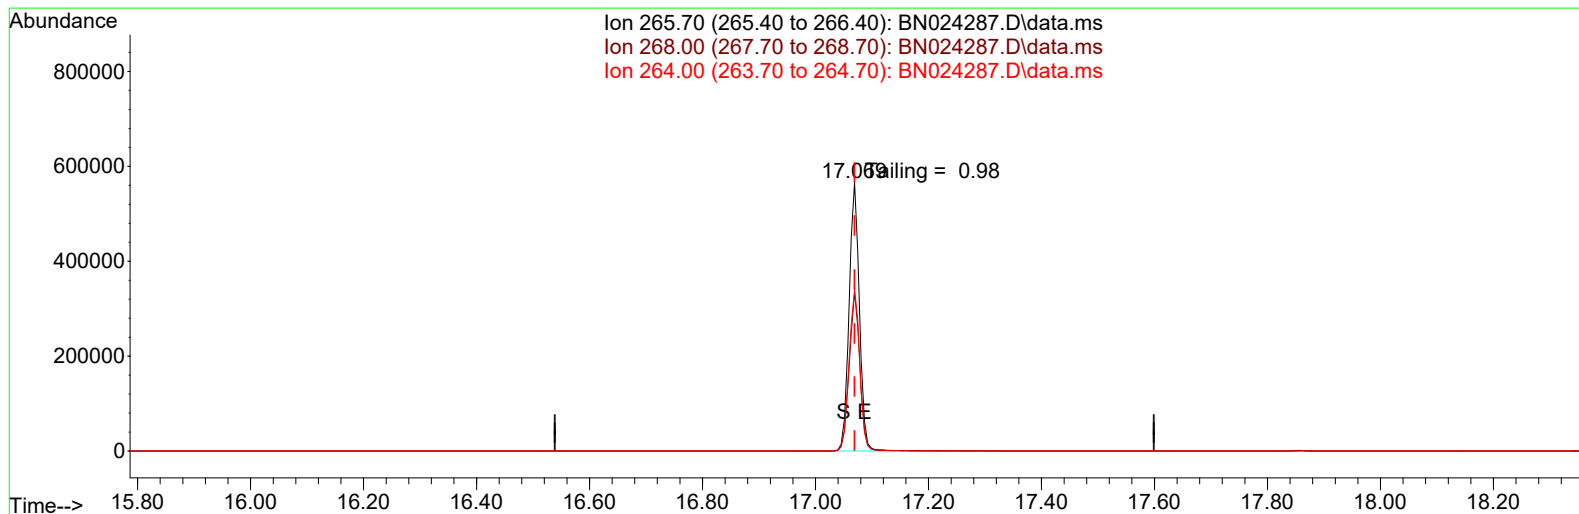

TIC: BN024287.D\data.ms

(70) Pentachlorophenol (C)




17.069min (0.000) 26963.79 ng

response 719457

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.09
264.00	61.60	60.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031523\
Data File : BN024287.D
Acq On : 15 Mar 2023 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 01:58:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 16 01:58:07 2023
Response via : Initial Calibration

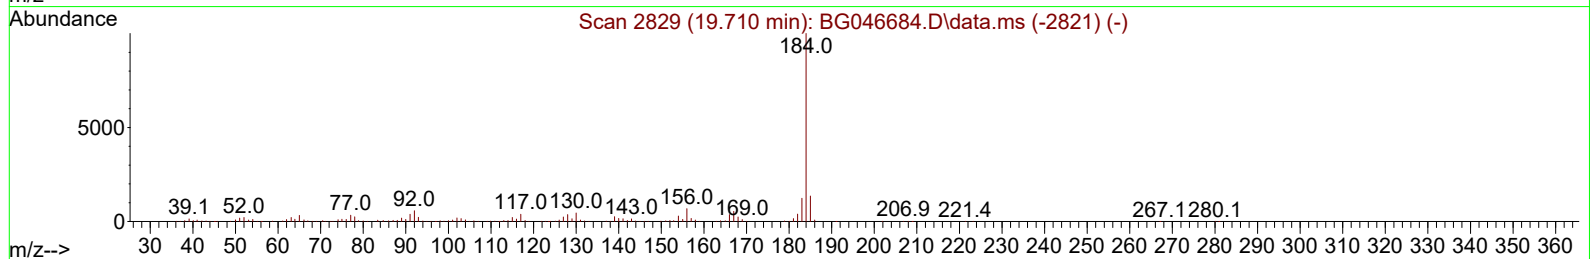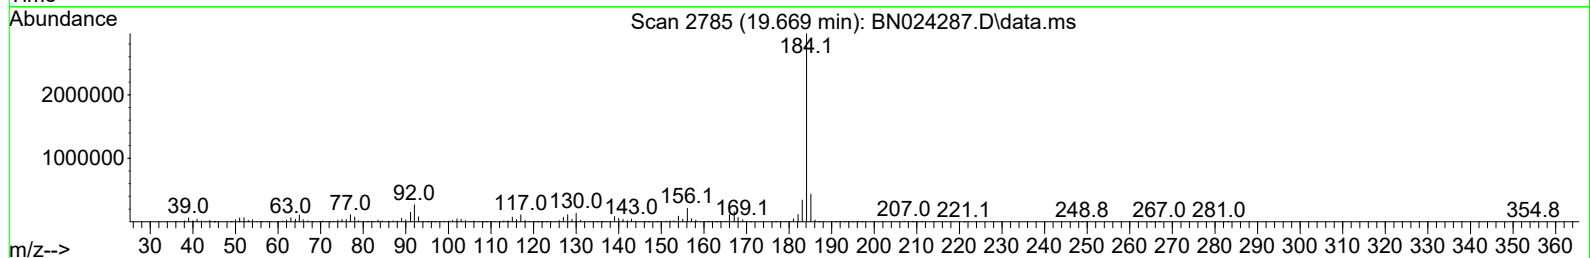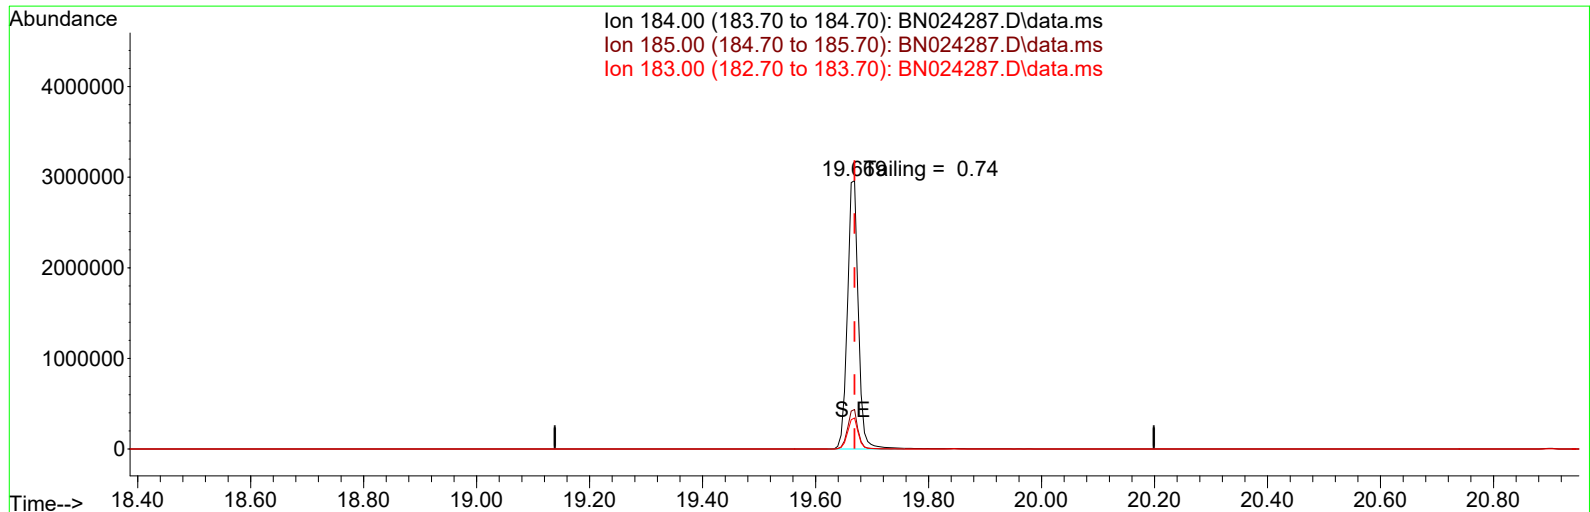

TIC: BN024287.D\data.ms

(77) Benzidine**19.669min (0.000) 2038956.86 ng****response 3959651**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.73
183.00	13.20	11.60
0.00	0.00	0.00