
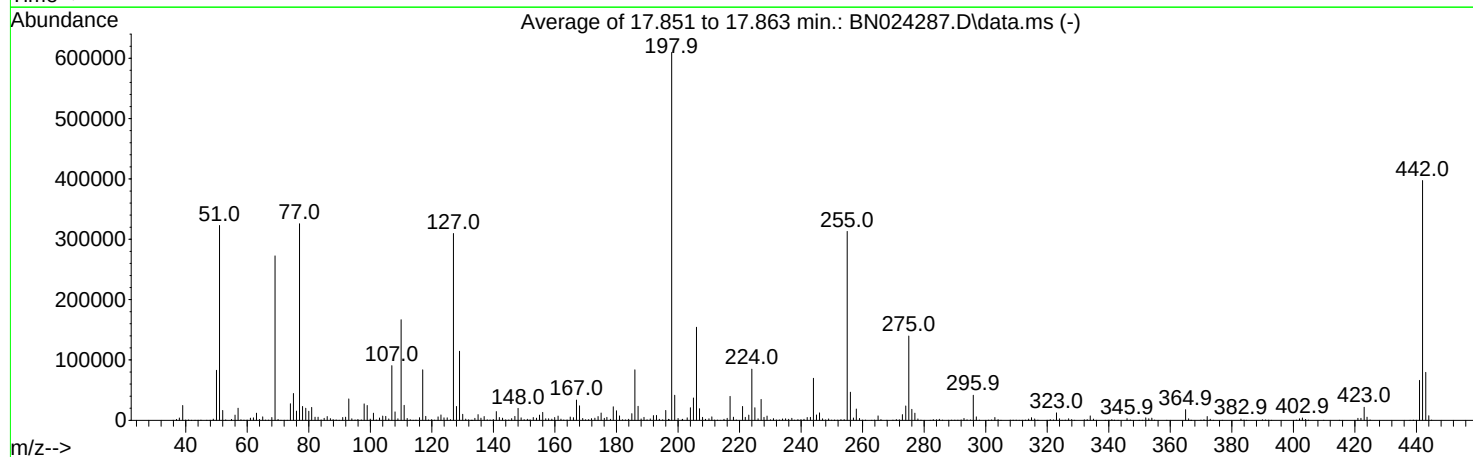


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031523\
 Data File : BN024287.D
 Acq On : 15 Mar 2023 10:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 16 01:06:57 2023

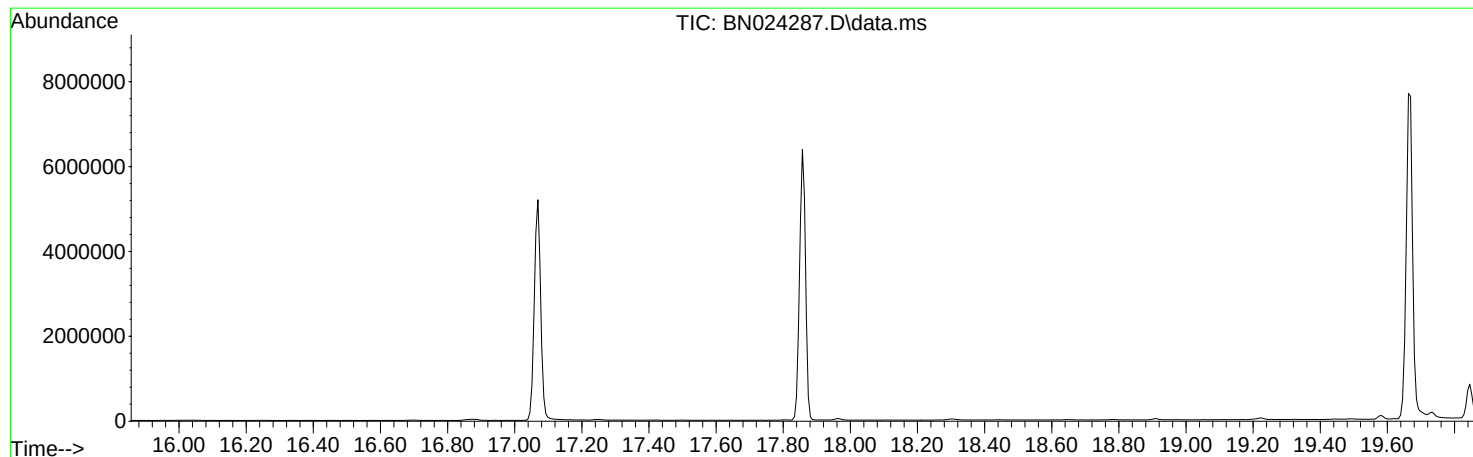




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.0	322909	PASS
68	69	0.00	2	1.7	4573	PASS
69	198	0.00	100	44.7	272533	PASS
70	69	0.00	2	0.6	1545	PASS
127	198	10	80	50.8	309568	PASS
197	198	0.00	2	0.3	1714	PASS
198	198	100	100	100.0	609685	PASS
199	198	5	9	6.8	41424	PASS
275	198	10	60	22.9	139691	PASS
365	198	1	100	2.9	17741	PASS
441	198	0.01	100	10.9	66219	PASS
442	442	50	100	100.0	397397	PASS
443	442	15	24	20.0	79493	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031523\
Data File : BN024287.D
Acq On : 15 Mar 2023 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 16 01:58:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 16 01:58:07 2023
Response via : Initial Calibration

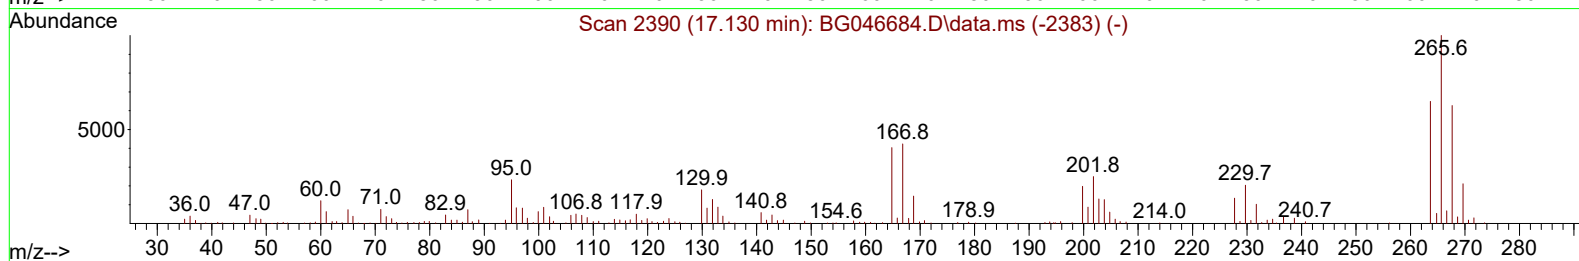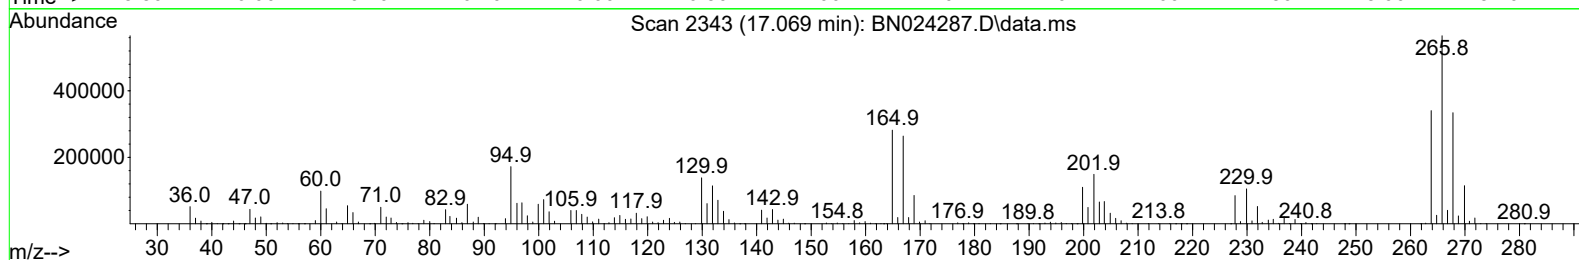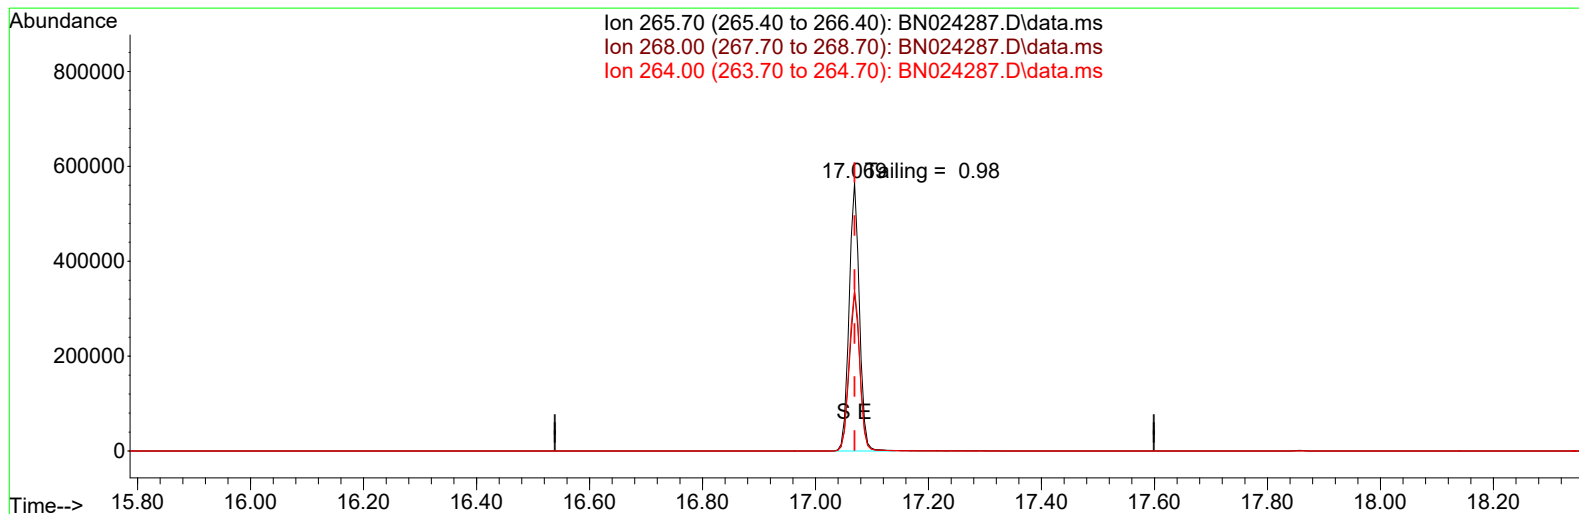

TIC: BN024287.D\data.ms

(70) Pentachlorophenol (C)

17.069min (0.000) 26963.79 ng




response 719457

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.09
264.00	61.60	60.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031523\
Data File : BN024287.D
Acq On : 15 Mar 2023 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 16 01:58:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 16 01:58:07 2023
Response via : Initial Calibration

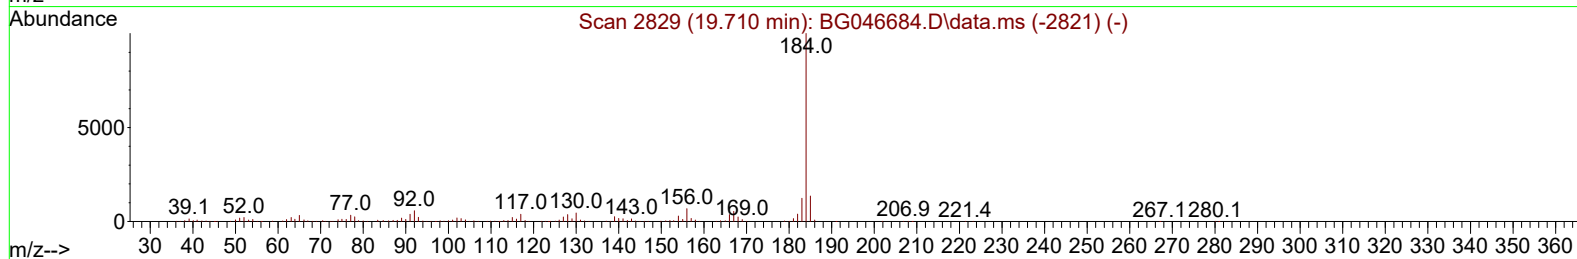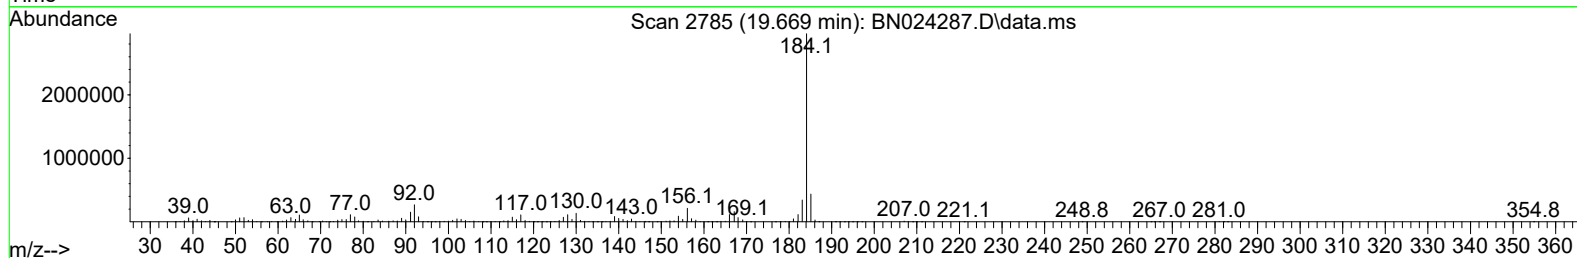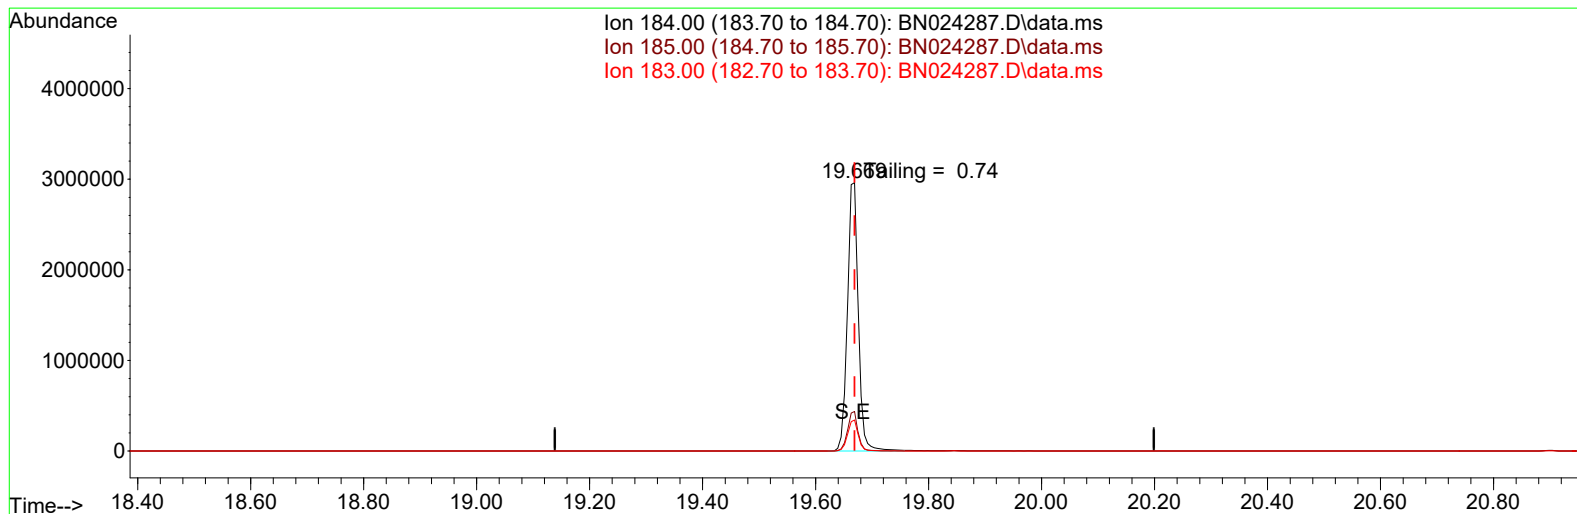

TIC: BN024287.D\data.ms

(77) Benzidine

19.669min (0.000) 2038956.86 ng

response 3959651

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.73
183.00	13.20	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/15/2023	BNA_N	<u>BN024287.D</u>
Compound Name	Response	Retention Time
DDT	1901066	20.898
DDD	34838	20.451
DDE	1654	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36492	1937558	1.88

Instrument :
BNA_N
ClientSampleId :
DFTPP