
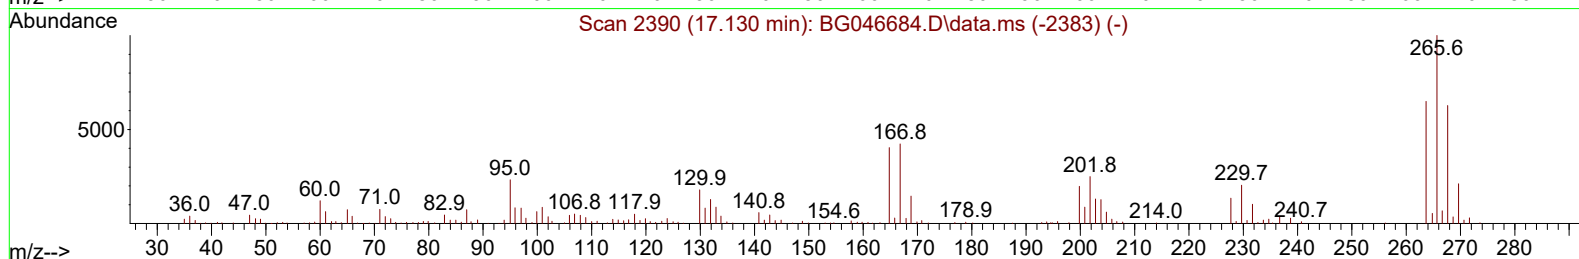
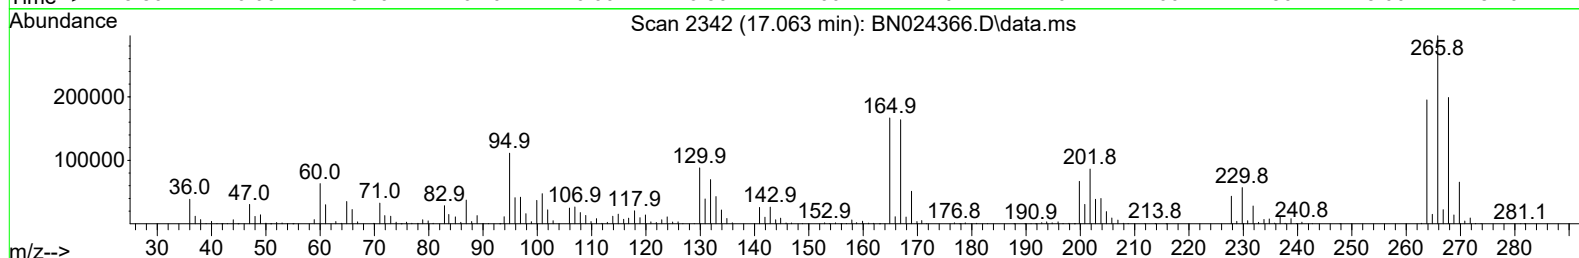


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
Data File : BN024366.D
Acq On : 18 Mar 2023 04:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 04:51:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 18 04:50:47 2023
Response via : Initial Calibration

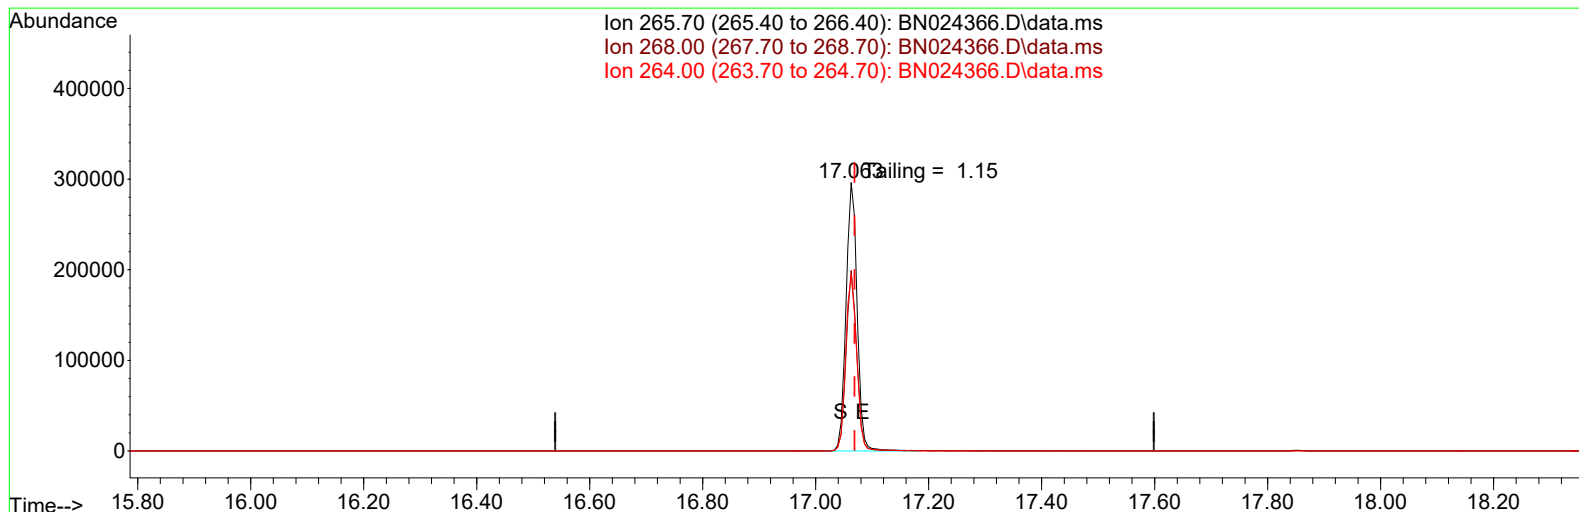

TIC: BN024366.D\data.ms

(70) Pentachlorophenol (C)




17.063min (-0.006) 21248.83 ng

response 405049

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.19
264.00	61.60	65.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
 Data File : BN024366.D
 Acq On : 18 Mar 2023 04:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 04:51:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 18 04:50:47 2023
 Response via : Initial Calibration

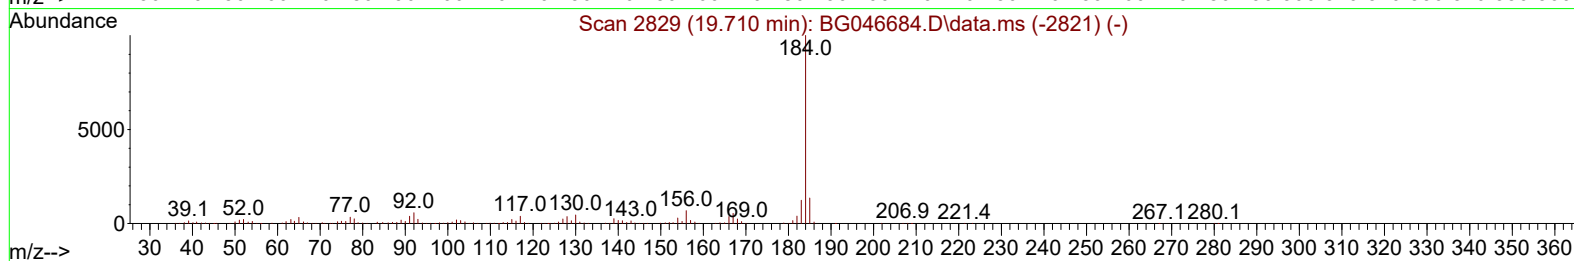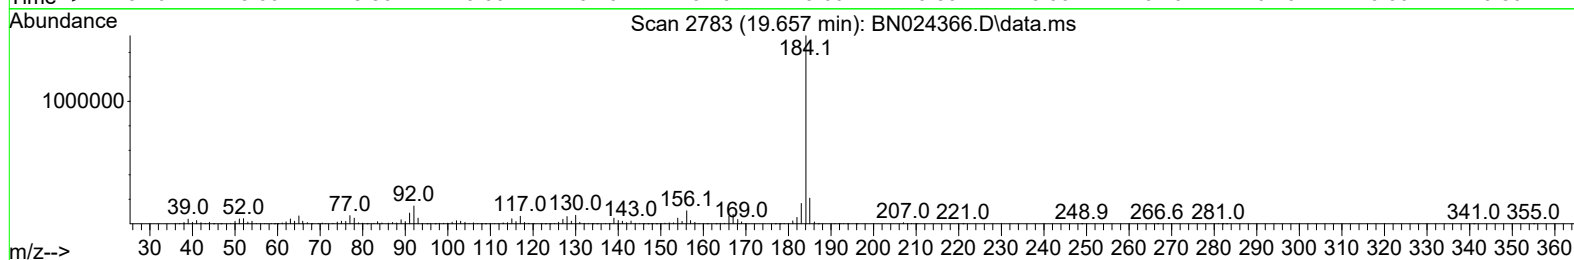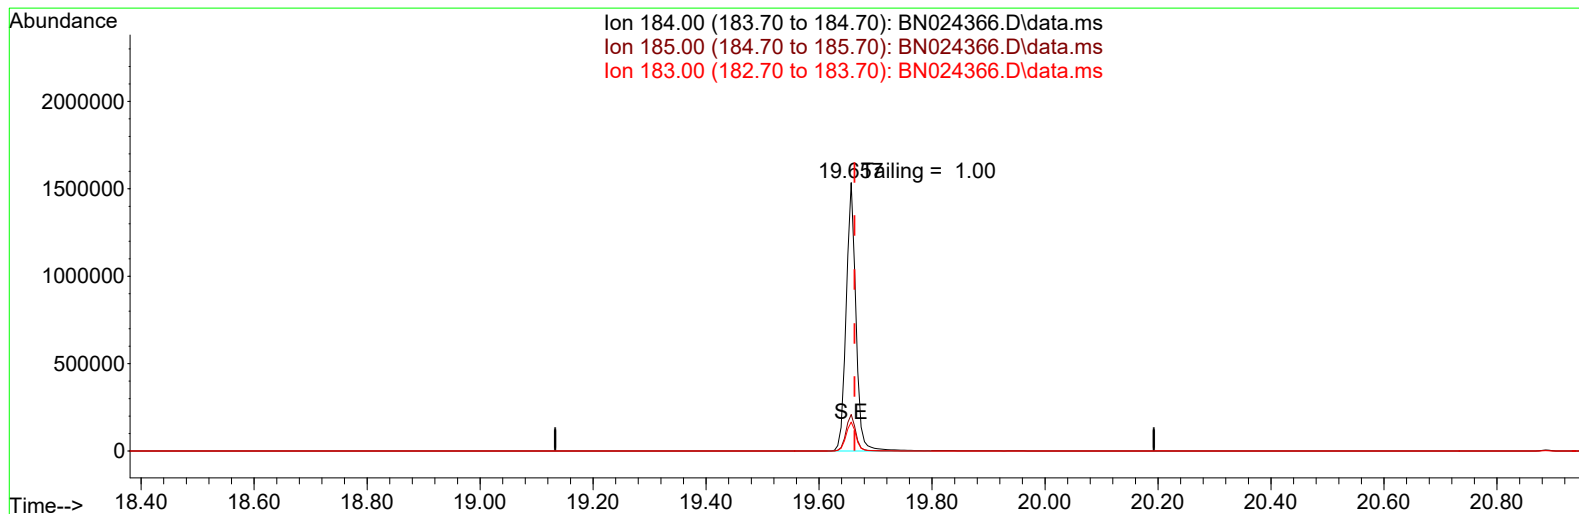

TIC: BN024366.D\data.ms

(77) Benzidine

19.657min (-0.006) 0.00 ng

response 1841886

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	10.83
0.00	0.00	0.00