
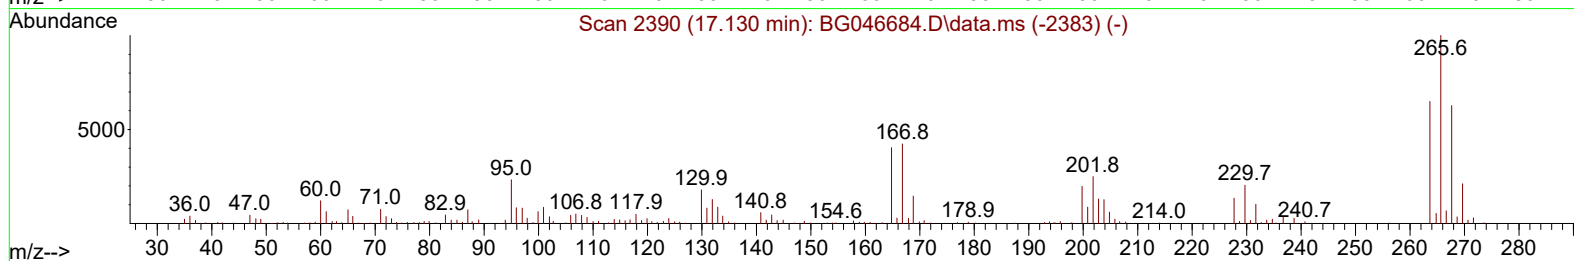
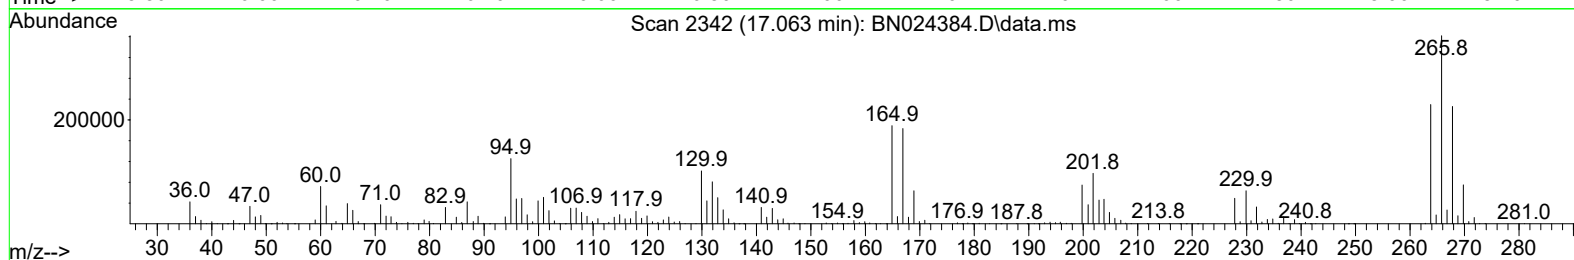


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
Data File : BN024384.D
Acq On : 18 Mar 2023 16:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Mar 20 02:11:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 02:11:29 2023
Response via : Initial Calibration

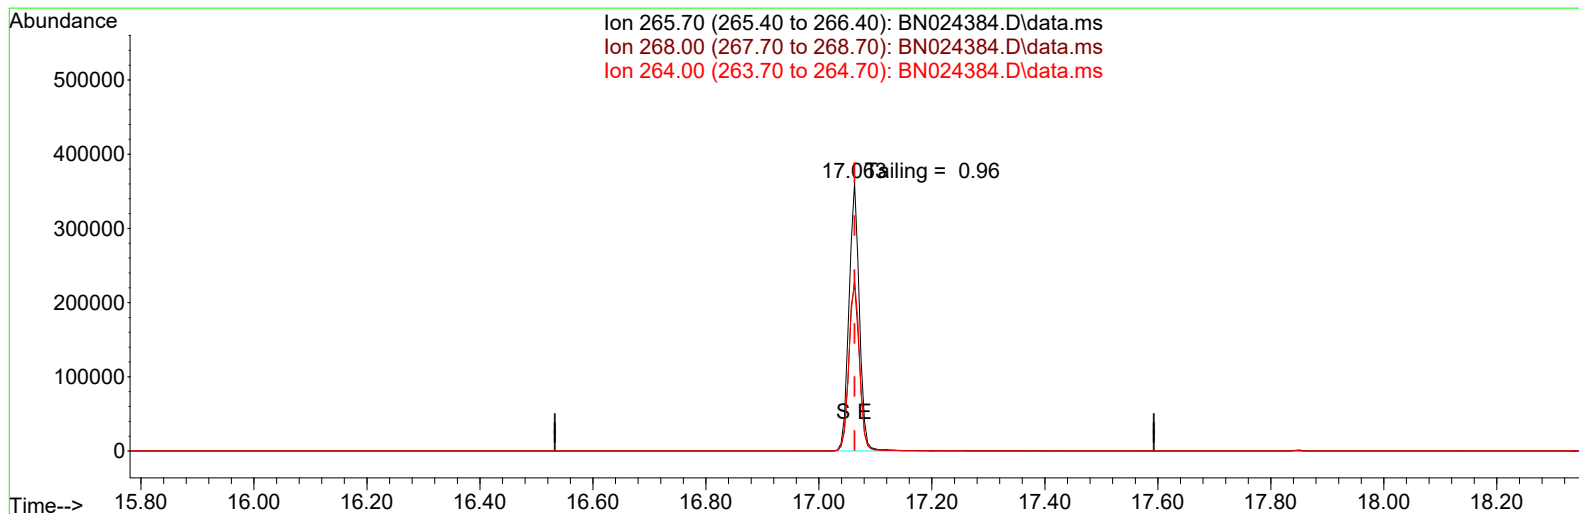

TIC: BN024384.D\data.ms

(70) Pentachlorophenol (C)




17.063min (0.000) 21258.01 ng

response 464281

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.37
264.00	61.60	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
Data File : BN024384.D
Acq On : 18 Mar 2023 16:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Mar 20 02:11:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 02:11:29 2023
Response via : Initial Calibration

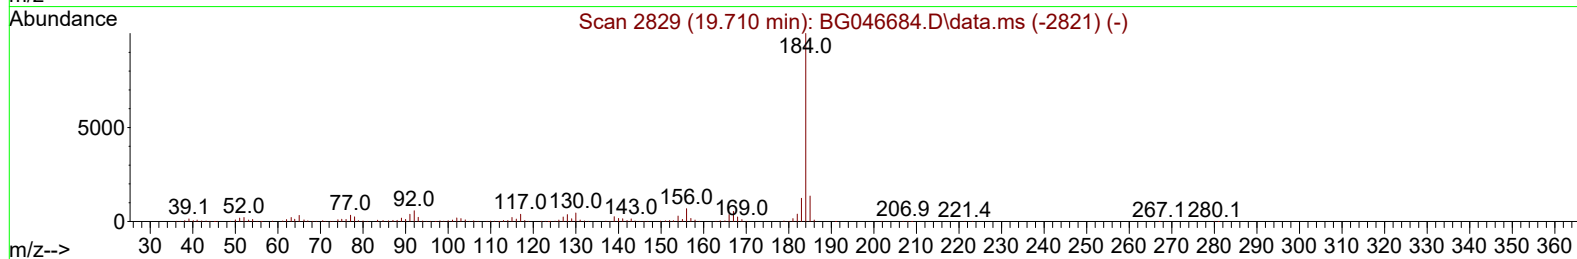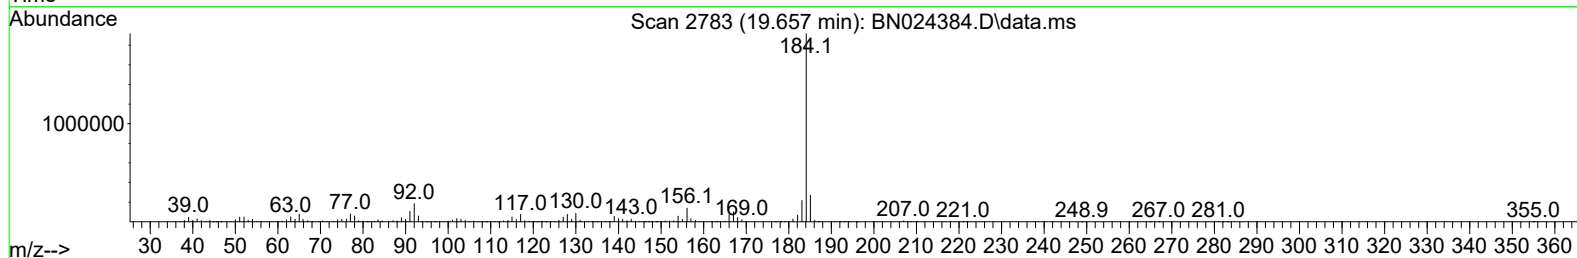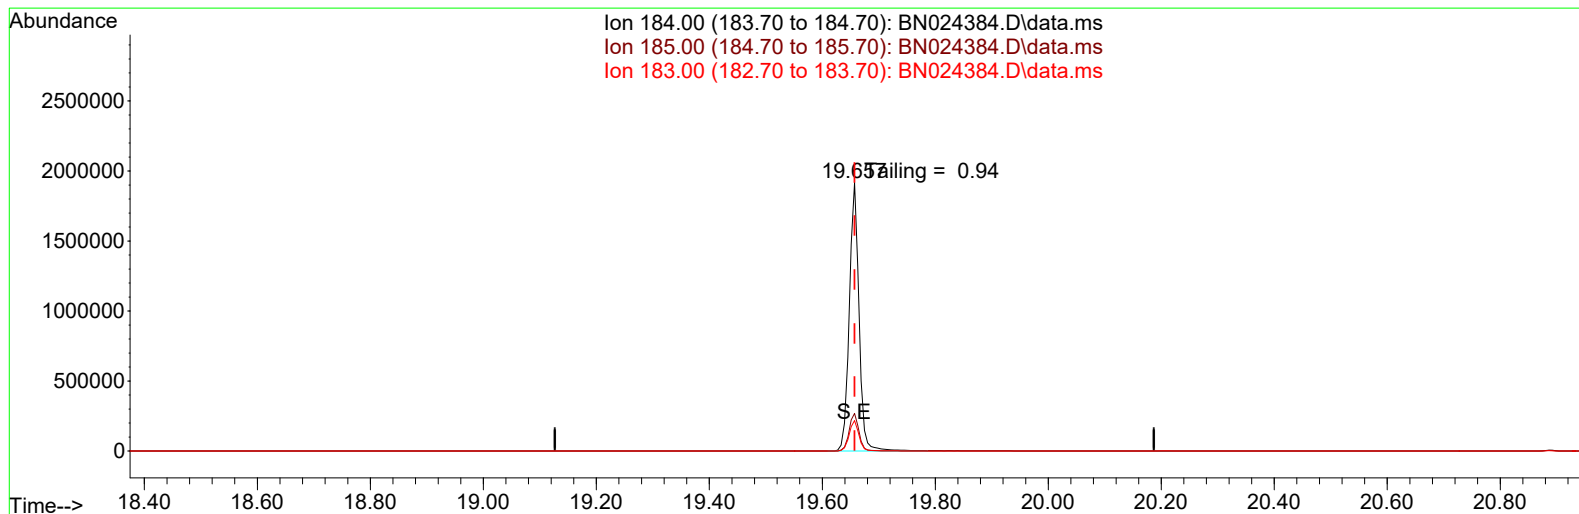

TIC: BN024384.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 2303421

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	11.35
0.00	0.00	0.00