
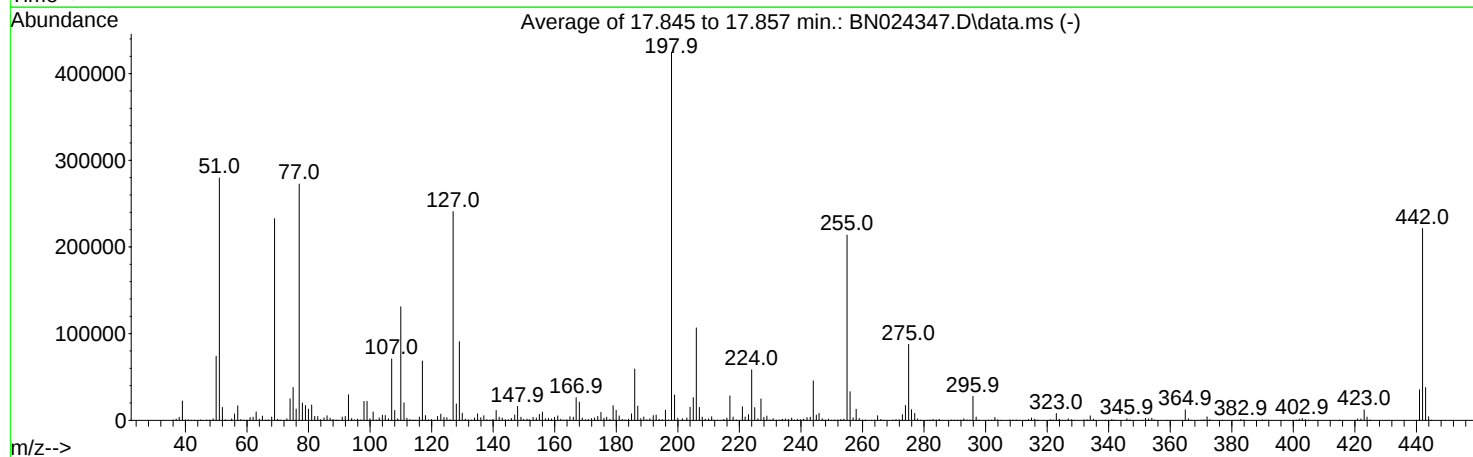


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
 Data File : BN024347.D
 Acq On : 17 Mar 2023 15:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 18 05:49:08 2023

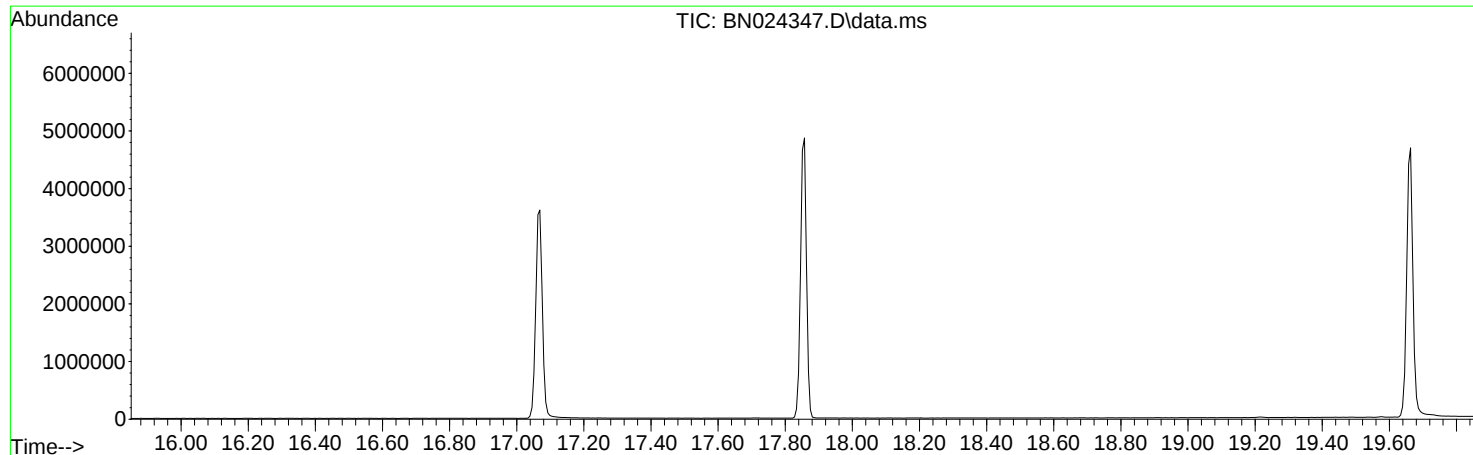




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.9	279552	PASS
68	69	0.00	2	1.7	3876	PASS
69	198	0.00	100	54.8	232661	PASS
70	69	0.00	2	0.5	1231	PASS
127	198	10	80	56.7	240853	PASS
197	198	0.00	2	0.1	429	PASS
198	198	100	100	100.0	424448	PASS
199	198	5	9	6.9	29355	PASS
275	198	10	60	20.7	87693	PASS
365	198	1	100	2.8	12048	PASS
441	198	0.01	100	8.3	35432	PASS
442	442	50	100	100.0	221269	PASS
443	442	15	24	17.1	37851	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
 Data File : BN024347.D
 Acq On : 17 Mar 2023 15:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 18 04:50:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 18 04:50:47 2023
 Response via : Initial Calibration

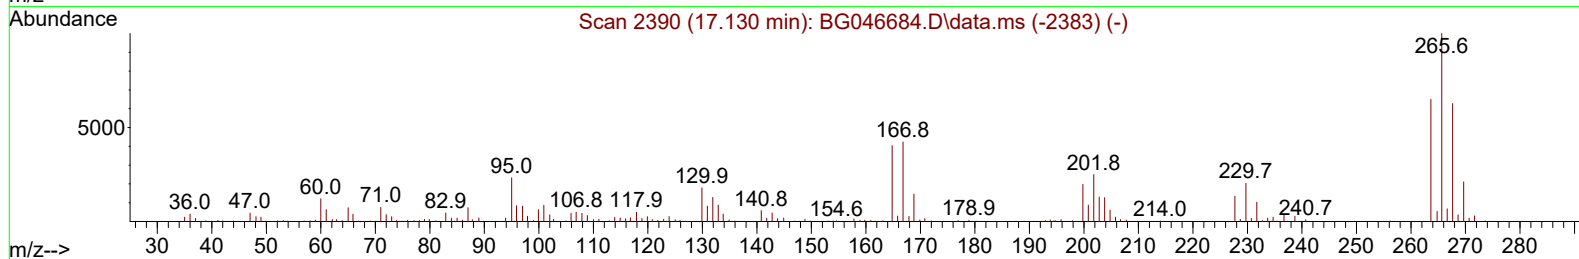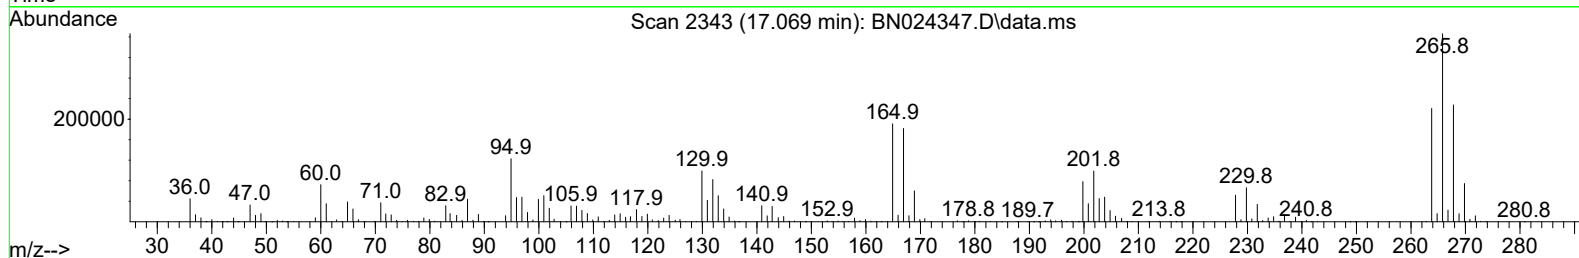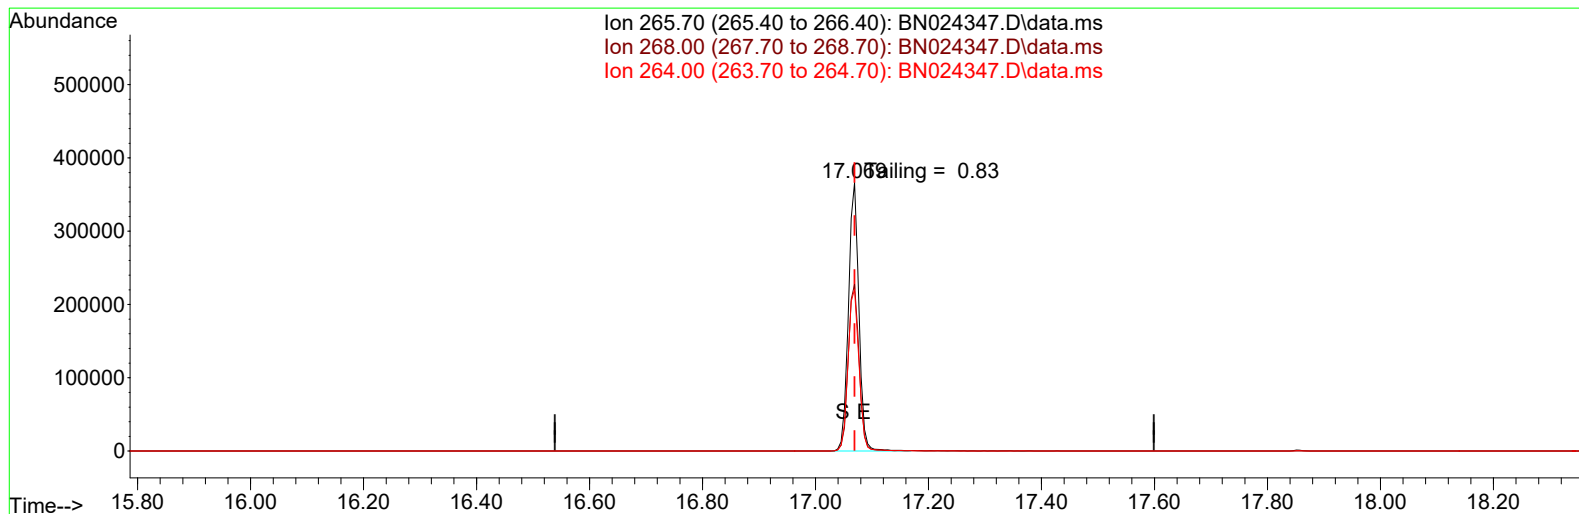

TIC: BN024347.D\data.ms

(70) Pentachlorophenol (C)

17.069min (0.000) 21114.59 ng




response 472582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.14
264.00	61.60	60.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
 Data File : BN024347.D
 Acq On : 17 Mar 2023 15:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 18 04:50:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 18 04:50:47 2023
 Response via : Initial Calibration

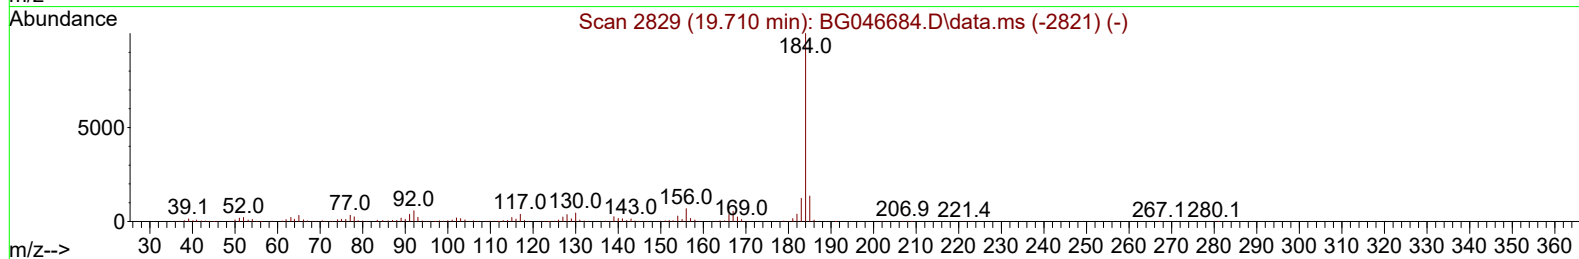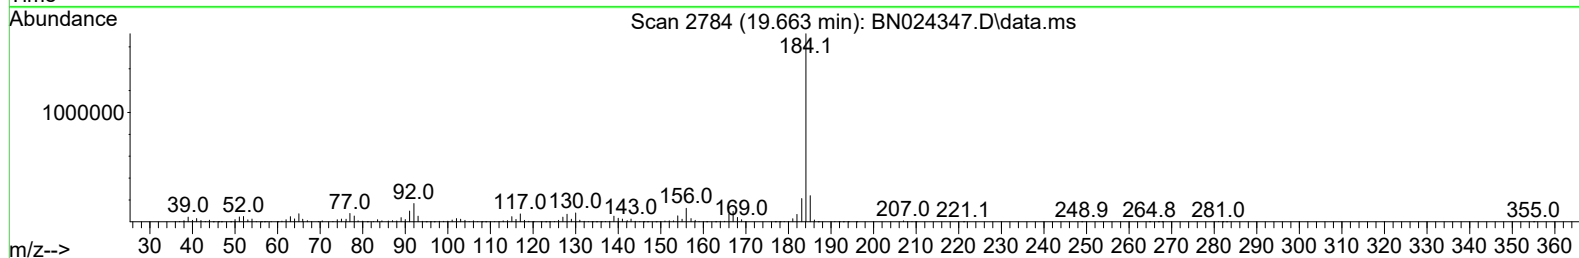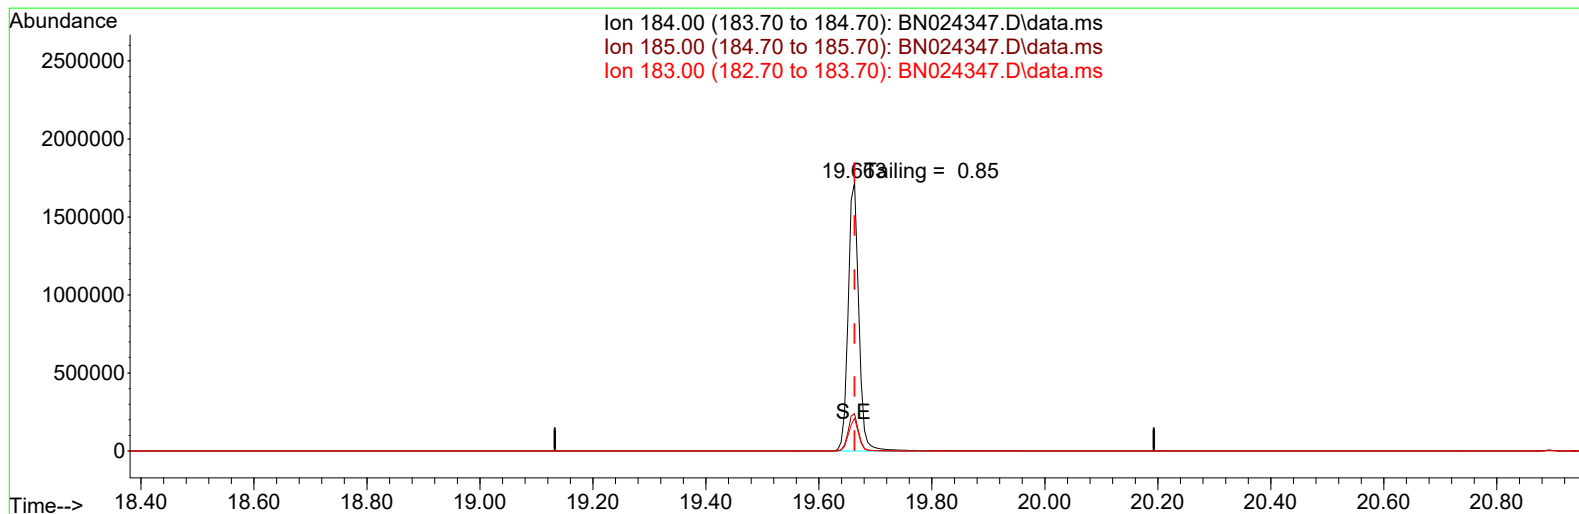

TIC: BN024347.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 2268701

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2023	BNA_N	<u>BN024347.D</u>
Compound Name	Response	Retention Time
DDT	1294088	20.892
DDD	22837	20.451
DDE	1280	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24117	1318205	1.83

Instrument :
BNA_N
ClientSampleId :
DFTPP