
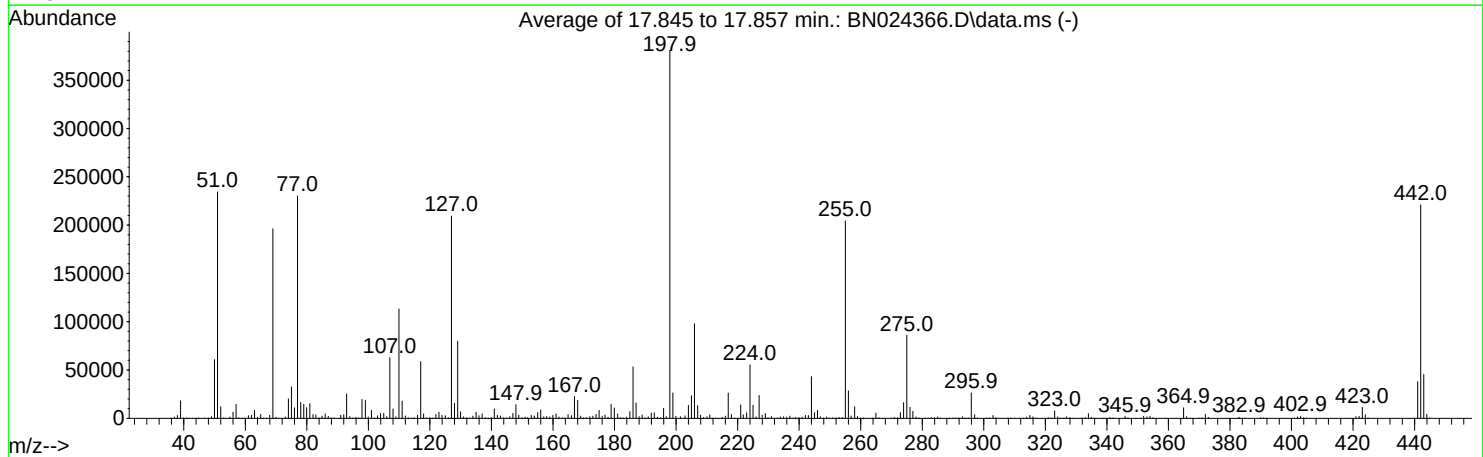


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
 Data File : BN024366.D
 Acq On : 18 Mar 2023 04:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 18 05:49:08 2023

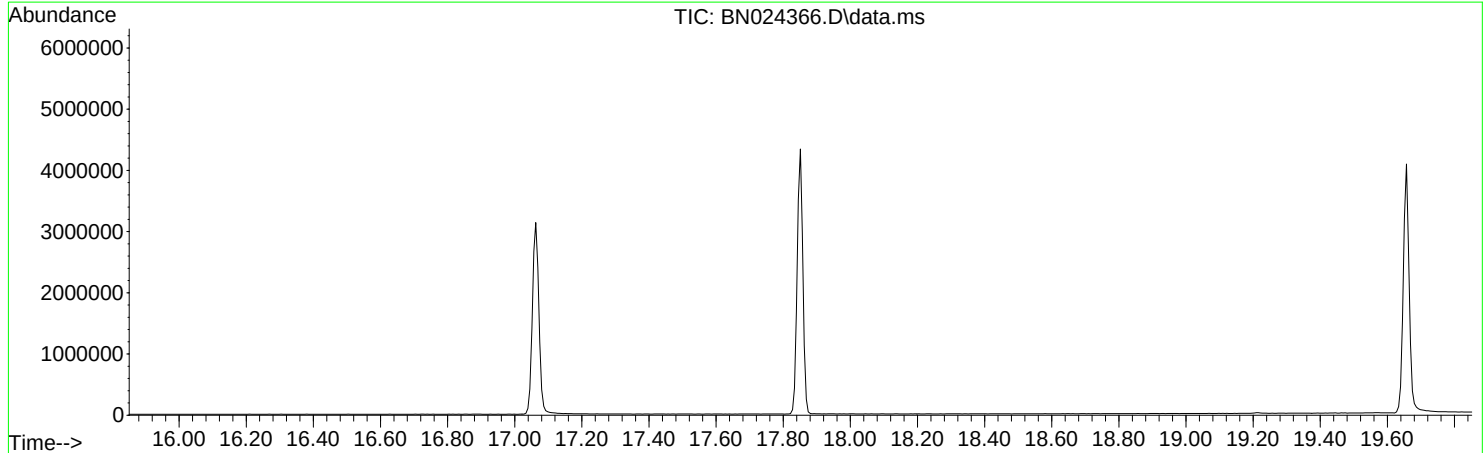




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.5	234389	PASS
68	69	0.00	2	1.6	3157	PASS
69	198	0.00	100	51.5	196309	PASS
70	69	0.00	2	0.5	1012	PASS
127	198	10	80	55.0	209408	PASS
197	198	0.00	2	0.5	1778	PASS
198	198	100	100	100.0	380885	PASS
199	198	5	9	6.9	26328	PASS
275	198	10	60	22.5	85829	PASS
365	198	1	100	2.8	10821	PASS
441	198	0.01	100	9.9	37816	PASS
442	442	50	100	100.0	220864	PASS
443	442	15	24	20.5	45381	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
 Data File : BN024366.D
 Acq On : 18 Mar 2023 04:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 18 04:51:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 18 04:50:47 2023
 Response via : Initial Calibration

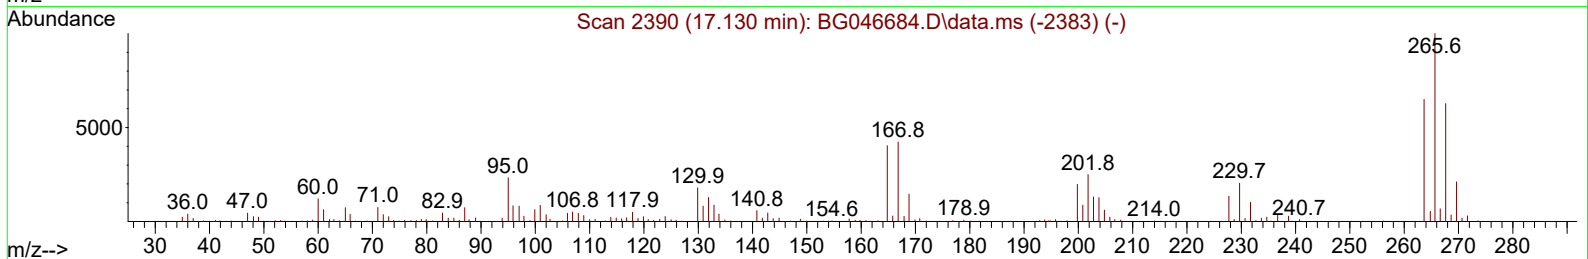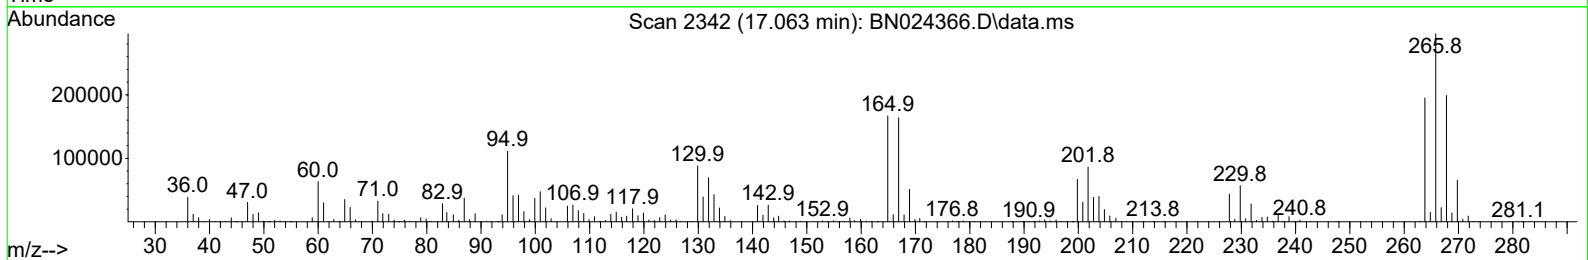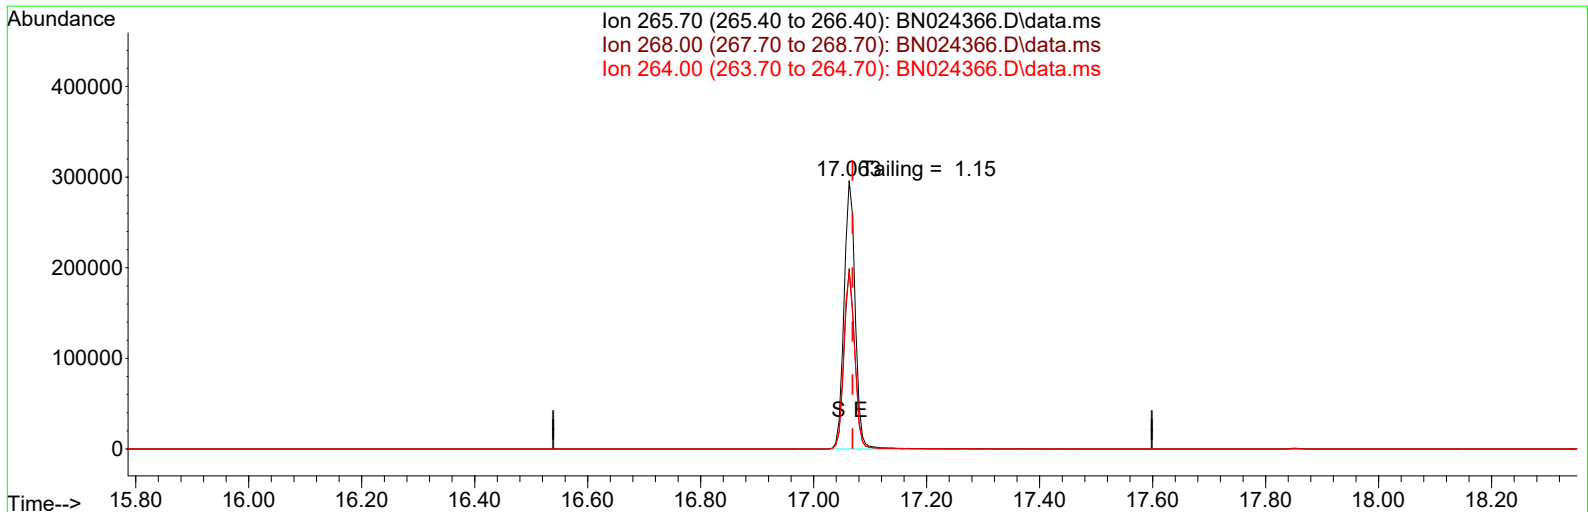

TIC: BN024366.D\data.ms

(70) Pentachlorophenol (C)

17.063min (-0.006) 21248.83 ng




response 405049

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.19
264.00	61.60	65.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031723\
 Data File : BN024366.D
 Acq On : 18 Mar 2023 04:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 18 04:51:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 18 04:50:47 2023
 Response via : Initial Calibration

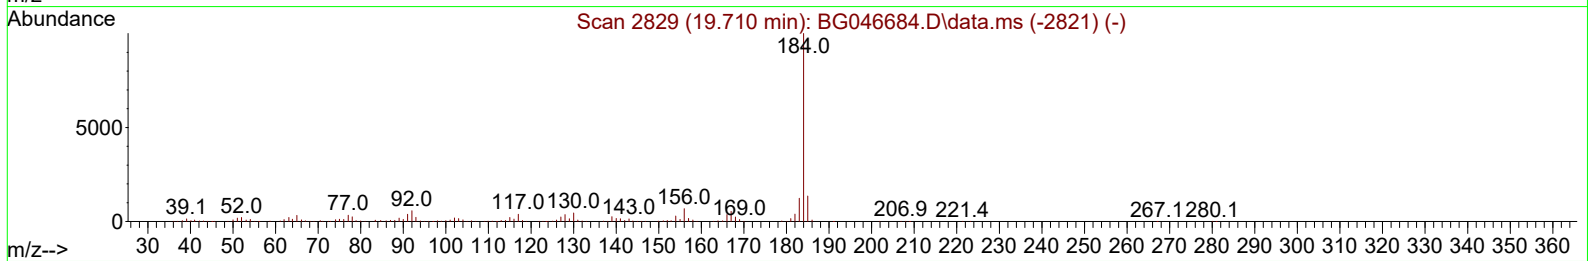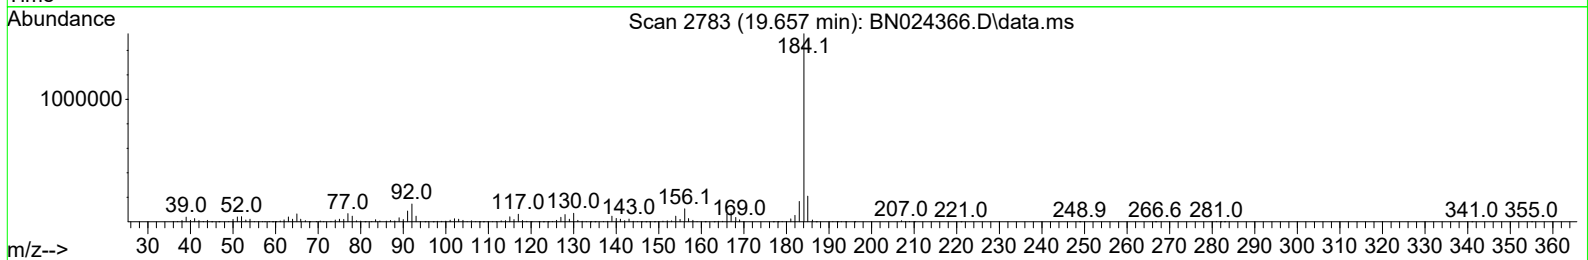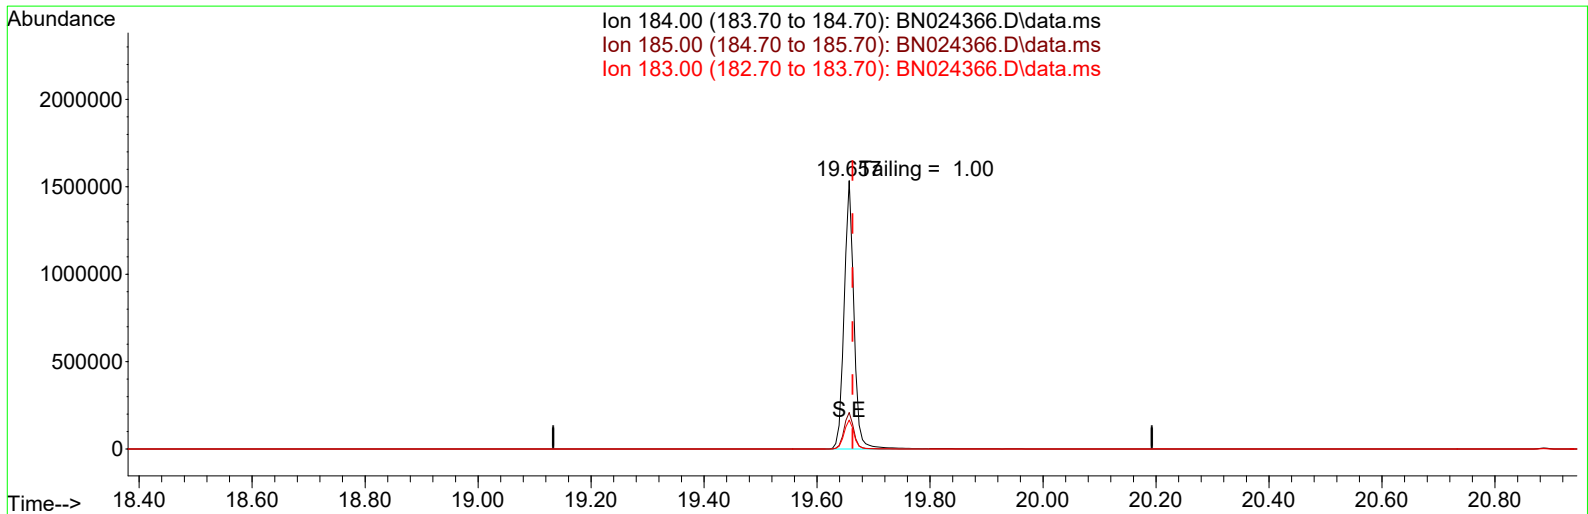

TIC: BN024366.D\data.ms

(77) Benzidine

19.657min (-0.006) 0.00 ng

response 1841886

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	10.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2023	BNA_N	<u>BN024366.D</u>
Compound Name	Response	Retention Time
DDT	1110661	20.886
DDD	23190	20.445
DDE	1861	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25051	1135712	2.21

Instrument :
BNA_N
ClientSampleId :
DFTPP