

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031819\
 Data File : BN004810.D
 Acq On : 18 Mar 2019 22:39
 Operator : JU/SJ
 Sample : K1920-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C09H3

Quant Time: Mar 19 00:40:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 15 04:01:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	30560	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.49	136	135215	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.35	164	81954	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.10	188	195715	20.00	ng/ul	-0.01
78) Chrysene-d12	21.30	240	241627	20.00	ng/ul	-0.02
86) Perylene-d12	23.56	264	235290	20.00	ng/ul	-0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	1901	3.51	ng/uL	-0.01
5) Phenol-d5	6.88	99	14149	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	32352	24.56	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.24	132	48461	22.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	29091	13.25	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	28908	28.04	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.59	143	33487	28.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	56705	25.41	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.65	131	4942	1.85	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	196277	27.70	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	240802	28.23	ng/ul	0.00
52) 4-Nitrophenol-d4	14.57	143	3813	2.90	ng/ul	0.00
58) Fluorene-d10	15.35	176	174117	28.91	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.47	200	31368	23.22	ng/ul	0.00
71) Anthracene-d10	17.20	188	284595	29.85	ng/ul	-0.01
79) Pyrene-d10	19.50	212	338084	28.64	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.41	264	345209	27.32	ng/ul	-0.02


Target Compounds					Ovalue	
45) Dimethylphthalate	13.80	163	9831	1.414	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031819\
Data File : BN004810.D
Acq On : 18 Mar 2019 22:39
Operator : JU/SJ
Sample : K1920-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C09H3

Quant Time: Mar 19 00:40:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 15 04:01:10 2019
Response via : Initial Calibration

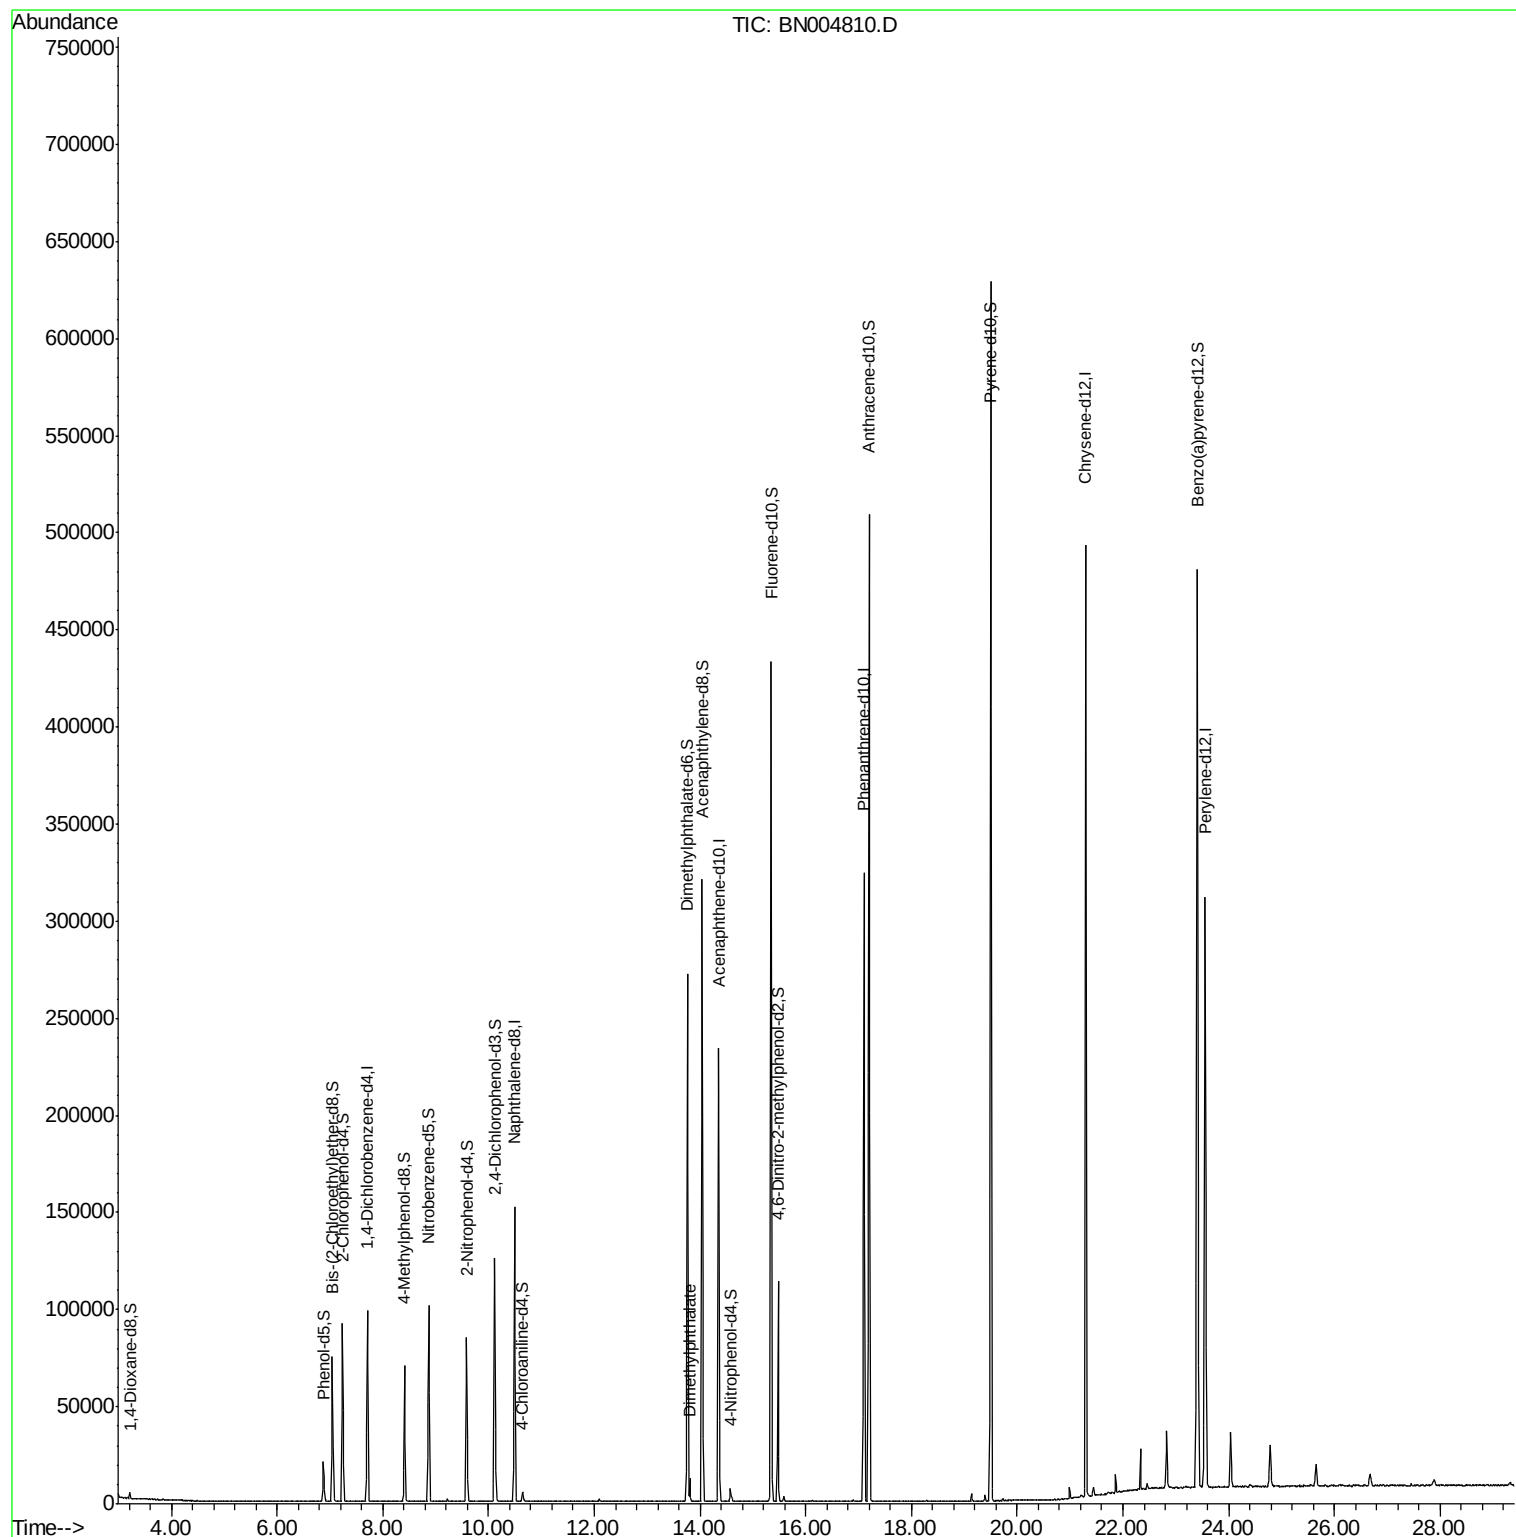

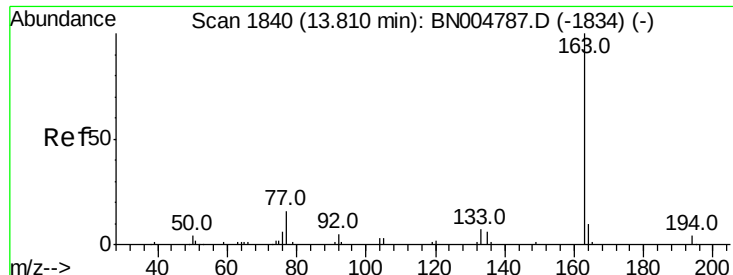

#45

Dimethylphthalate

Concen: 1.414 ng/ul

RT: 13.80 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BN004810.D

Acq: 18 Mar 2019 22:39

Instrument :

BNA_N

ClientSampleId :

C09H3


Tot Ion:163 Resp: 9831

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.2

164 9.8 7.9 11.9

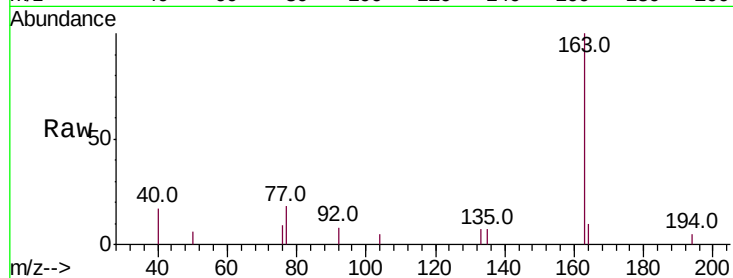

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

