

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031819\
 Data File : BN004805.D
 Acq On : 18 Mar 2019 19:43
 Operator : JU/SJ
 Sample : K1920-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C09B5

Quant Time: Mar 19 00:40:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 15 04:01:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	26698	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	117337	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.35	164	71469	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.10	188	170489	20.00	ng/ul	-0.01
78) Chrysene-d12	21.30	240	220965	20.00	ng/ul	-0.02
86) Perylene-d12	23.55	264	248473	20.00	ng/ul	-0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	1744	3.68	ng/uL	0.00
5) Phenol-d5	6.88	99	8674	3.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	21383	18.58	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.24	132	31213	16.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	18234	9.50	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	18381	20.55	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.59	143	20877	20.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	35350	18.26	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.65	131	1866	0.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	129717	20.99	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	155765	20.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	1894	1.65	ng/ul	0.00
58) Fluorene-d10	15.35	176	115822	22.05	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.47	200	17740	15.07	ng/ul	0.00
71) Anthracene-d10	17.20	188	190758	22.97	ng/ul	-0.01
79) Pyrene-d10	19.50	212	230081	21.31	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.41	264	273299	20.48	ng/ul	-0.02


Target Compounds					Ovalue	
45) Dimethylphthalate	13.81	163	11082	1.828	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031819\
Data File : BN004805.D
Acq On : 18 Mar 2019 19:43
Operator : JU/SJ
Sample : K1920-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C09B5

Quant Time: Mar 19 00:40:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 15 04:01:10 2019
Response via : Initial Calibration

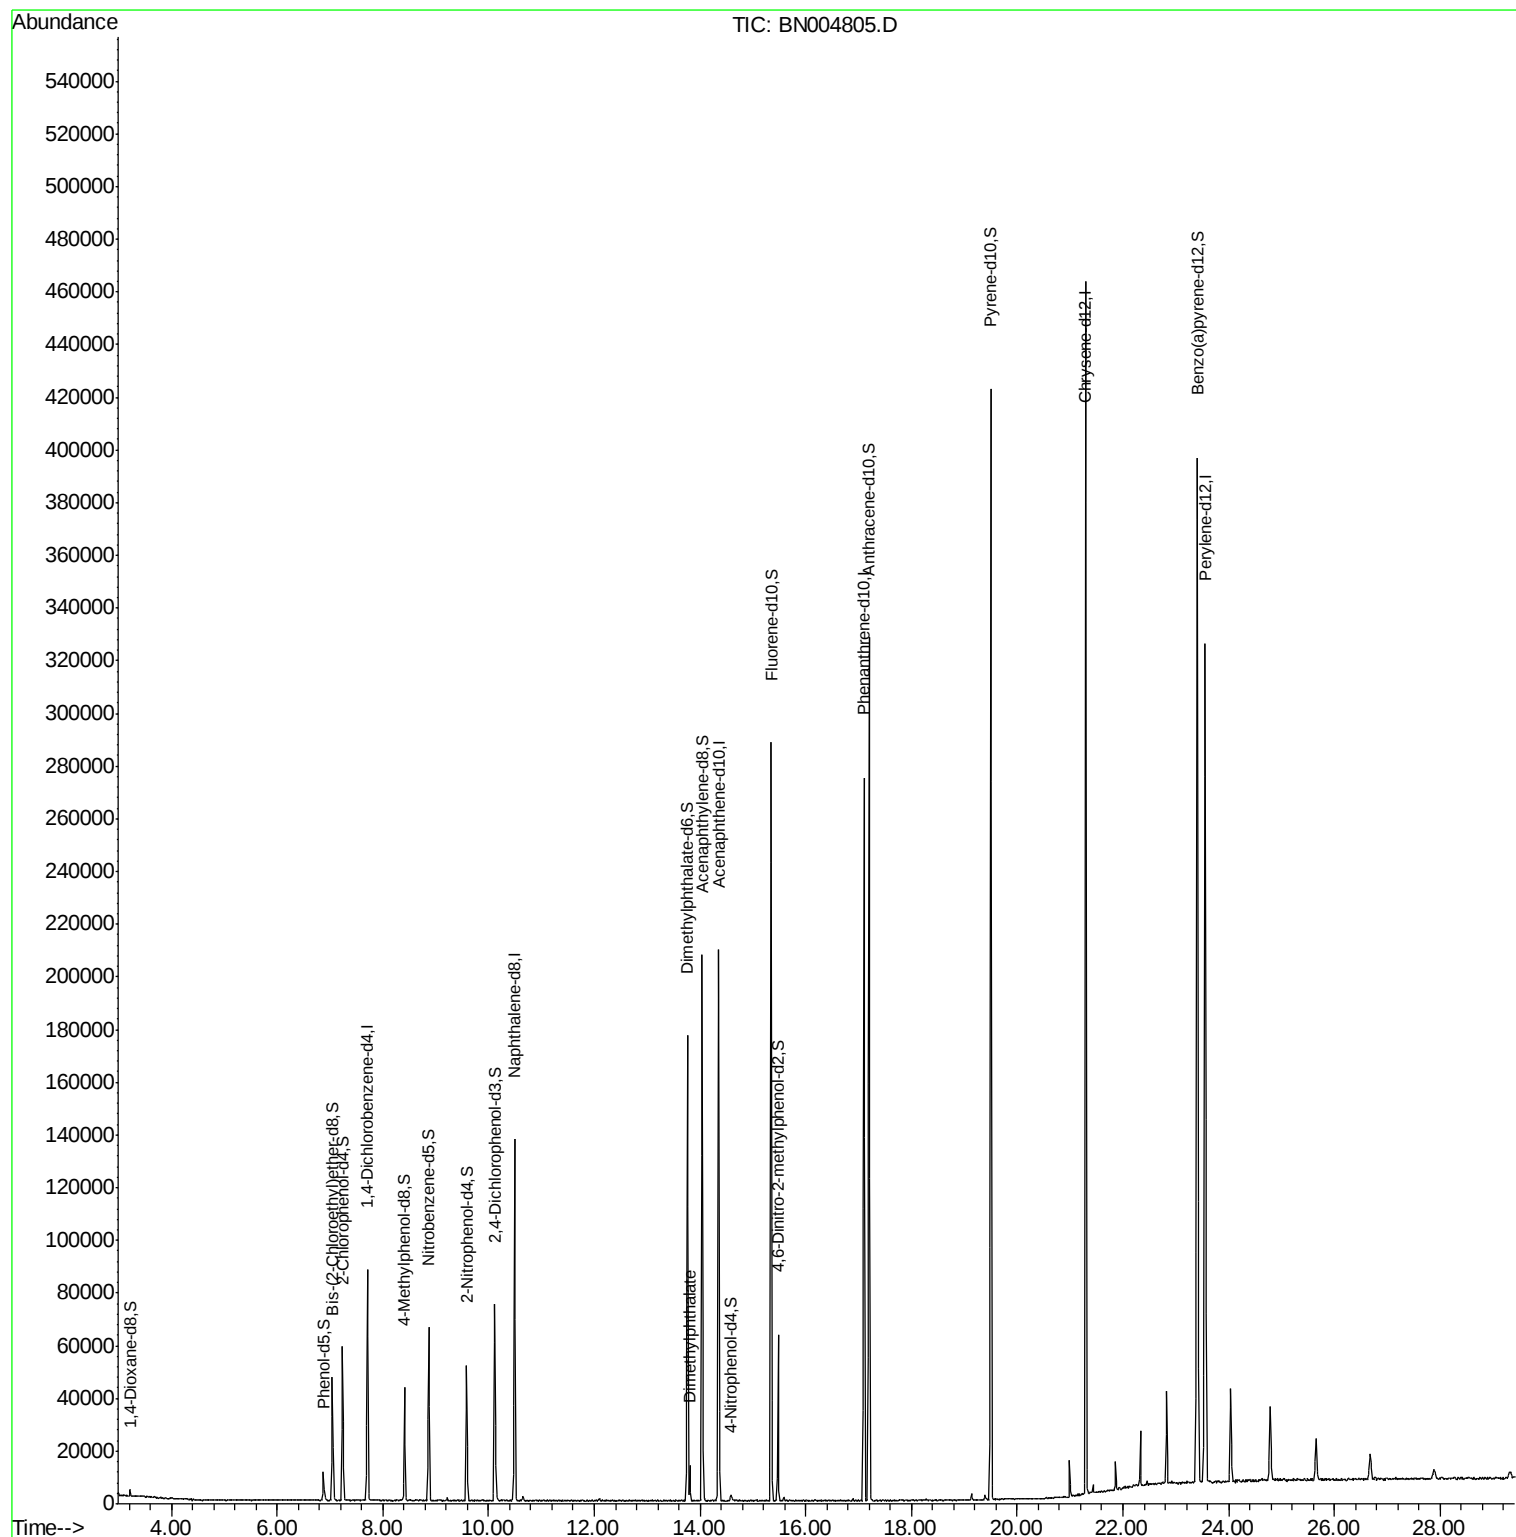

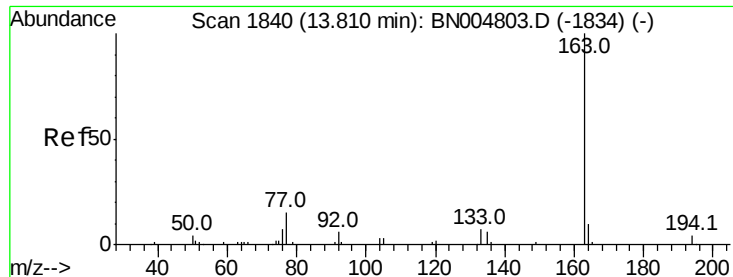

#45

Dimethylphthalate

Concen: 1.828 ng/ul

RT: 13.81 min Scan# 1840

Delta R.T. -0.01 min

Lab File: BN004805.D

Acq: 18 Mar 2019 19:43

Instrument :

BNA_N

ClientSampleId :

C09B5


Tot Ion:163 Resp: 11082

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.3 7.9 11.9

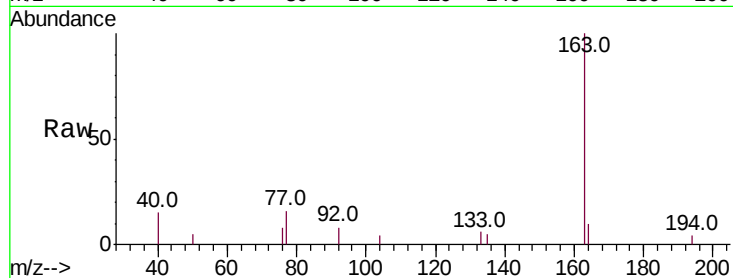

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

