


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN032019\  
 Data File : BN004814.D  
 Acq On : 20 Mar 2019 10:33  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN032019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 20 16:06:20 2019

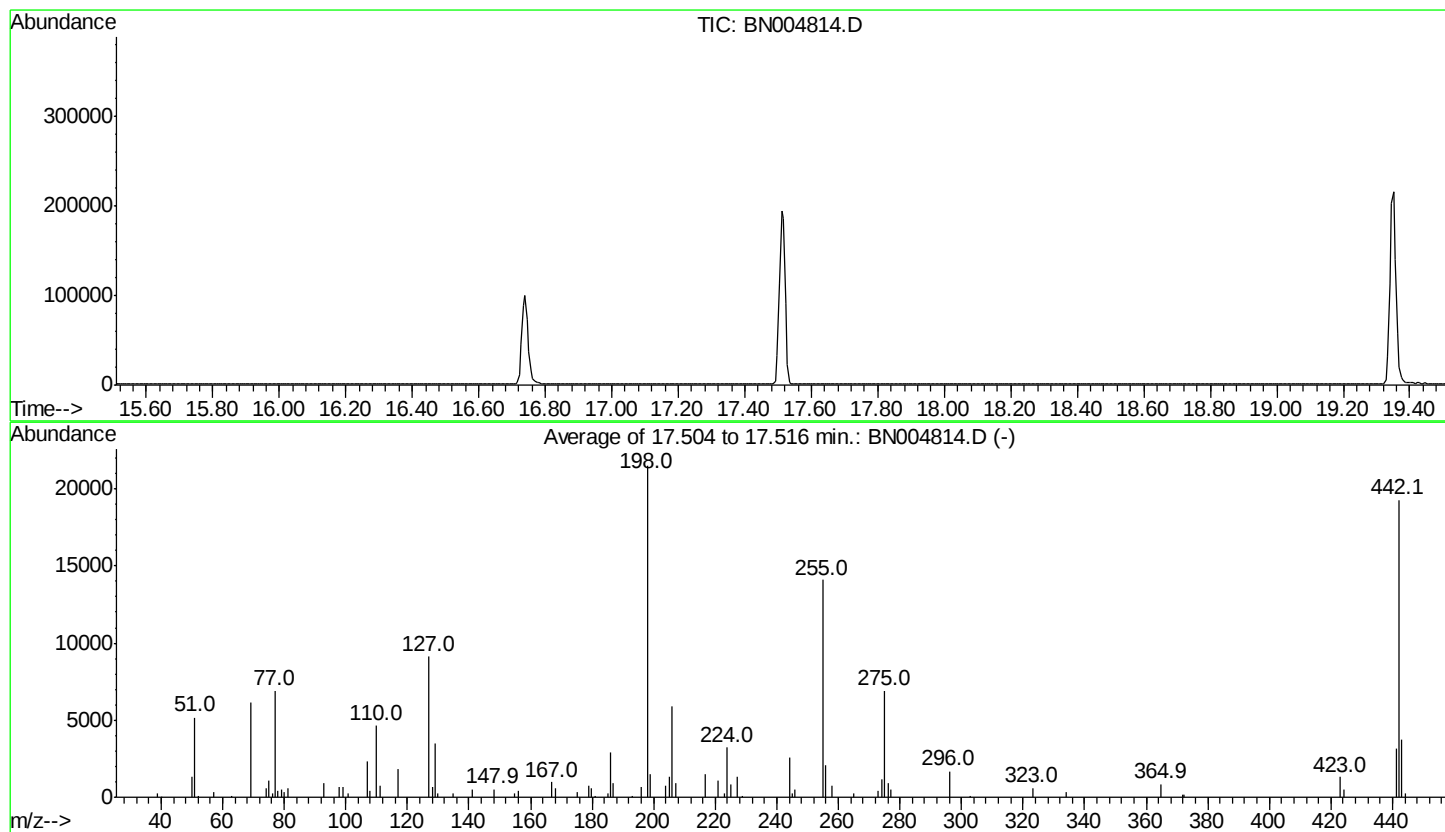

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2463

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 24.0      | 5170    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 28.7      | 6166    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 42.4      | 9119    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 21502   | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 1514    | PASS             |
| 275         | 198          | 10           | 60           | 32.1      | 6912    | PASS             |
| 365         | 198          | 1            | 100          | 4.0       | 864     | PASS             |
| 441         | 198          | 0.01         | 100          | 14.5      | 3125    | PASS             |
| 442         | 198          | 50           | 100          | 89.8      | 19299   | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 3769    | PASS             |