


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN032019\
 Data File : BN004823.D
 Acq On : 20 Mar 2019 17:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 20 16:06:20 2019

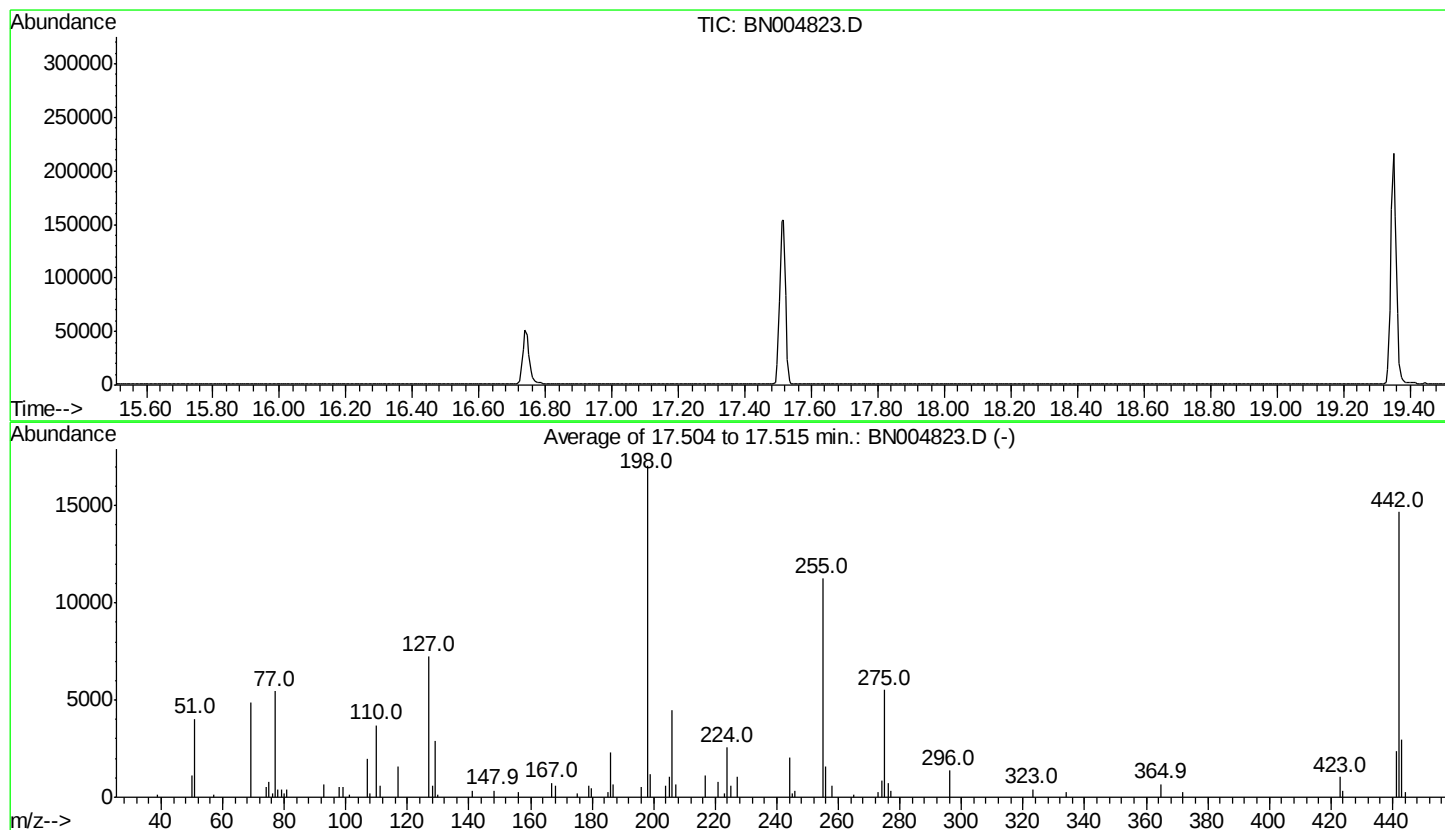

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.7	4041	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.7	4901	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	7237	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17061	PASS
199	198	5	9	6.8	1157	PASS
275	198	10	60	32.4	5521	PASS
365	198	1	100	4.0	679	PASS
441	198	0.01	100	14.0	2393	PASS
442	198	50	100	86.0	14676	PASS
443	442	15	24	20.1	2954	PASS