


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032119\
 Data File : BN004842.D
 Acq On : 21 Mar 2019 10:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 20 16:06:20 2019

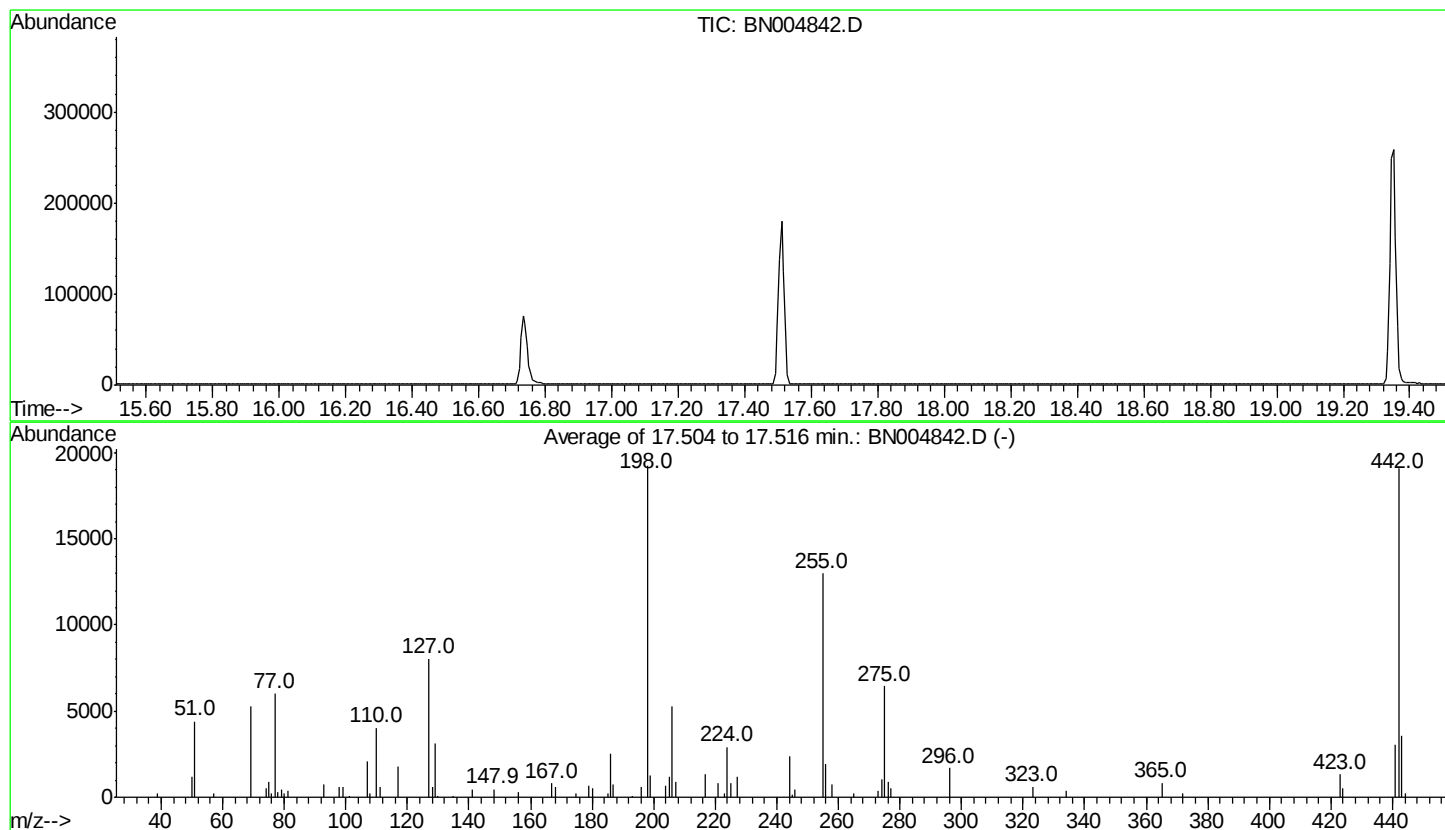

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	4412	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.2	5241	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	8056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19249	PASS
199	198	5	9	6.7	1298	PASS
275	198	10	60	33.5	6456	PASS
365	198	1	100	4.3	831	PASS
441	198	0.01	100	15.8	3044	PASS
442	198	50	100	99.2	19102	PASS
443	442	15	24	18.9	3601	PASS