
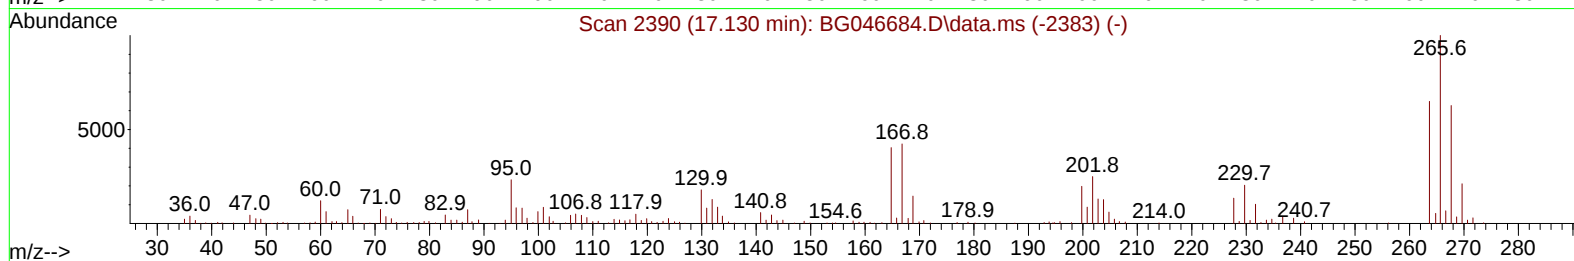
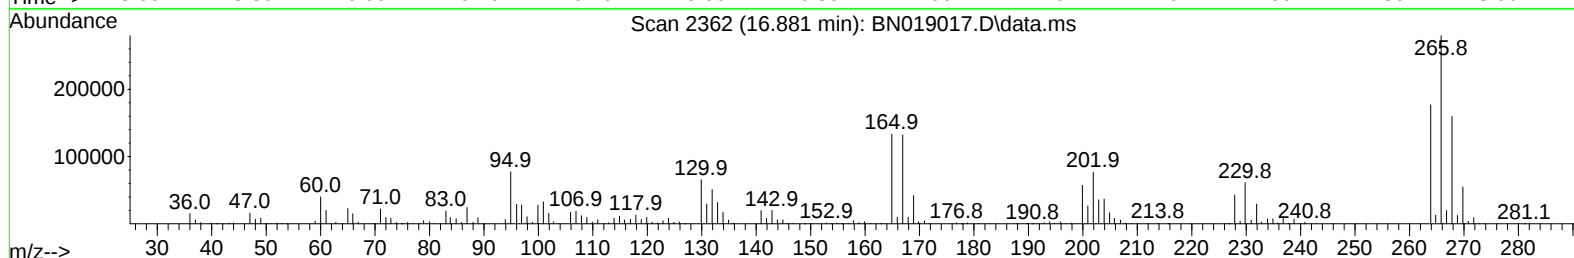


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
Data File : BN019017.D
Acq On : 21 Mar 2022 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 08:12:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

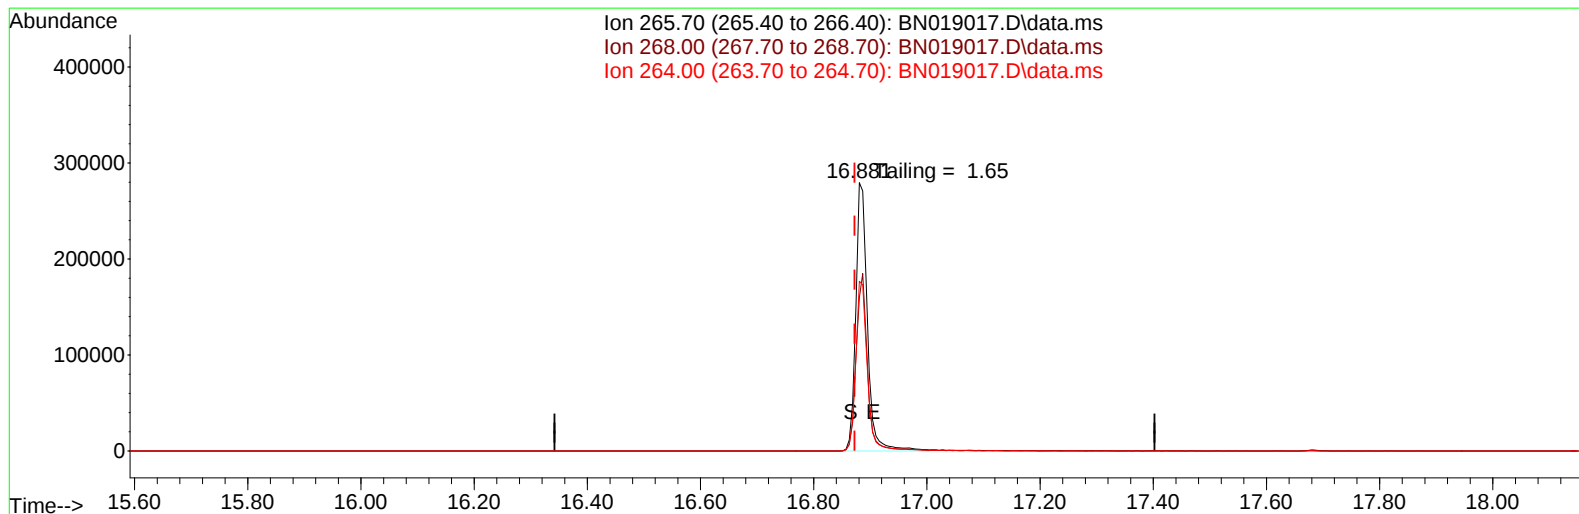

TIC: BN019017.D\data.ms

(70) Pentachlorophenol (C)




16.881min (+ 0.009) 19121.91 ng

response 403672

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.10
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
Data File : BN019017.D
Acq On : 21 Mar 2022 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 08:12:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

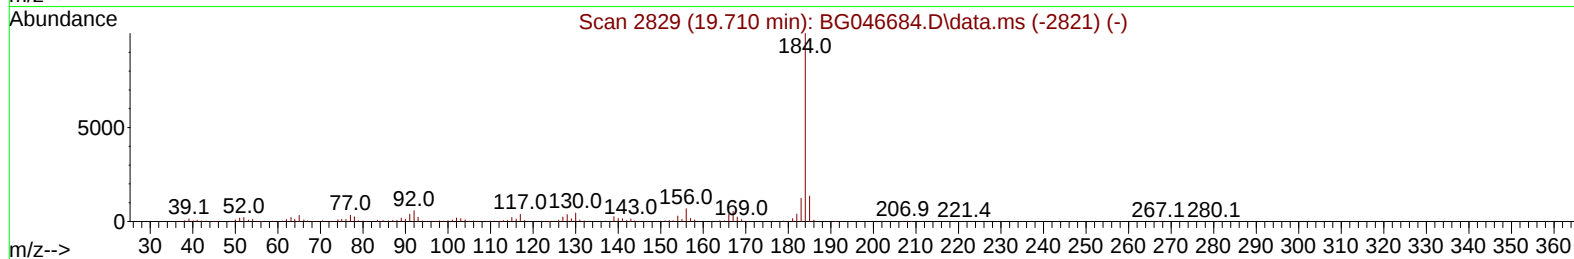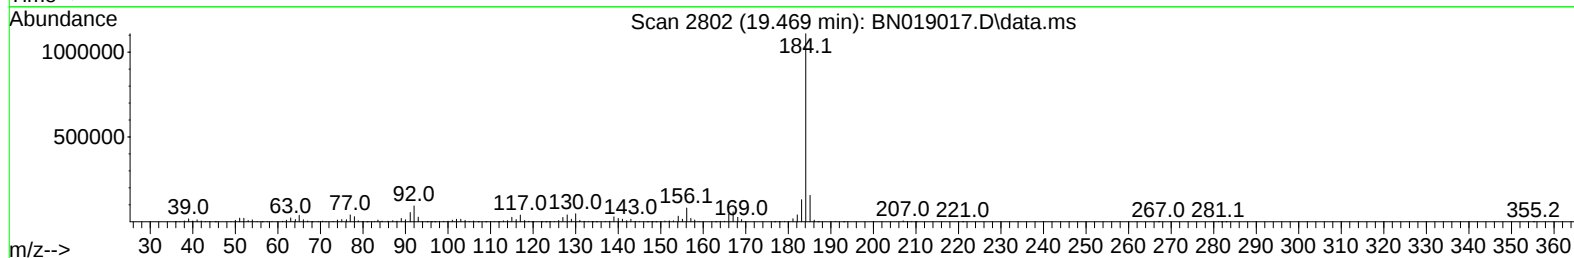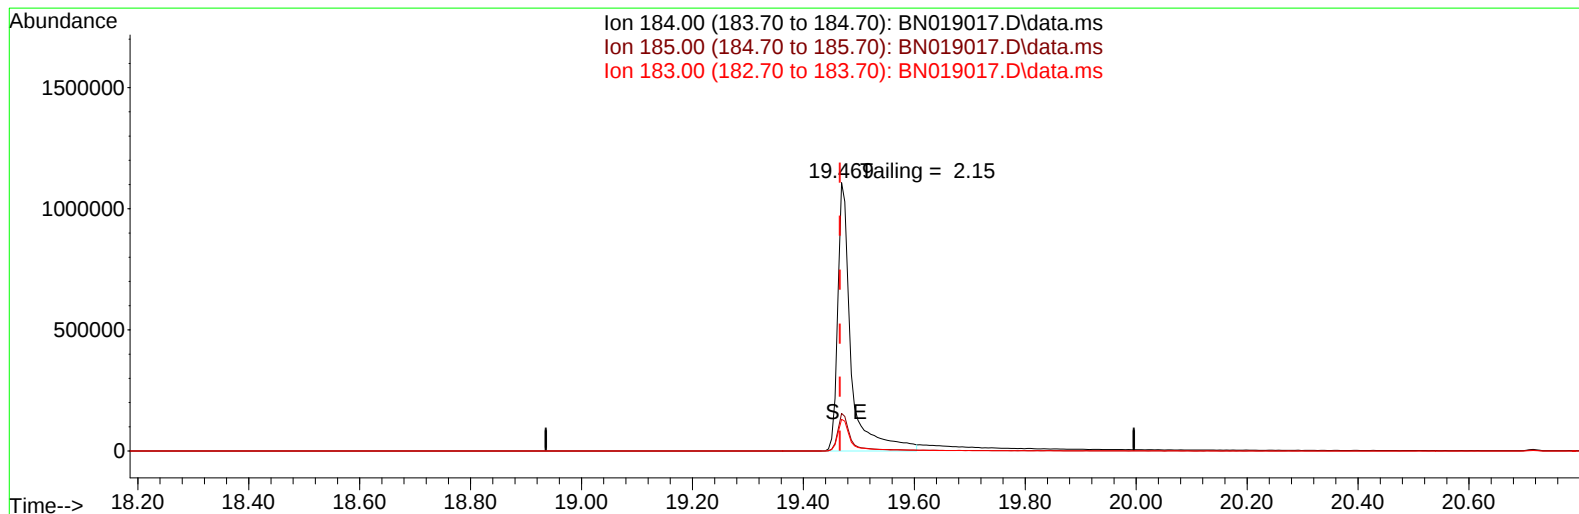

TIC: BN019017.D\data.ms

(77) Benzidine

19.469min (+ 0.003) 0.00 ng

response 2048880

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.05
183.00	13.20	11.80
0.00	0.00	0.00