

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
 Data File : BN019051.D
 Acq On : 22 Mar 2022 09:28
 Operator : CG/JU
 Sample : N2000-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE-132D2-20220315

Quant Time: Mar 22 12:18:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 13:18:23 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.854	152	5996	0.400	ng	0.00
7) Naphthalene-d8	10.658	136	16429	0.400	ng	# 0.00
13) Acenaphthene-d10	14.485	164	9519	0.400	ng	-0.01
19) Phenanthrene-d10	17.236	188	15014	0.400	ng	# 0.00
29) Chrysene-d12	21.422	240	8007	0.400	ng	# 0.00
35) Perylene-d12	23.788	264	7086	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.406	112	1434	0.107	ng	0.00
5) Phenol-d6	7.024	99	644	0.046	ng	0.01
8) Nitrobenzene-d5	9.014	82	2561	0.216	ng	0.00
11) 2-Methylnaphthalene-d10	12.250	152	7398	0.271	ng	0.00
14) 2,4,6-Tribromophenol	15.985	330	667	0.145	ng	0.00
15) 2-Fluorobiphenyl	13.116	172	10017	0.263	ng	-0.01
27) Fluoranthene-d10	19.261	212	13635	0.306	ng	0.00
31) Terphenyl-d14	19.860	244	7667	0.390	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.247	88	33805	4.562	ng	98
9) Naphthalene	10.712	128	1261	0.027	ng	# 81
17) Acenaphthene	14.549	154	1072	0.035	ng	93
25) Phenanthrene	17.277	178	1798	0.038	ng	# 96
34) Bis(2-ethylhexyl)phtha...	21.333	149	992	0.061	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
Data File : BN019051.D
Acq On : 22 Mar 2022 09:28
Operator : CG/JU
Sample : N2000-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Quant Time: Mar 22 12:18:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 13:18:23 2022
Response via : Initial Calibration

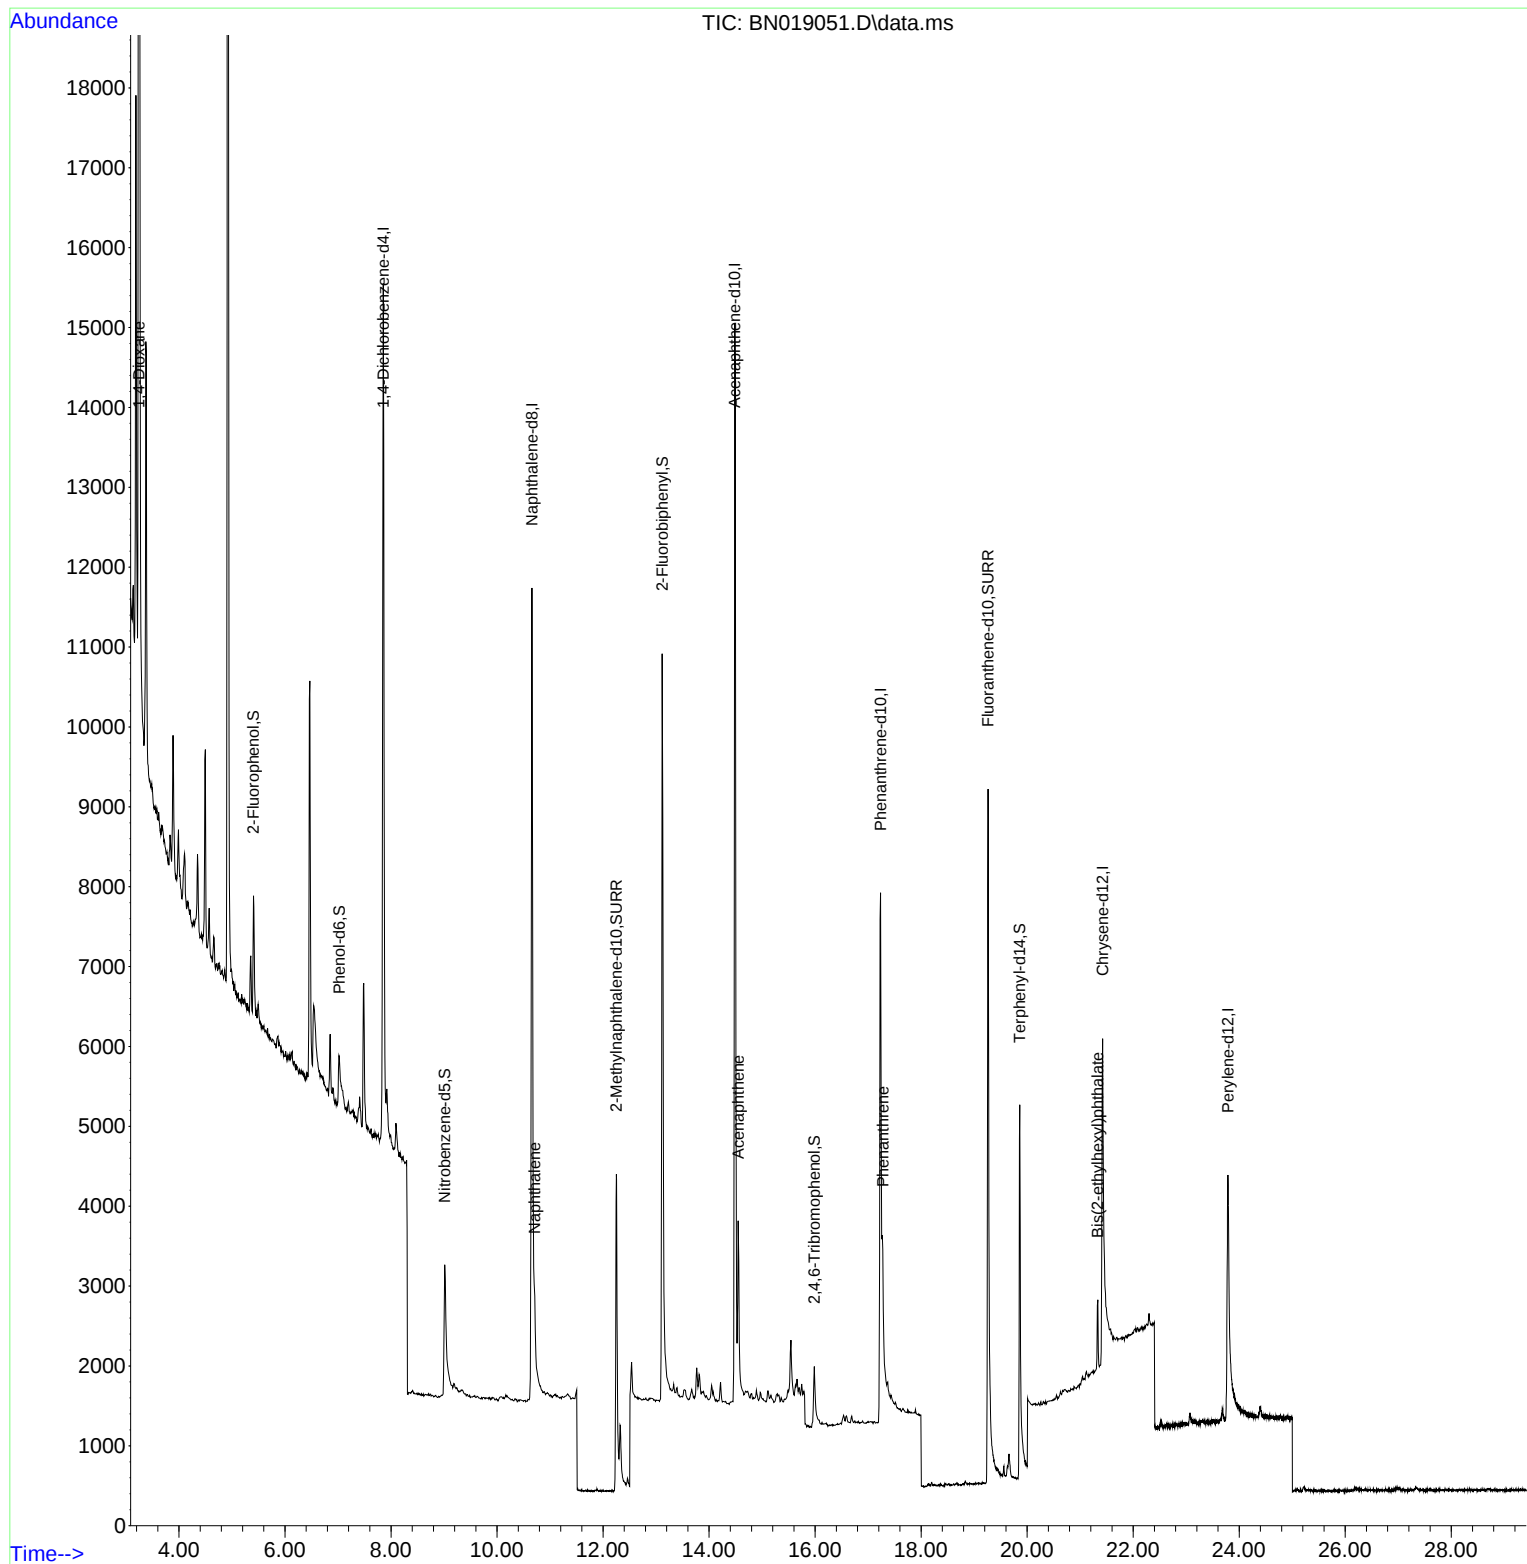



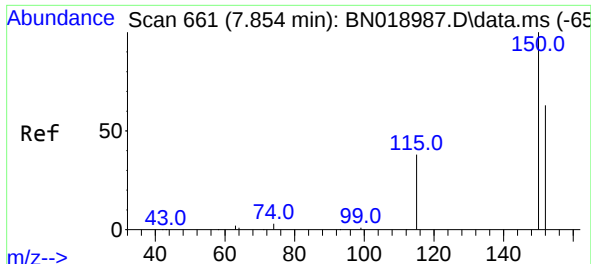


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.854 min Scan# 60
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315



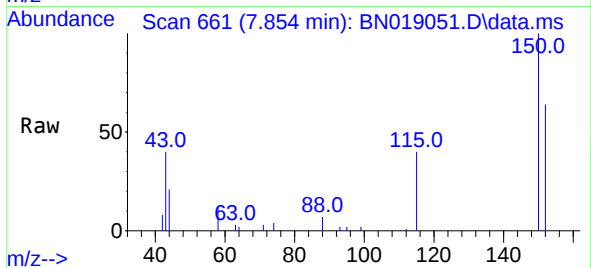



Tgt Ion:152 Resp: 5996
Ion Ratio Lower Upper
152 100
150 155.7 123.9 185.9
115 61.6 48.2 72.4

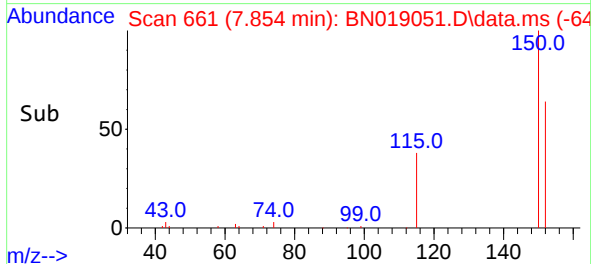

#2
1,4-Dioxane
Concen: 4.562 ng
RT: 3.247 min Scan# 23
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion: 88 Resp: 33805
Ion Ratio Lower Upper
88 100
43 32.9 24.6 37.0
58 80.3 65.4 98.2


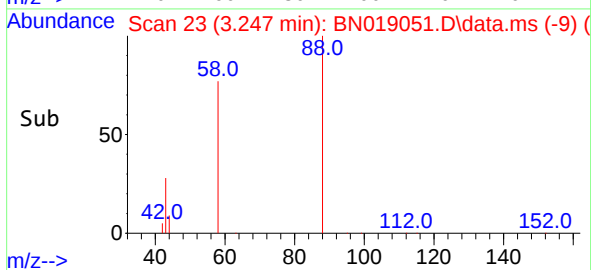

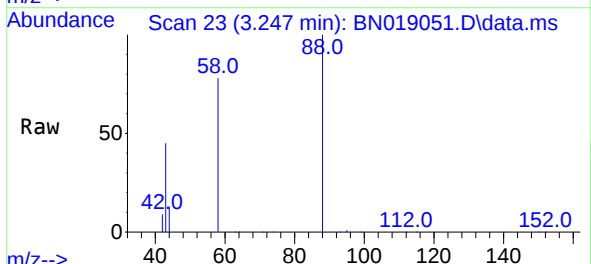


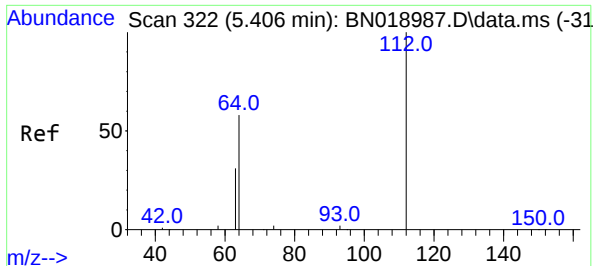

#4
2-Fluorophenol
Concen: 0.107 ng
RT: 5.406 min Scan# 31
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28




Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Tgt Ion:112 Resp: 1434
Ion Ratio Lower Upper
112 100
64 63.8 47.8 71.8
63 30.8 25.7 38.5

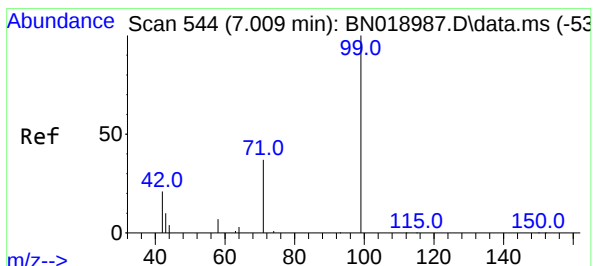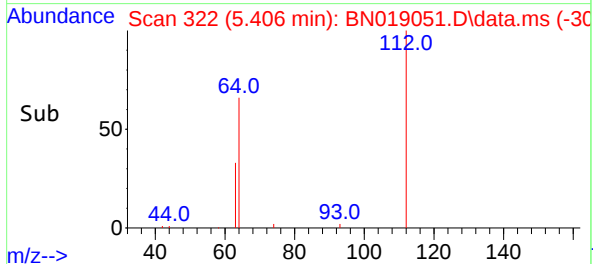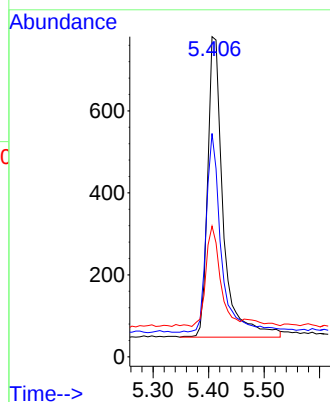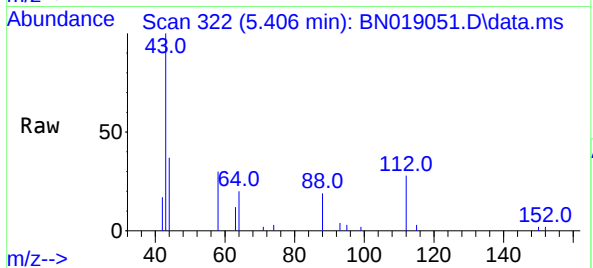

#5
Phenol-d6
Concen: 0.046 ng
RT: 7.024 min Scan# 546
Delta R.T. 0.015 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion: 99 Resp: 644
Ion Ratio Lower Upper
99 100
42 22.2 16.2 24.4
71 56.5 27.7 41.5#


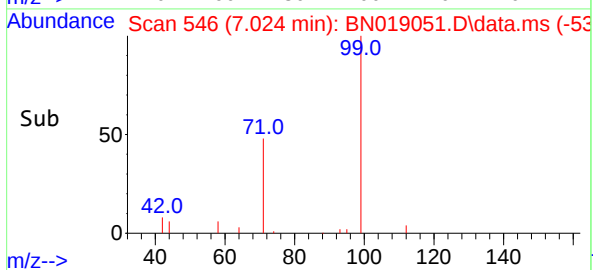
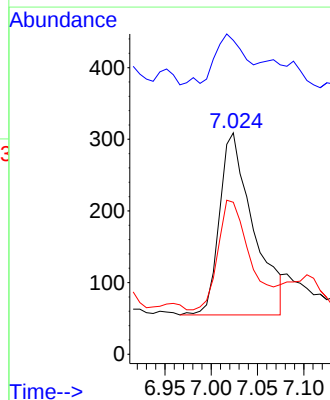
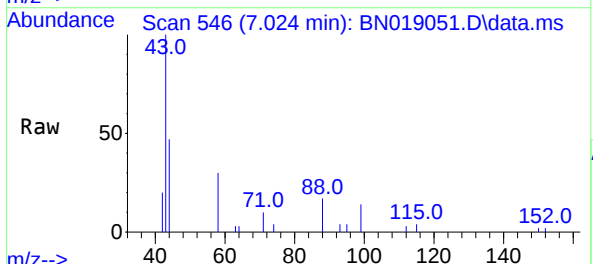




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.658 min Scan# 944
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28




Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Tgt Ion:	136	Resp:	16429
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.0	13.4
54	10.1	5.8	8.6#
68	7.3	4.6	7.0#

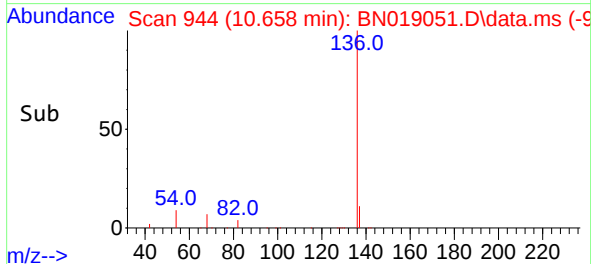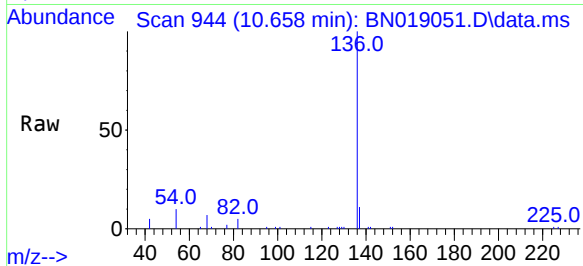

#8
Nitrobenzene-d5
Concen: 0.216 ng
RT: 9.014 min Scan# 790
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion:	82	Resp:	2561
Ion Ratio	Lower	Upper	
82	100		
128	39.0	33.0	49.6
54	59.3	42.5	63.7


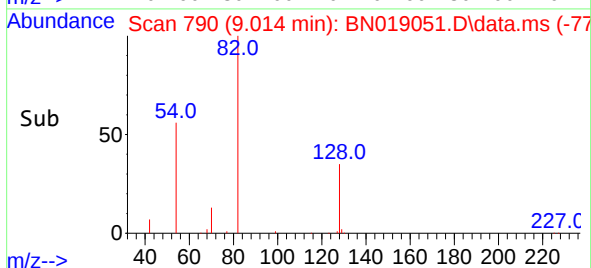
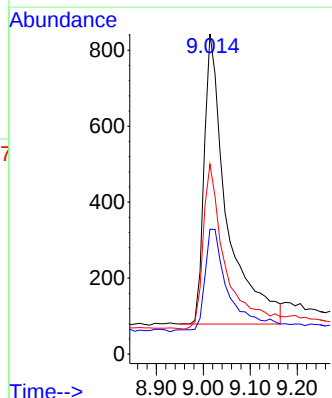
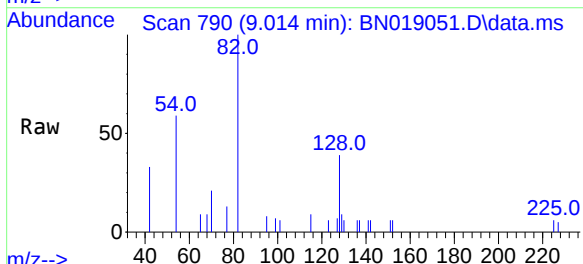


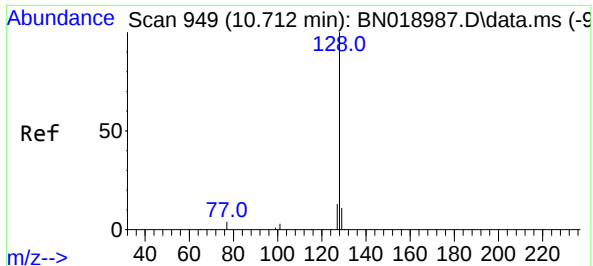

#9
Naphthalene
Concen: 0.027 ng
RT: 10.712 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28




Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Tgt Ion:128 Resp: 1261
Ion Ratio Lower Upper
128 100
129 19.4 9.0 13.4#
127 20.1 10.7 16.1#

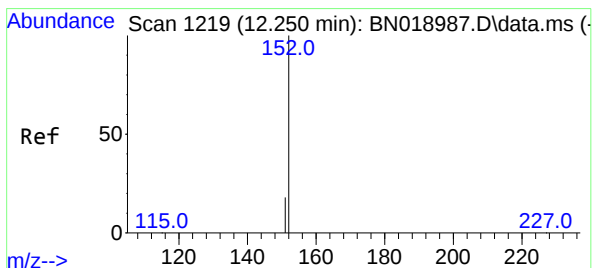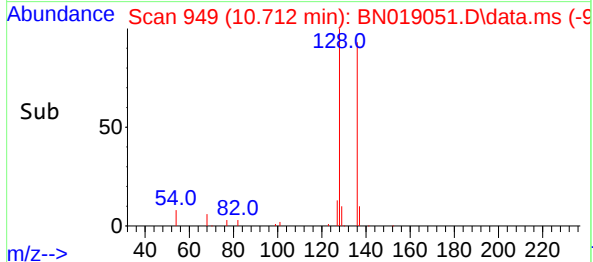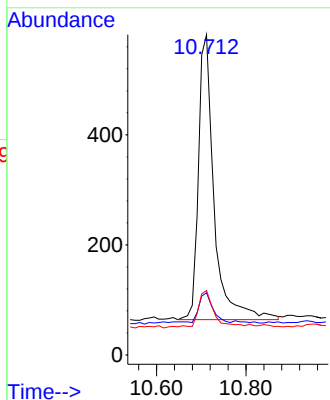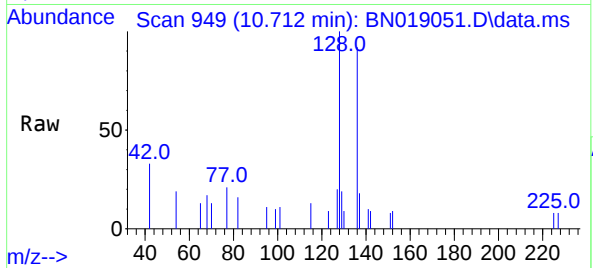

#11
2-Methylnaphthalene-d10
Concen: 0.271 ng
RT: 12.250 min Scan# 1219
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion:152 Resp: 7398
Ion Ratio Lower Upper
152 100
151 20.0 16.5 24.7


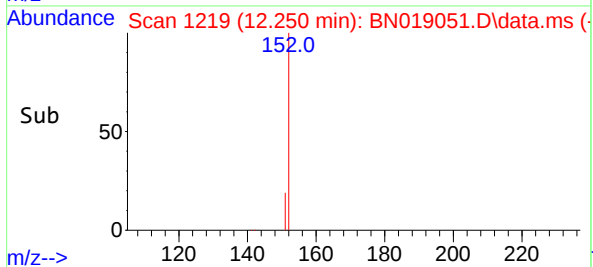
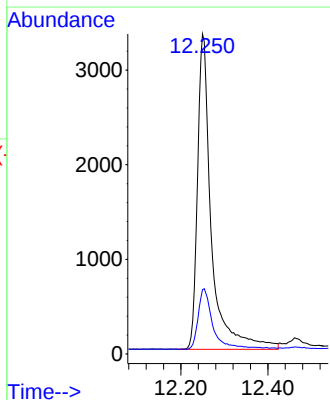
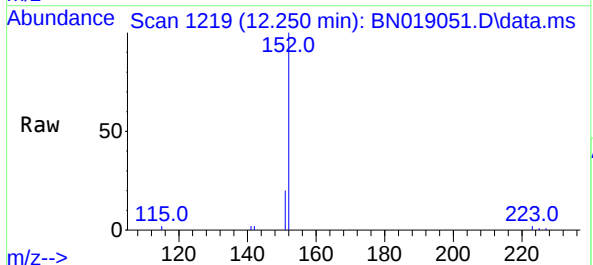




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.485 min Scan# 1473
Delta R.T. -0.011 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28




Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Tgt Ion:164 Resp: 9519
Ion Ratio Lower Upper
164 100
162 106.0 85.2 127.8
160 51.1 41.5 62.3

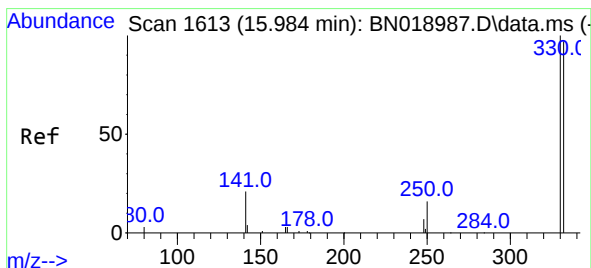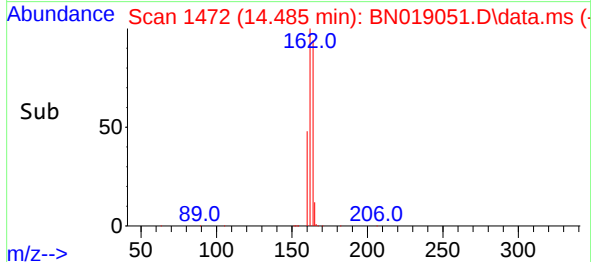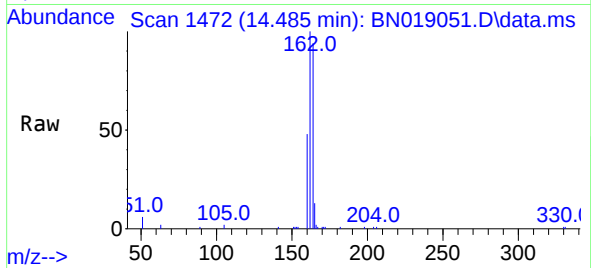

#14
2,4,6-Tribromophenol
Concen: 0.145 ng
RT: 15.985 min Scan# 1613
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion:330 Resp: 667
Ion Ratio Lower Upper
330 100
332 98.8 76.8 115.2
141 43.3 32.2 48.2


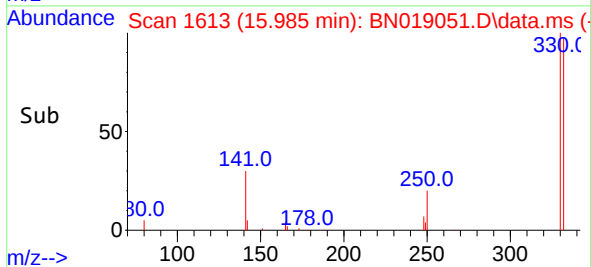

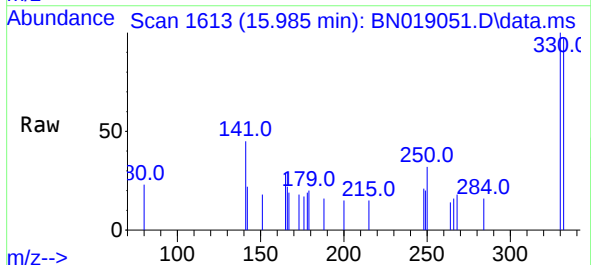




#15
2-Fluorobiphenyl
Concen: 0.263 ng
RT: 13.116 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28




Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Tgt Ion:	172	Resp:	10017
Ion	Ratio	Lower	Upper
172	100		
171	34.9	28.2	42.2
170	24.4	18.7	28.1

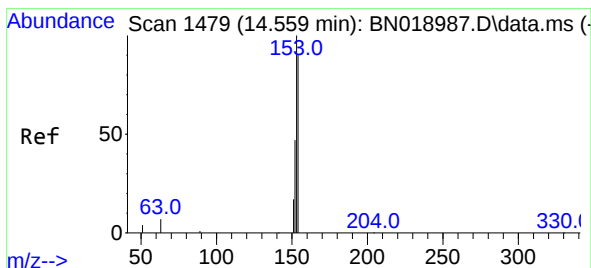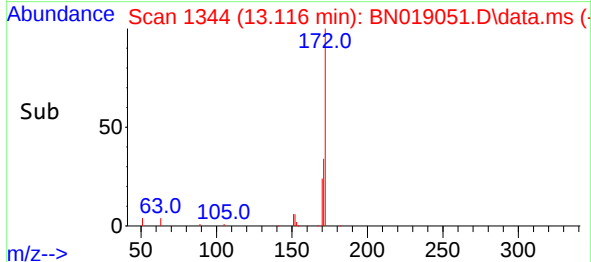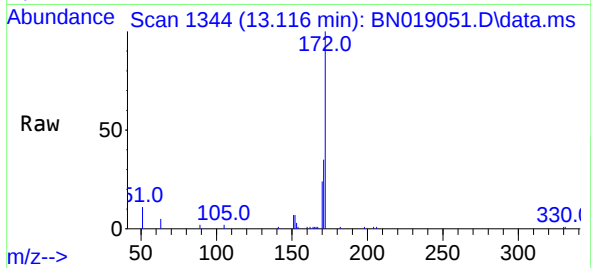

#17
Acenaphthene
Concen: 0.035 ng
RT: 14.549 min Scan# 1478
Delta R.T. -0.011 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion:	154	Resp:	1072
Ion	Ratio	Lower	Upper
154	100		
153	120.2	89.7	134.5
152	60.0	44.7	67.1


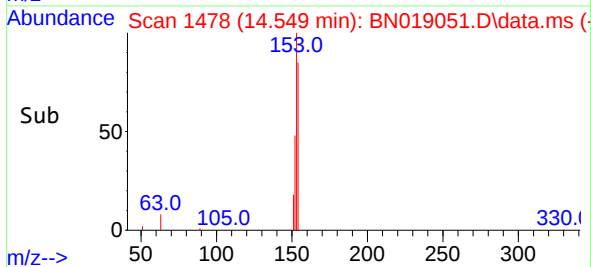

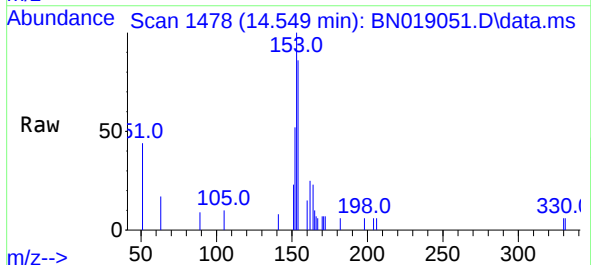




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.236 min Scan# 1735
Delta R.T. -0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28




Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Tgt Ion:188 Resp: 15014
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.8 11.8 17.8#

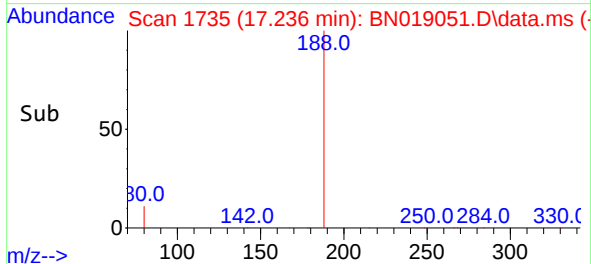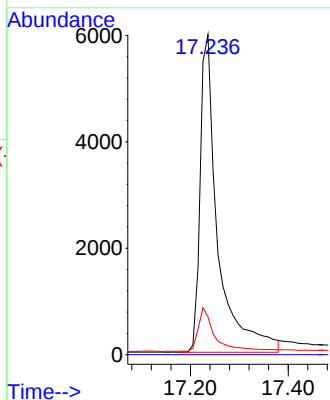

#25
Phenanthrene
Concen: 0.038 ng
RT: 17.277 min Scan# 1739
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion:178 Resp: 1798
Ion Ratio Lower Upper
178 100
176 19.5 15.4 23.0
179 19.0 12.2 18.2#


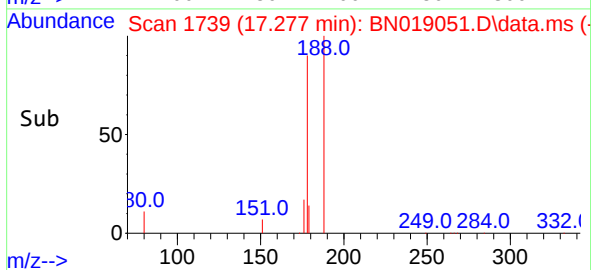
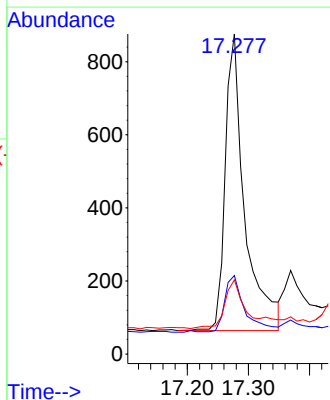
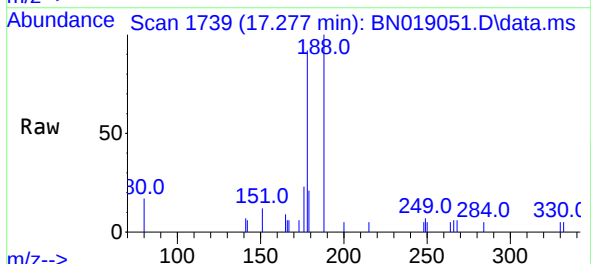




#27
Fluoranthene-d10
Concen: 0.306 ng
RT: 19.261 min Scan# 2108
Delta R.T. -0.004 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28




Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315


Tgt Ion:212 Resp: 13635
Ion Ratio Lower Upper
212 100
106 15.9 12.7 19.1
104 8.7 7.1 10.7

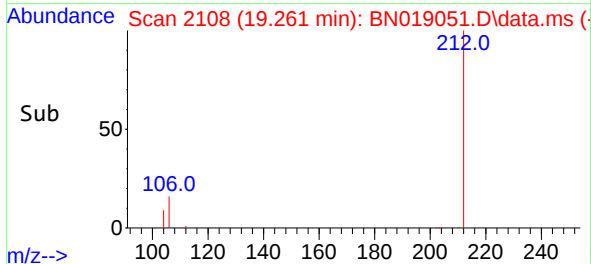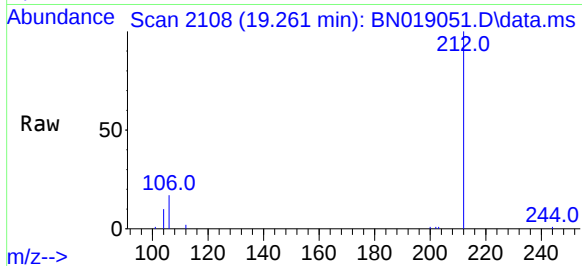

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.422 min Scan# 2443
Delta R.T. 0.000 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Tgt Ion:240 Resp: 8007
Ion Ratio Lower Upper
240 100
120 16.8 8.5 12.7#
236 29.7 22.4 33.6


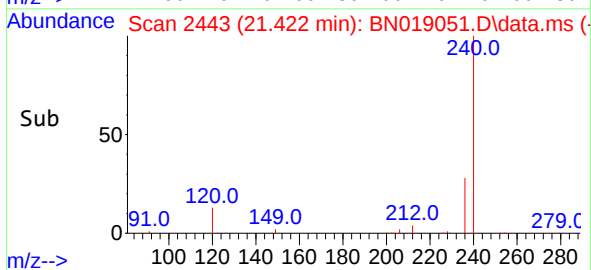

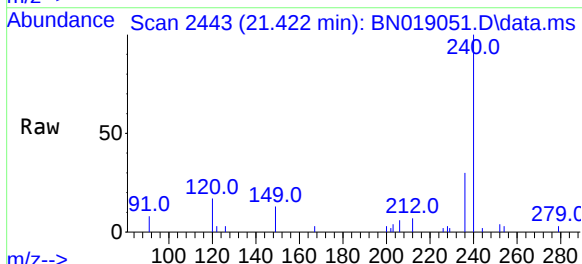




#31
 Terphenyl-d14
 Concen: 0.390 ng
 RT: 19.860 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN019051.D
 Acq: 22 Mar 2022 09:28




Instrument :
 BNA_N
 ClientSampleId :
 RE-132D2-20220315


Tgt Ion:244 Resp: 7667
 Ion Ratio Lower Upper
 244 100
 212 11.3 8.2 12.4
 122 0.0 0.0 0.0

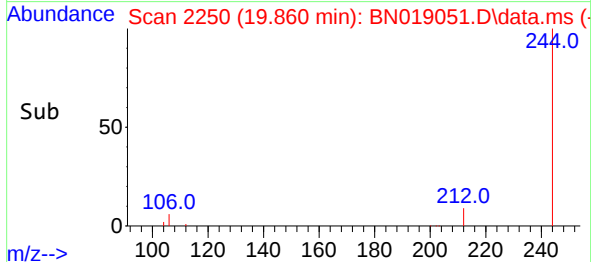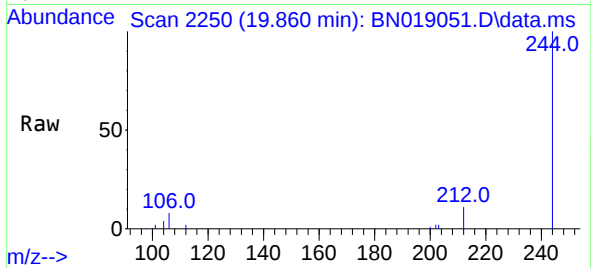

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.061 ng
 RT: 21.333 min Scan# 2433
 Delta R.T. 0.000 min
 Lab File: BN019051.D
 Acq: 22 Mar 2022 09:28


Tgt Ion:149 Resp: 992
 Ion Ratio Lower Upper
 149 100
 167 26.8 21.8 32.8
 279 4.1 2.0 3.0#

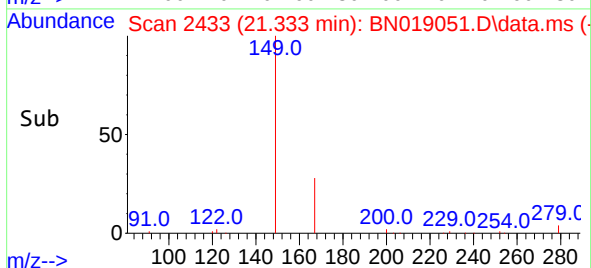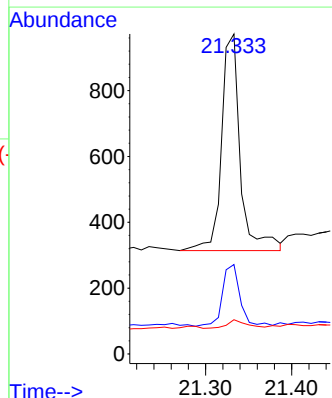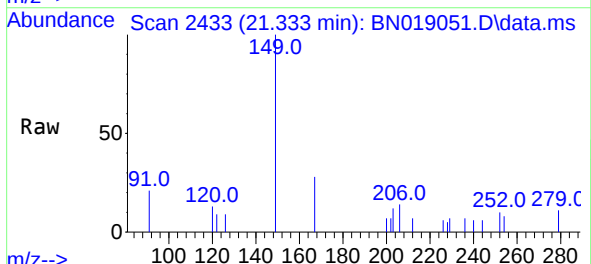

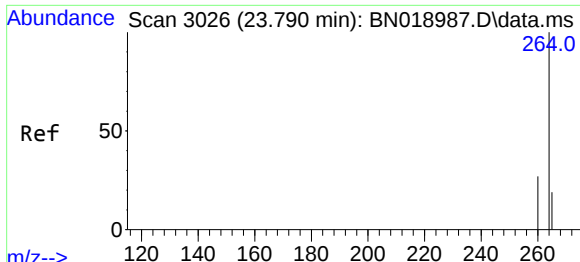

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.788 min Scan# 30
Delta R.T. -0.003 min
Lab File: BN019051.D
Acq: 22 Mar 2022 09:28

Instrument :
BNA_N
ClientSampleId :
RE-132D2-20220315

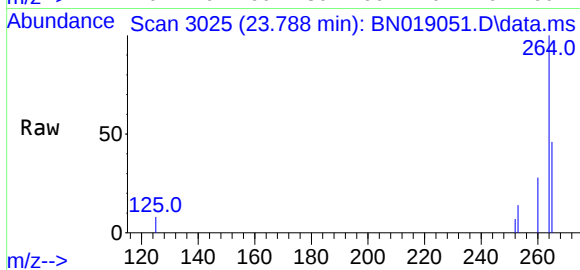

Tgt Ion:264 Resp: 7086
Ion Ratio Lower Upper
264 100
260 28.2 22.4 33.6
265 46.0 25.3 37.9#

