
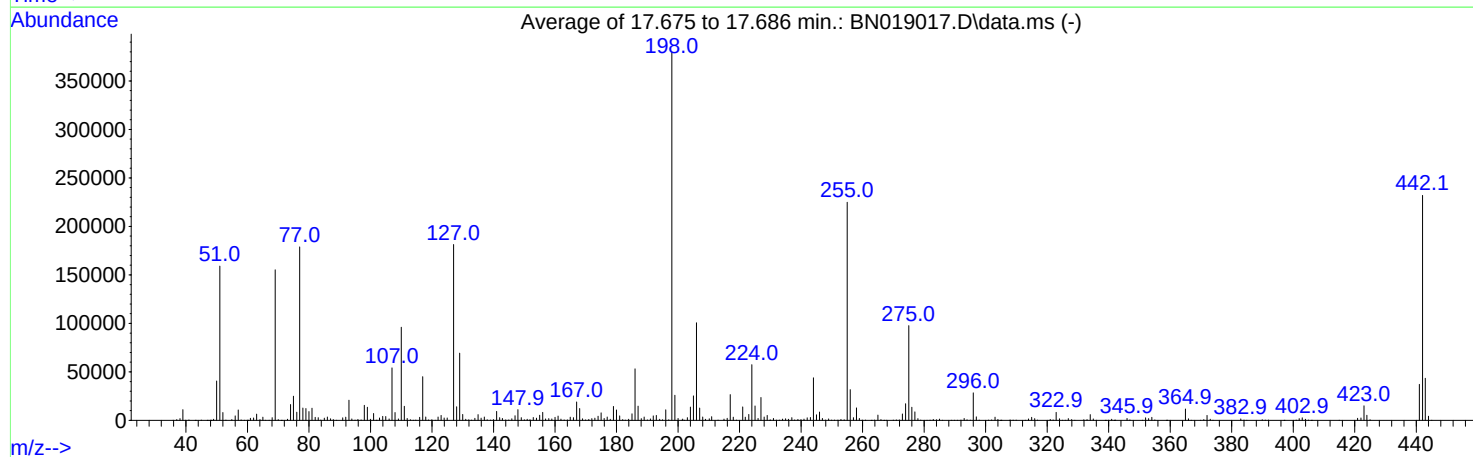


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
 Data File : BN019017.D
 Acq On : 21 Mar 2022 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

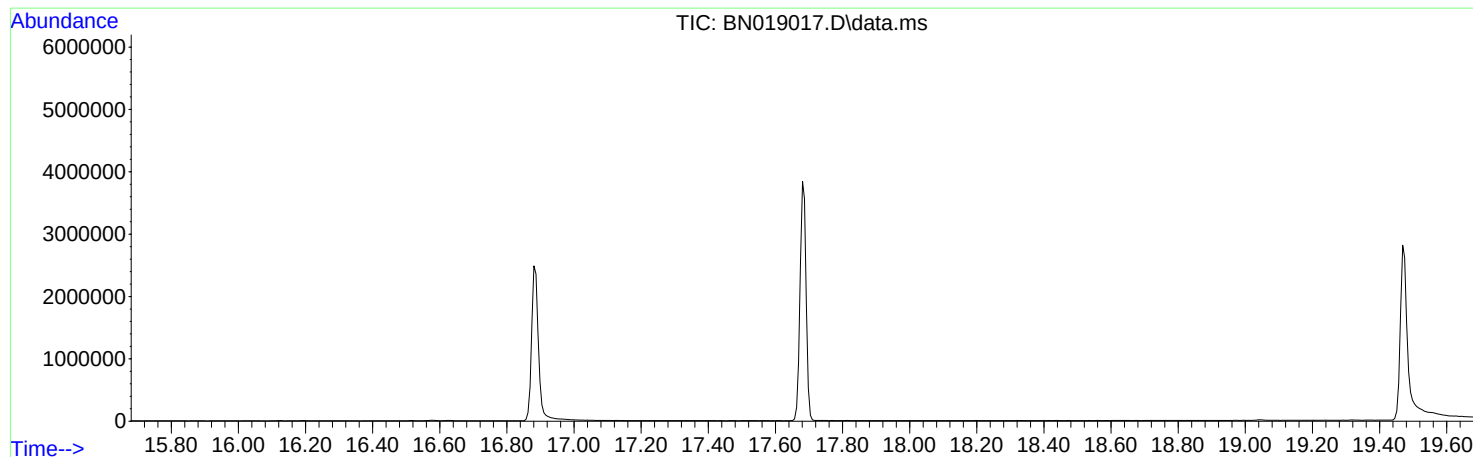




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	159104	PASS
68	69	0.00	2	1.8	2780	PASS
69	198	0.00	100	40.9	155243	PASS
70	69	0.00	2	0.6	862	PASS
127	198	10	80	47.8	181376	PASS
197	198	0.00	2	0.2	592	PASS
198	198	100	100	100.0	379349	PASS
199	198	5	9	6.8	25923	PASS
275	198	10	60	25.8	97693	PASS
365	198	1	100	3.1	11767	PASS
441	198	0.01	100	9.8	37192	PASS
442	442	50	100	100.0	232043	PASS
443	442	15	24	18.7	43477	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
 Data File : BN019017.D
 Acq On : 21 Mar 2022 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 08:12:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 14 15:11:57 2022
 Response via : Initial Calibration

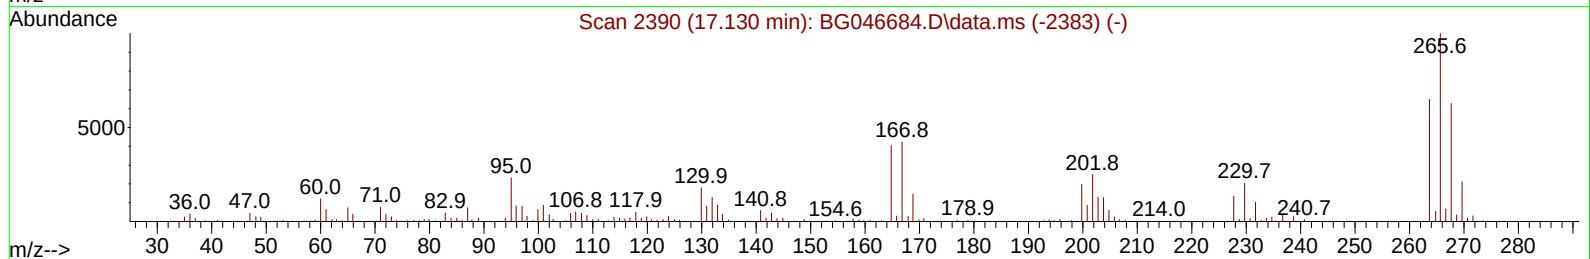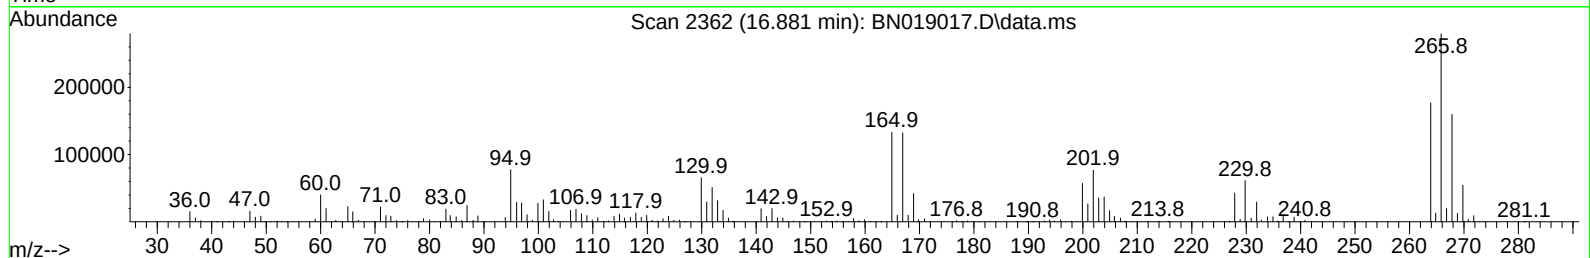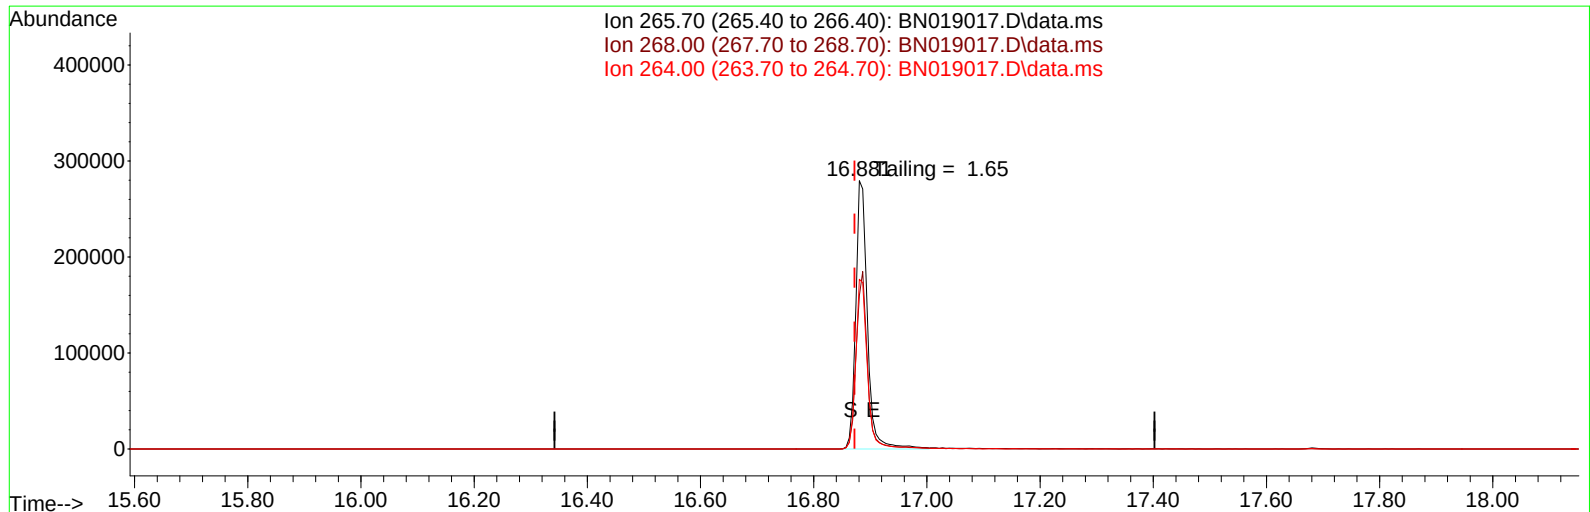

TIC: BN019017.D\data.ms

(70) Pentachlorophenol (C)

16.881min (+ 0.009) 19121.91 ng




response 403672

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.10
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
Data File : BN019017.D
Acq On : 21 Mar 2022 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 22 08:12:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

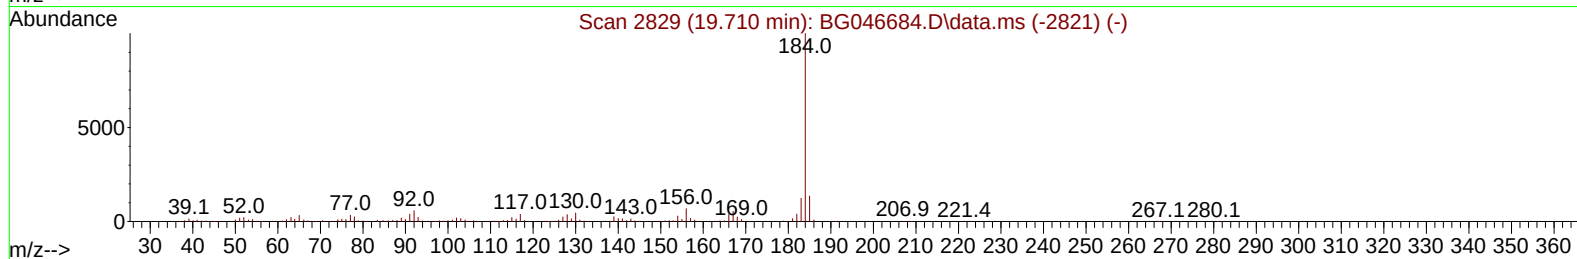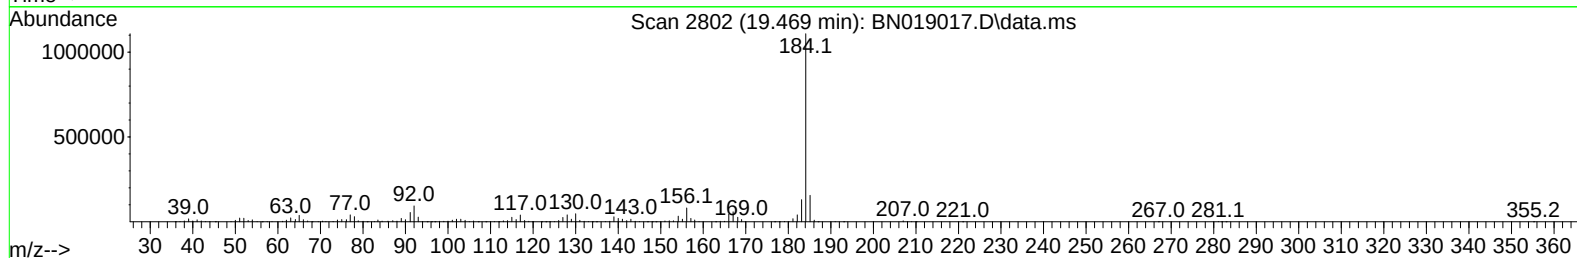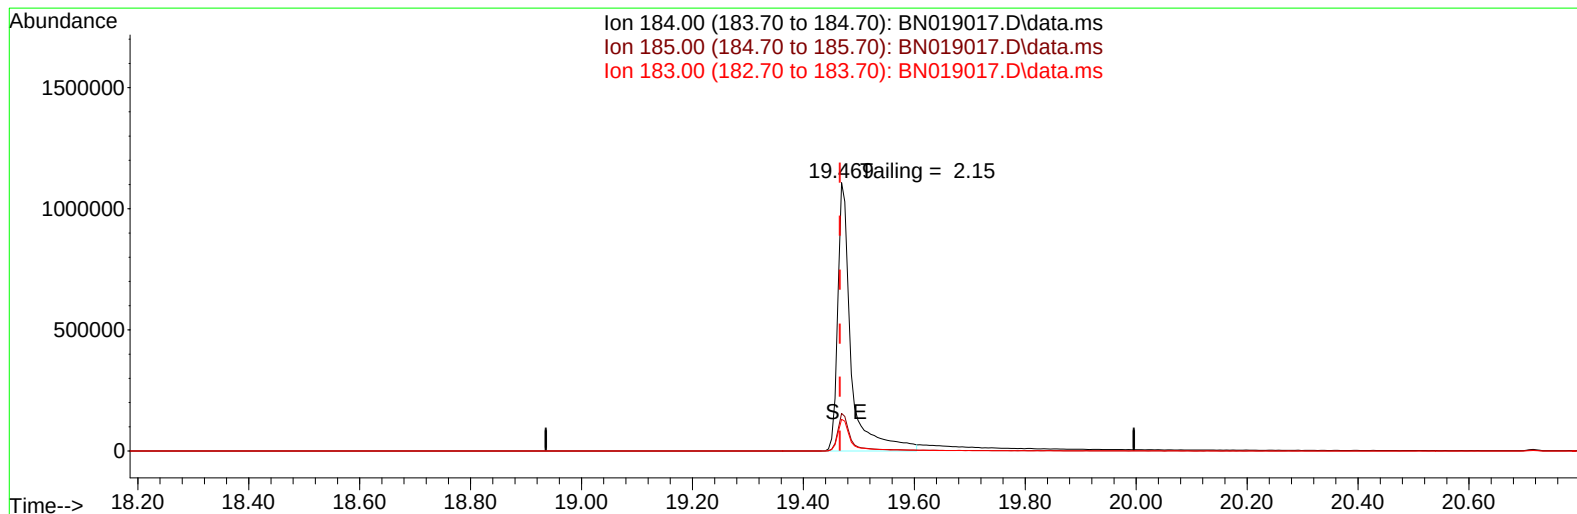

TIC: BN019017.D\data.ms

(77) Benzidine

19.469min (+ 0.003) 0.00 ng

response 2048880

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.05
183.00	13.20	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/21/2022	BNA_N	<u>BN019017.D</u>
Compound Name	Response	Retention Time
DDT	1363368	20.716
DDD	16371	20.275
DDE	1094	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17465	1380833	1.26

Instrument :
BNA_N
ClientSampleId :
DFTPP