
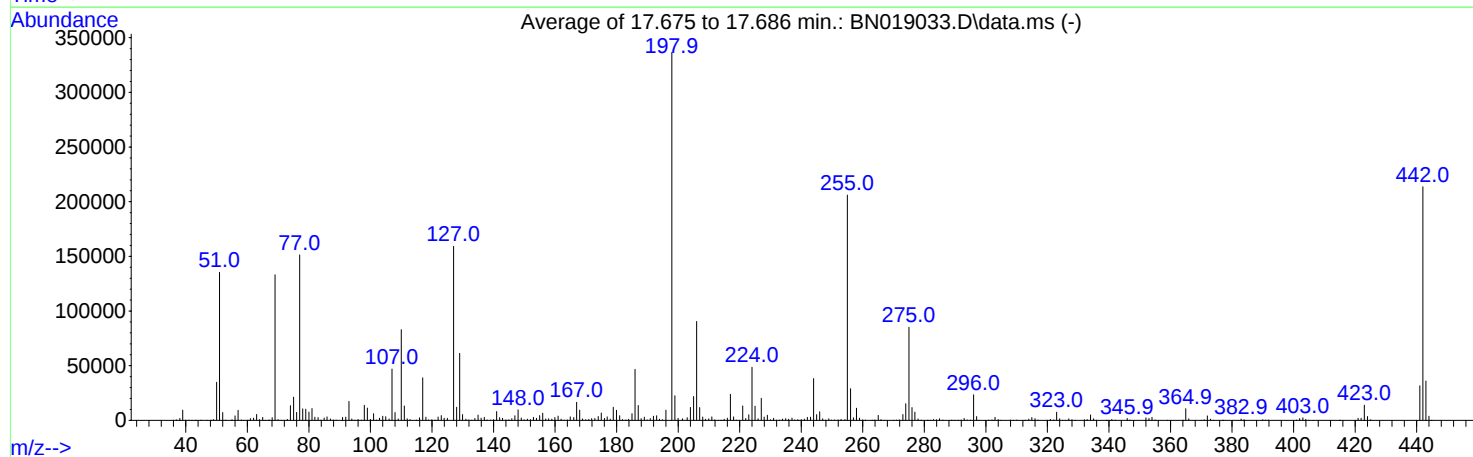


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
 Data File : BN019033.D
 Acq On : 21 Mar 2022 22:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

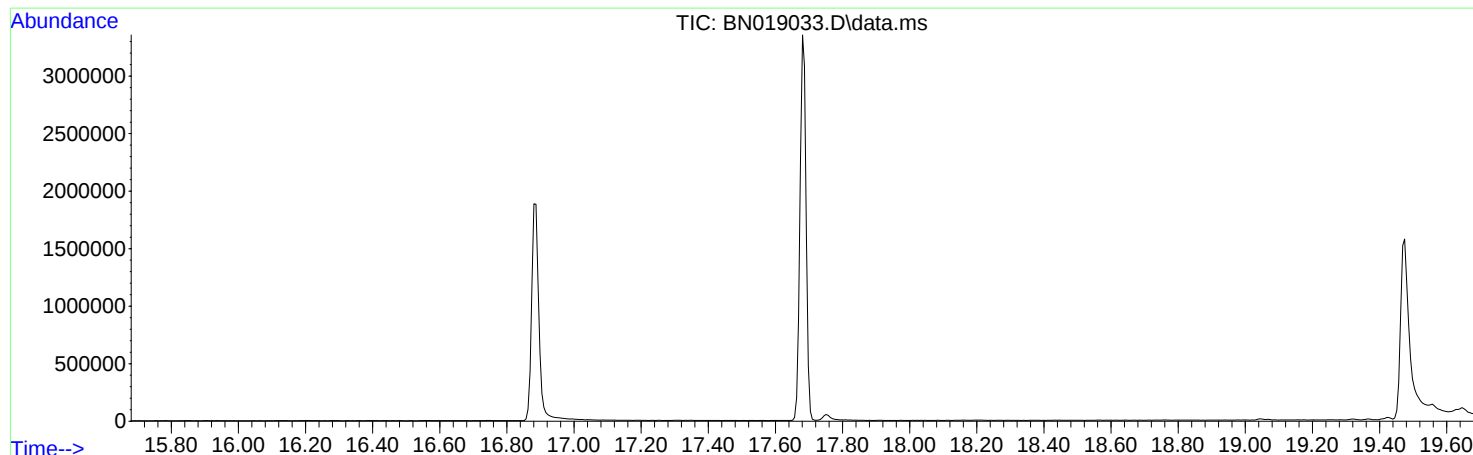




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	135399	PASS
68	69	0.00	2	1.9	2470	PASS
69	198	0.00	100	39.6	133123	PASS
70	69	0.00	2	0.6	782	PASS
127	198	10	80	47.3	159253	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	336448	PASS
199	198	5	9	6.7	22616	PASS
275	198	10	60	25.3	85160	PASS
365	198	1	100	3.2	10663	PASS
441	198	0.01	100	9.4	31576	PASS
442	442	50	100	100.0	213675	PASS
443	442	15	24	16.8	35979	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
 Data File : BN019033.D
 Acq On : 21 Mar 2022 22:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 08:17:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 14 15:11:57 2022
 Response via : Initial Calibration

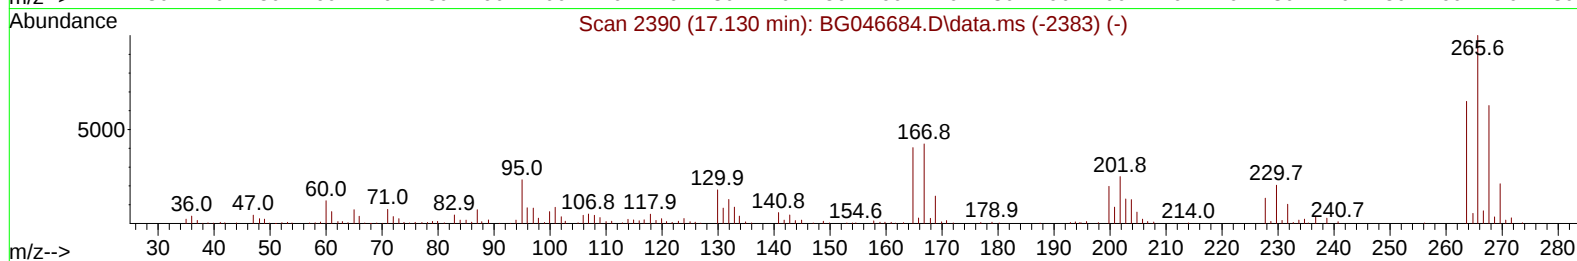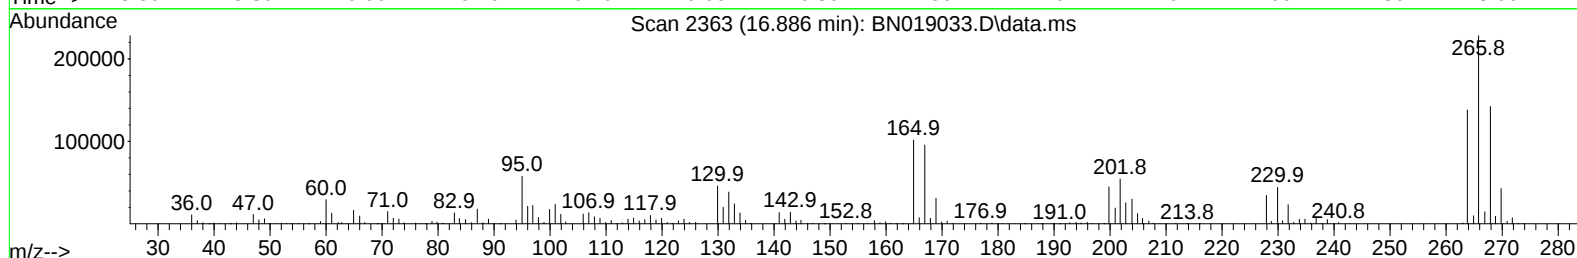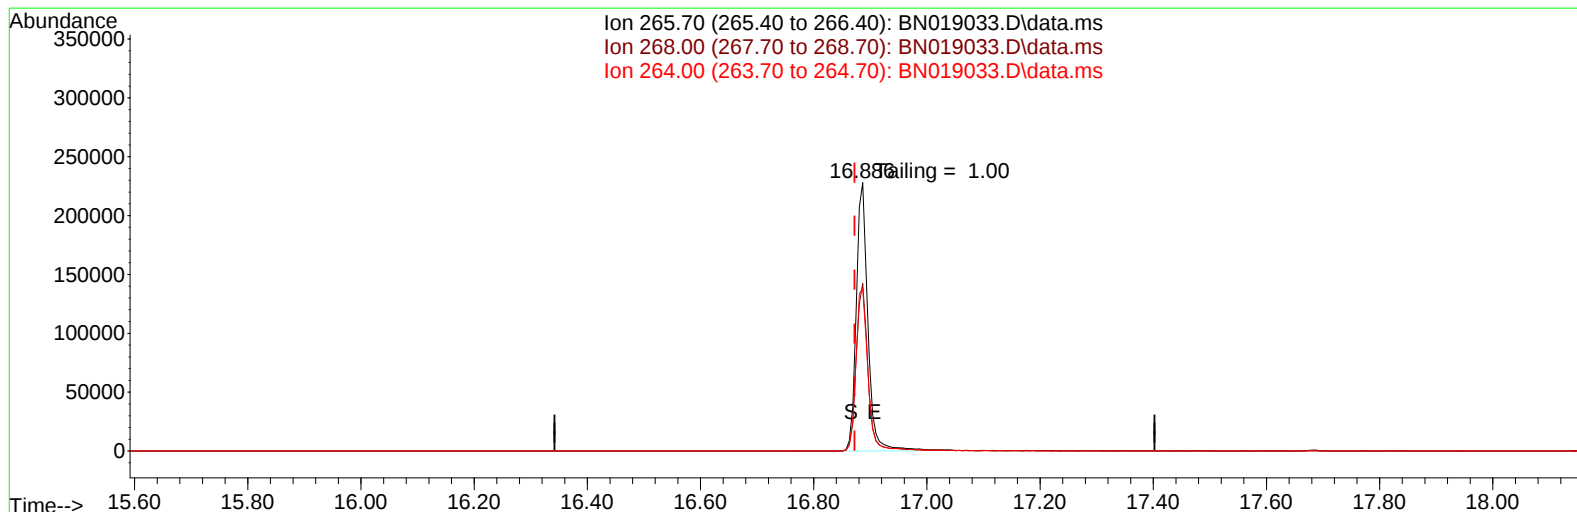

TIC: BN019033.D\data.ms

(70) Pentachlorophenol (C)

16.886min (+ 0.015) 17112.26 ng




response 326197

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.39
264.00	61.60	60.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032122\
Data File : BN019033.D
Acq On : 21 Mar 2022 22:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 22 08:17:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

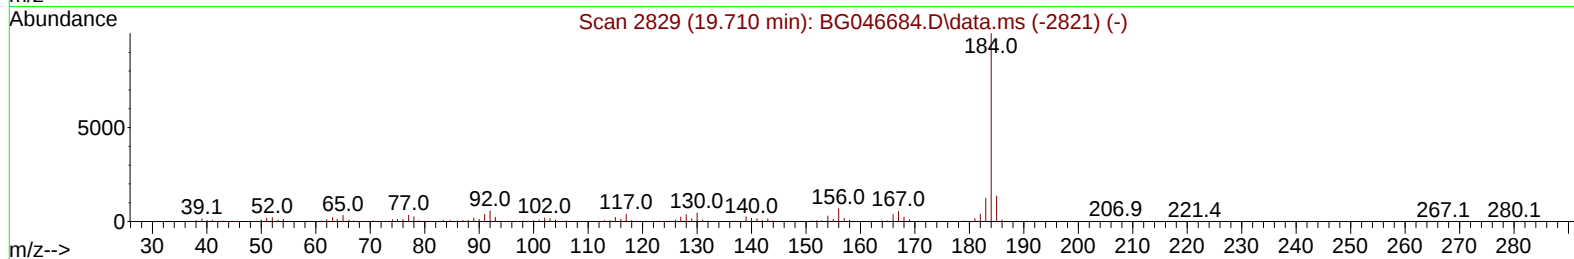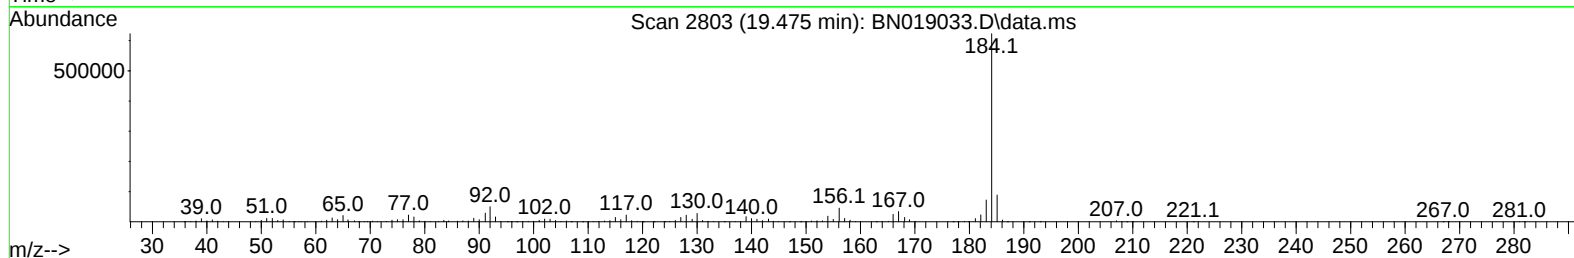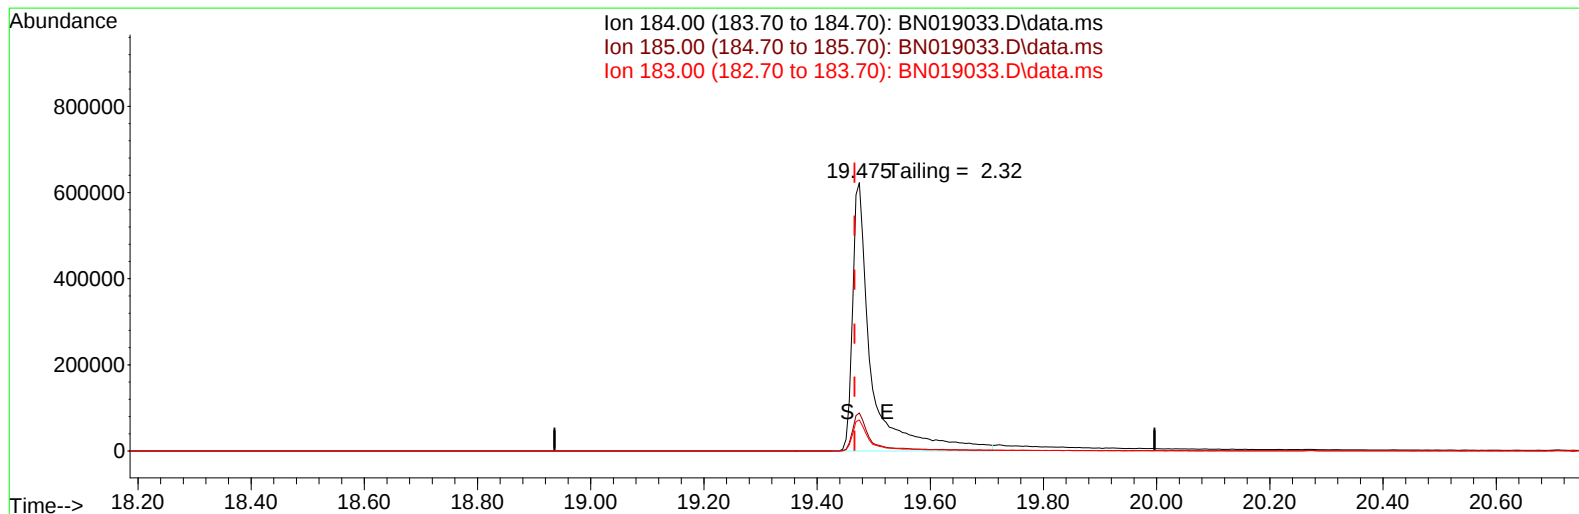

TIC: BN019033.D\data.ms

(77) Benzidine

19.475min (+ 0.009) 0.00 ng

response 1451121

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/21/2022	BNA_N	<u>BN019033.D</u>
Compound Name	Response	Retention Time
DDT	247705	20.71
DDD	414485	20.269
DDE	578	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
415063	662768	62.63

Instrument :
BNA_N
ClientSampleId :
DFTPP