


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032219\
 Data File : BN004889.D
 Acq On : 22 Mar 2019 15:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 20 16:06:20 2019

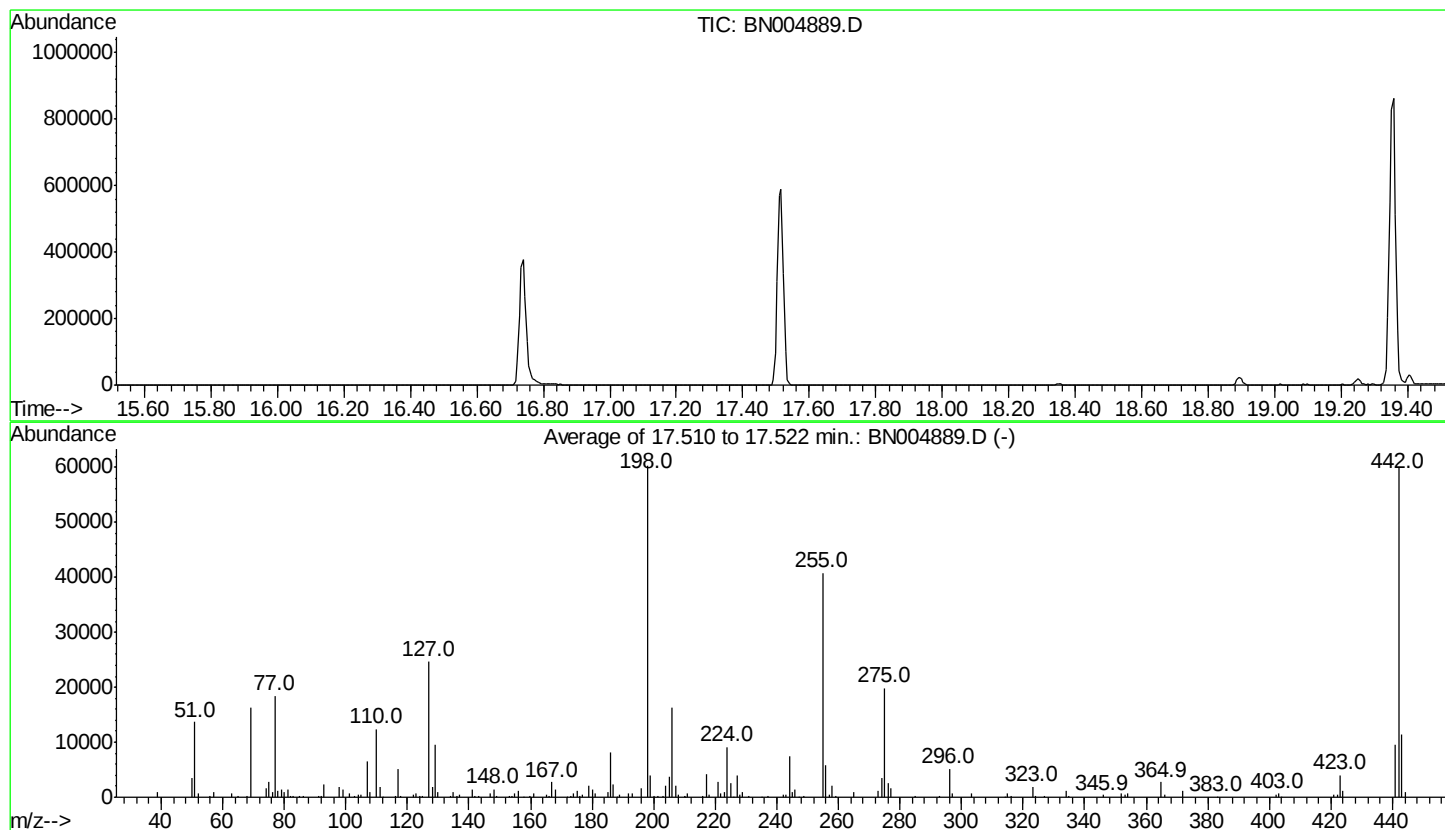

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	13639	PASS
68	69	0.00	2	1.7	279	PASS
69	198	0.00	100	27.1	16342	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.8	24576	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60309	PASS
199	198	5	9	6.7	4069	PASS
275	198	10	60	33.0	19892	PASS
365	198	1	100	4.5	2735	PASS
441	198	0.01	100	16.0	9668	PASS
442	198	50	100	99.5	60032	PASS
443	442	15	24	18.8	11303	PASS