

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
 Data File : BN014016.D
 Acq On : 22 Mar 2021 17:07
 Operator : CG/JU
 Sample : M1736-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DUP02-20210317

Quant Time: Mar 22 17:39:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 19 14:40:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	5241	0.40	ng	0.00
7) Naphthalene-d8	10.480	136	19652	0.40	ng	0.00
13) Acenaphthene-d10	14.321	164	11063	0.40	ng	-0.01
19) Phenanthrene-d10	17.068	188	24679	0.40	ng	# 0.00
29) Chrysene-d12	21.250	240	25359	0.40	ng	# 0.00
36) Perylene-d12	23.458	264	22905	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	1863	0.15	ng	0.00
5) Phenol-d6	6.871	99	1356	0.09	ng	0.00
8) Nitrobenzene-d5	8.845	82	4747	0.36	ng	0.00
11) 2-Methylnaphthalene-d10	12.066	152	11392	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	1456	0.40	ng	0.00
15) 2-Fluorobiphenyl	12.951	172	16139	0.39	ng	0.00
27) Fluoranthene-d10	19.099	212	28882	0.42	ng	0.00
31) Terphenyl-d14	19.700	244	31824	0.57	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.247	88	976	0.14	ng	# 64
12) 2-Methylnaphthalene	12.142	142	1028	0.03	ng	# 92
20) 4,6-Dinitro-2-methylph...	15.463	198	192	0.07	ng	# 1
25) Phenanthrene	17.104	178	1800	0.03	ng	# 92
34) Bis(2-ethylhexyl)phtha...	21.165	149	2629	0.10	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
Data File : BN014016.D
Acq On : 22 Mar 2021 17:07
Operator : CG/JU
Sample : M1736-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DUP02-20210317

Quant Time: Mar 22 17:39:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 19 14:40:09 2021
Response via : Initial Calibration




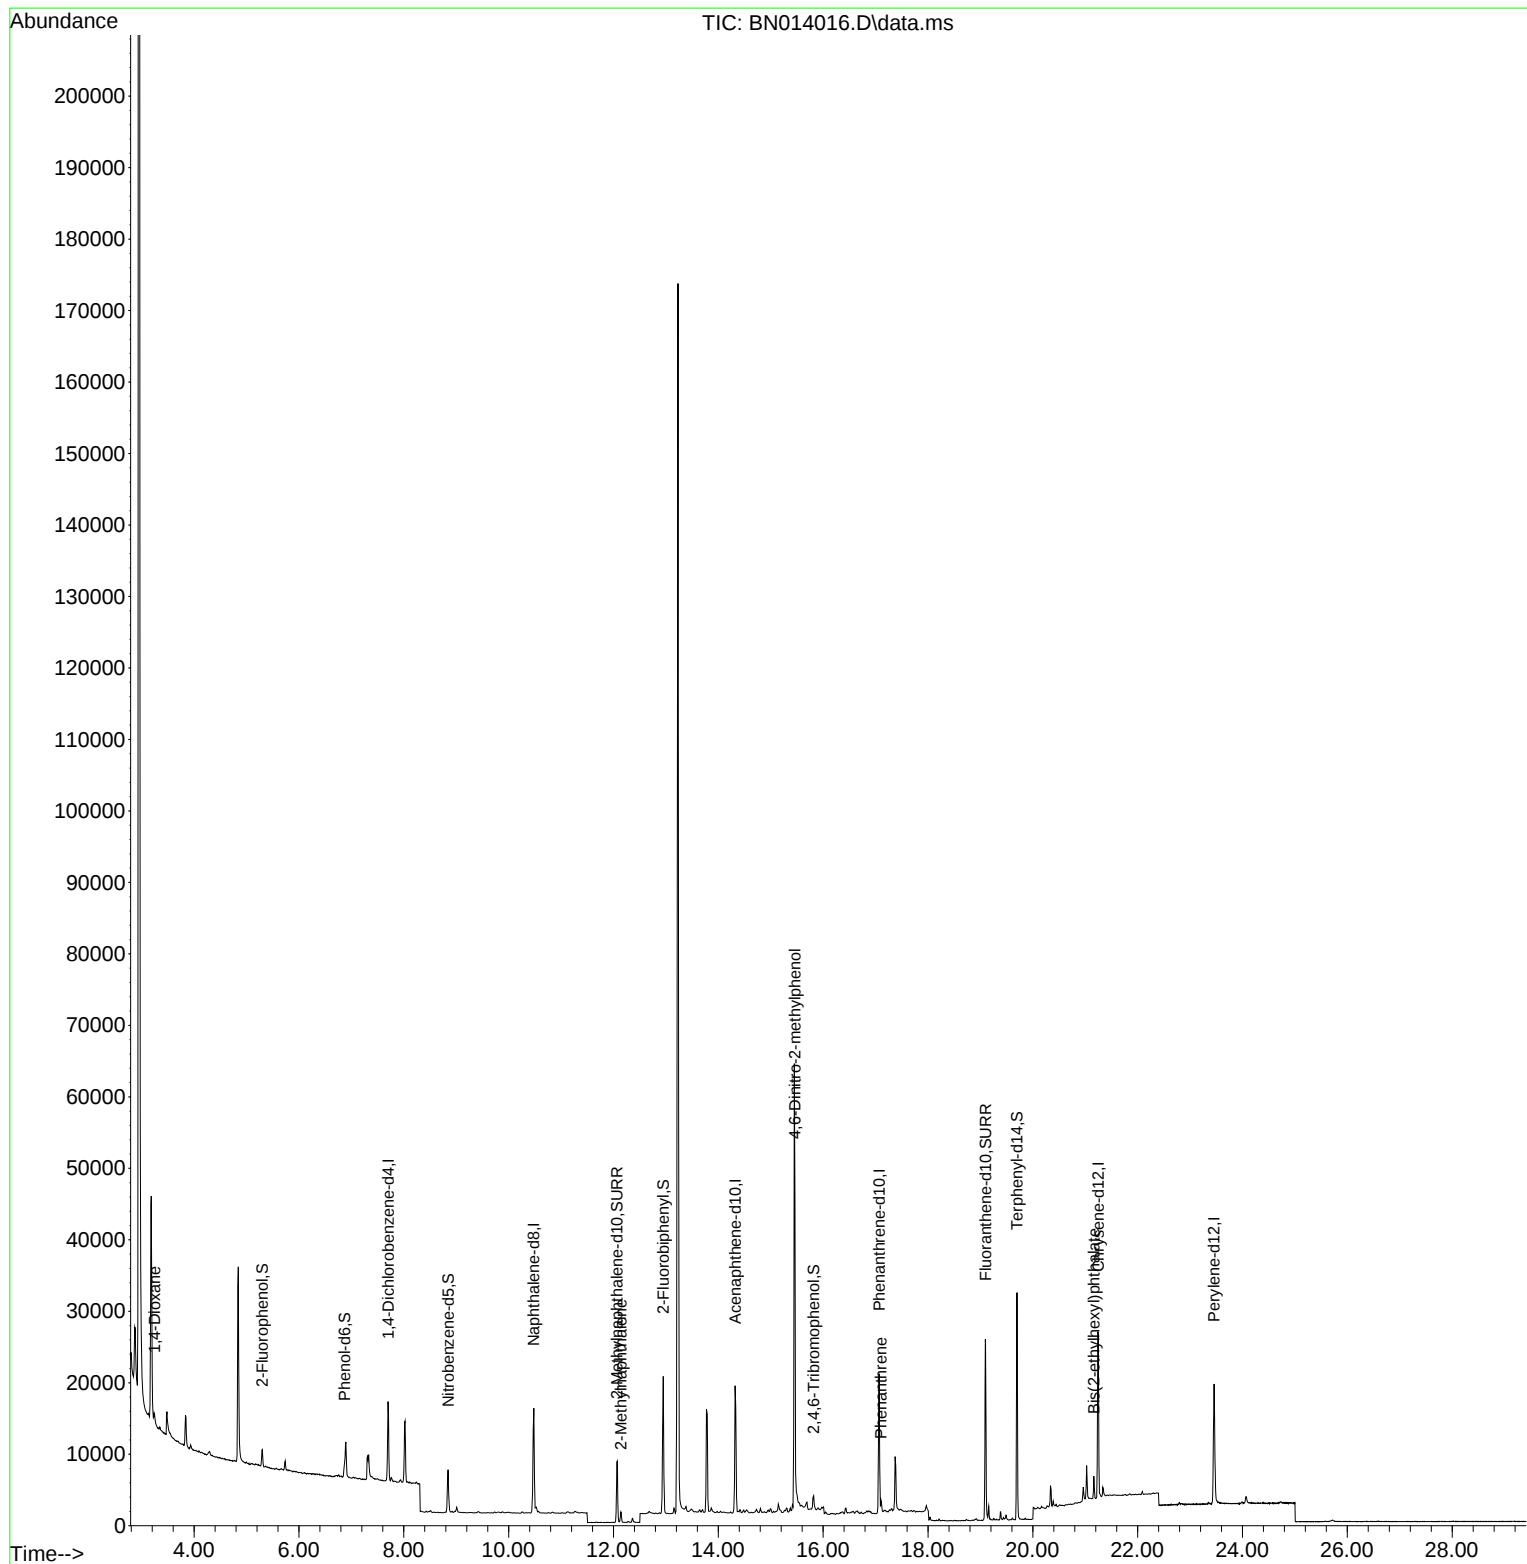




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.700 min Scan# 611
 Delta R.T. 0.000 min
 Lab File: BN014016.D
 Acq: 22 Mar 2021 17:07




Instrument :
 BNA_N
 ClientSampleId :
 DUP02-20210317


Tgt Ion:152 Resp: 5241
 Ion Ratio Lower Upper
 152 100
 150 156.9 121.8 182.8
 115 60.4 46.6 69.8

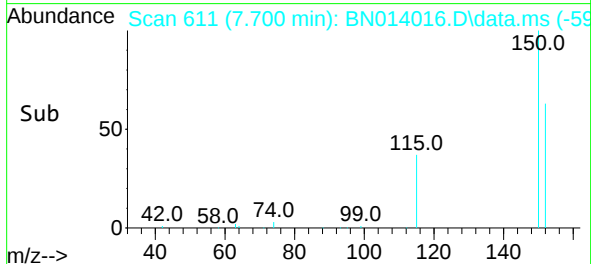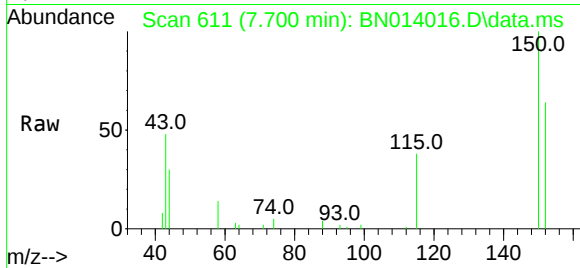

#2
 1,4-Dioxane
 Concen: 0.14 ng
 RT: 3.247 min Scan# 58
 Delta R.T. 0.000 min
 Lab File: BN014016.D
 Acq: 22 Mar 2021 17:07

Tgt Ion: 88 Resp: 976
 Ion Ratio Lower Upper
 88 100
 58 103.8 64.6 96.8#
 43 0.0 26.6 40.0#




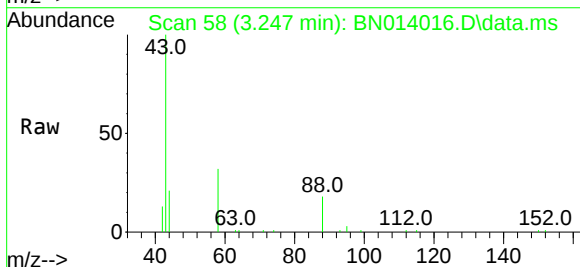


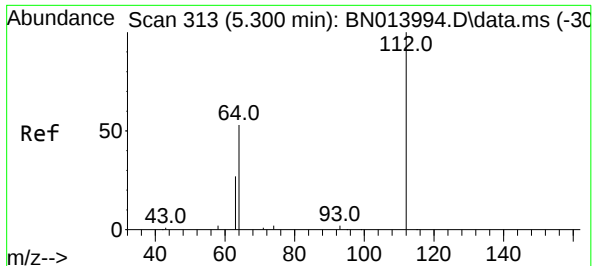

#4
2-Fluorophenol
Concen: 0.15 ng
RT: 5.300 min Scan# 313
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07




Instrument :
BNA_N
ClientSampleId :
DUP02-20210317


Tgt Ion:	112	Resp:	1863
Ion	Ratio	Lower	Upper
112	100		
64	58.6	44.3	66.5
63	31.3	23.0	34.6

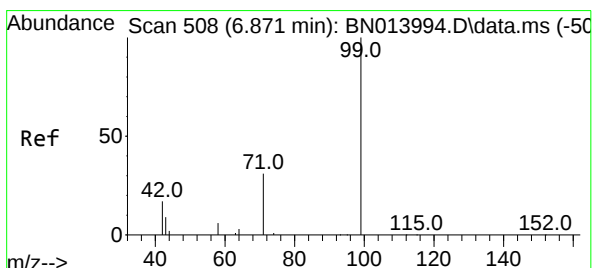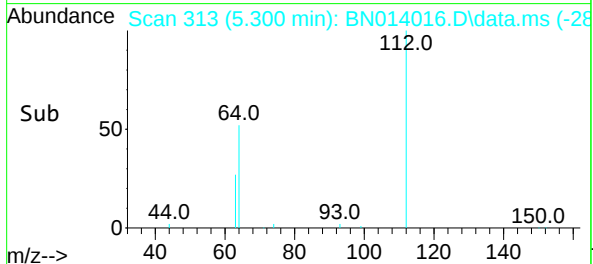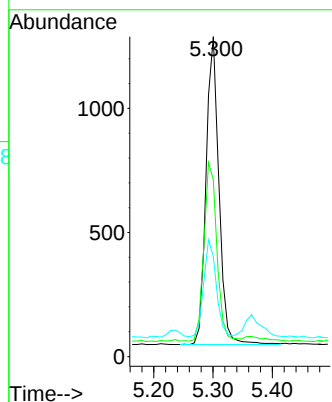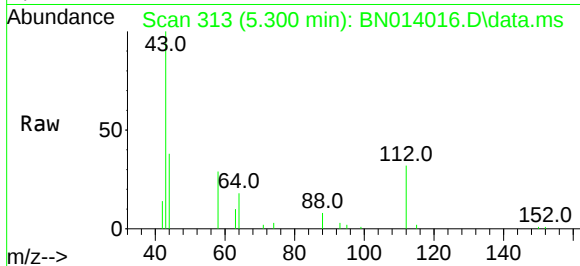

#5
Phenol-d6
Concen: 0.09 ng
RT: 6.871 min Scan# 508
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07

Tgt Ion:	99	Resp:	1356
Ion	Ratio	Lower	Upper
99	100		
42	0.0	15.2	22.8#
71	40.3	26.1	39.1#


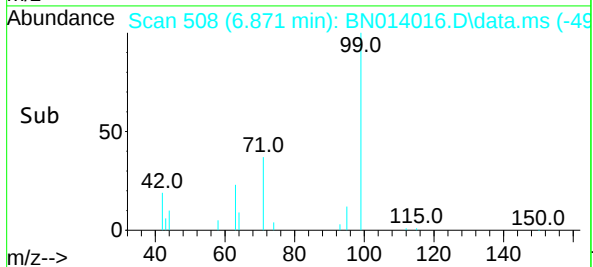
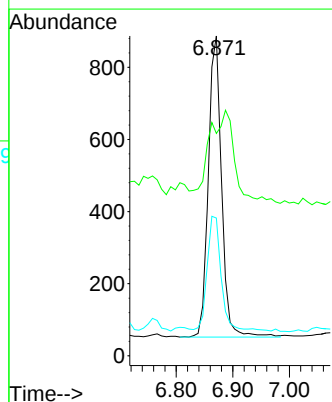
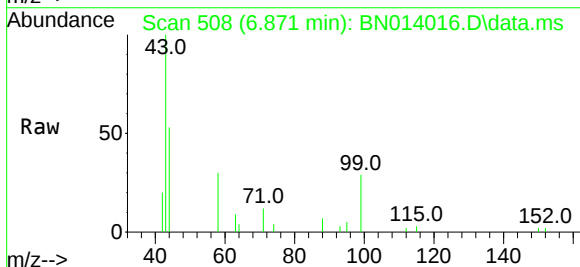




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.480 min Scan# 858
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07




Instrument :
BNA_N
ClientSampleId :
DUP02-20210317


Tgt Ion:	136	Resp:	19652
Ion Ratio	Lower	Upper	
136	100		
137	11.2	9.0	13.6
54	6.5	6.4	9.6
68	5.4	4.5	6.7

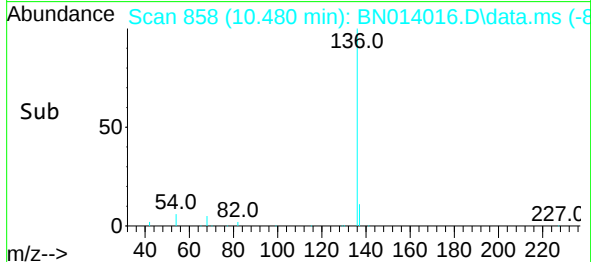

#8
Nitrobenzene-d5
Concen: 0.36 ng
RT: 8.845 min Scan# 729
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07

Tgt Ion:	82	Resp:	4747
Ion Ratio	Lower	Upper	
82	100		
128	40.0	39.2	58.8
54	52.8	40.1	60.1


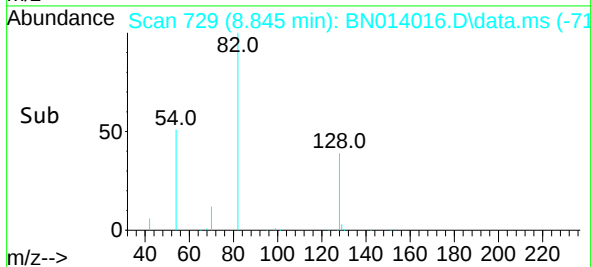

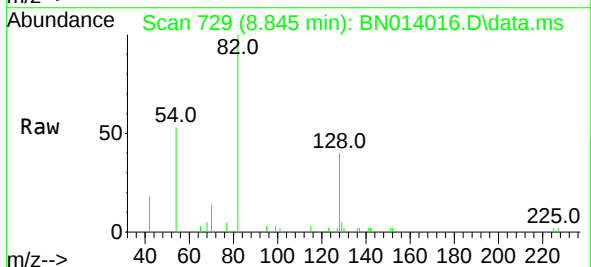




#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.066 min Scan# 1065
Delta R.T. -0.004 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07




Instrument :
BNA_N
ClientSampleId :
DUP02-20210317


Tgt Ion:152 Resp: 11392
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.2

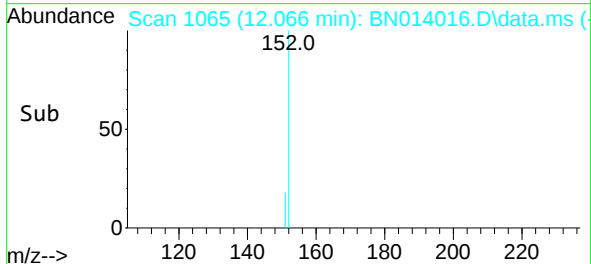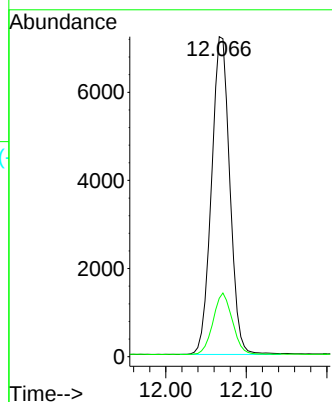

#12
2-Methylnaphthalene
Concen: 0.03 ng
RT: 12.142 min Scan# 1082
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07

Tgt Ion:142 Resp: 1028
Ion Ratio Lower Upper
142 100
141 91.4 70.5 105.7
115 44.6 27.4 41.0#


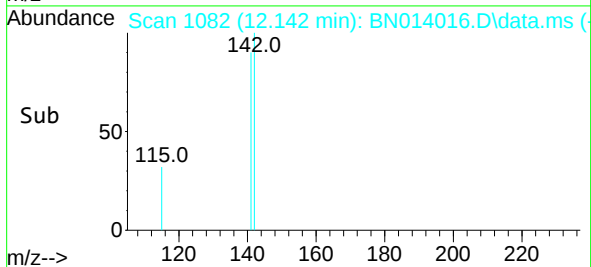
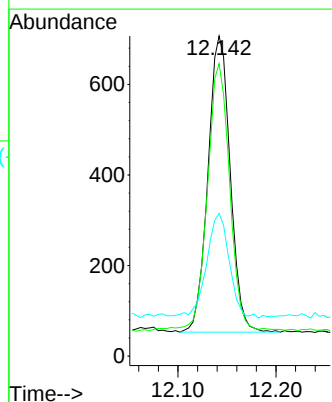
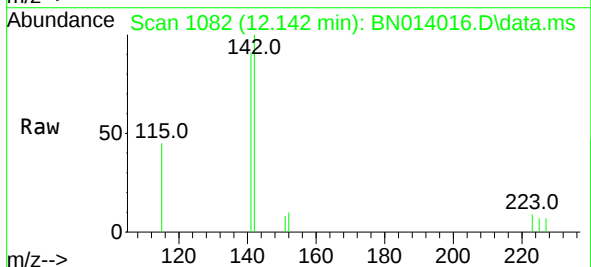




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.321 min Scan# 1307
Delta R.T. -0.013 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07




Instrument :
BNA_N
ClientSampleId :
DUP02-20210317


Tgt Ion:164 Resp: 11063
Ion Ratio Lower Upper
164 100
162 103.7 79.6 119.4
160 48.5 36.0 54.0

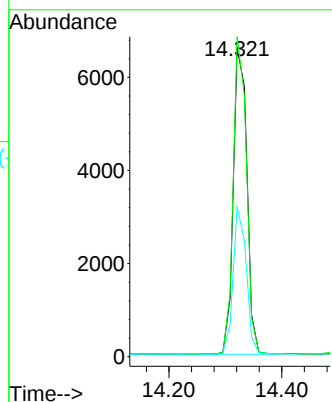

#14
2,4,6-Tribromophenol
Concen: 0.40 ng
RT: 15.818 min Scan# 1425
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07

Tgt Ion:330 Resp: 1456
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.1 26.8 40.2


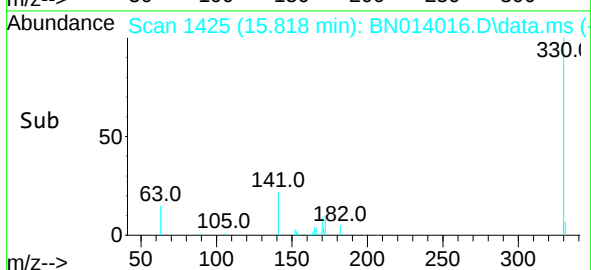






#15
2-Fluorobiphenyl
Concen: 0.39 ng
RT: 12.951 min Scan# 1199
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07




Instrument :
BNA_N
ClientSampleId :
DUP02-20210317


Tgt Ion:172 Resp: 16139
Ion Ratio Lower Upper
172 100
171 34.1 28.6 42.8
170 22.5 18.9 28.3

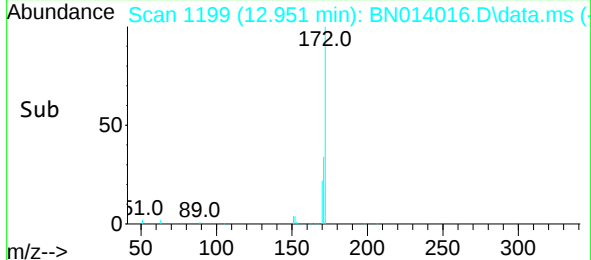

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.068 min Scan# 1527
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07

Tgt Ion:188 Resp: 24679
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.5 9.0 13.6#


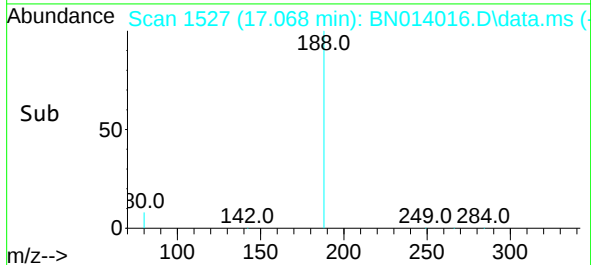

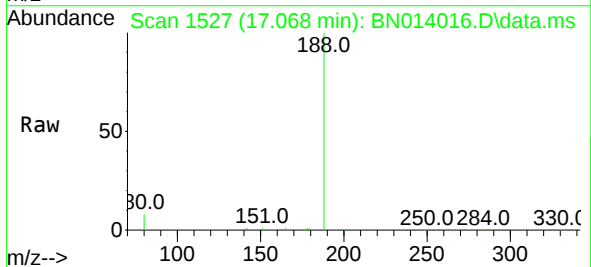


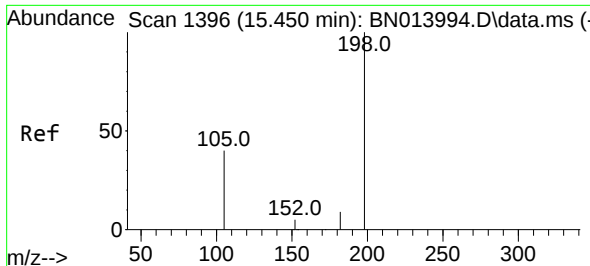

#20
4,6-Dinitro-2-methylphenol
Concen: 0.07 ng
RT: 15.463 min Scan# 1397
Delta R.T. 0.013 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07




Instrument :
BNA_N
ClientSampleId :
DUP02-20210317


Tgt Ion:198 Resp: 192
Ion Ratio Lower Upper
198 100
51 1302.9 61.7 92.5#
105 2166.9 33.0 49.6#

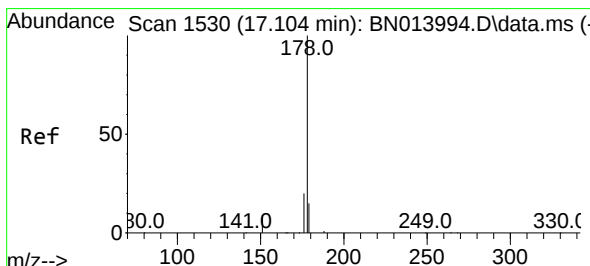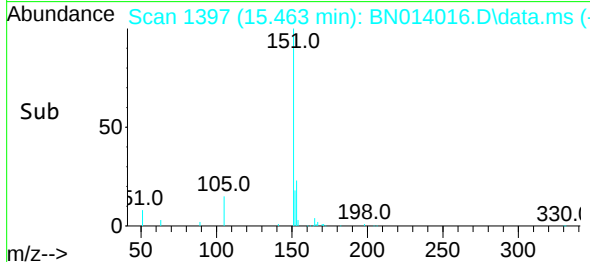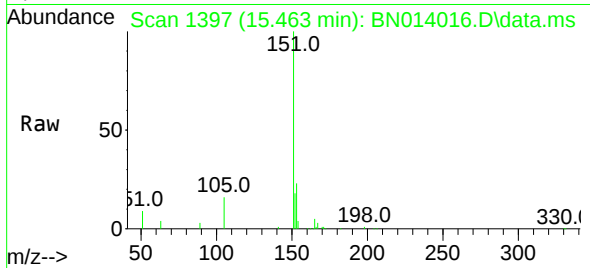

#25
Phenanthrene
Concen: 0.03 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07

Tgt Ion:178 Resp: 1800
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.4
179 22.6 12.3 18.5#


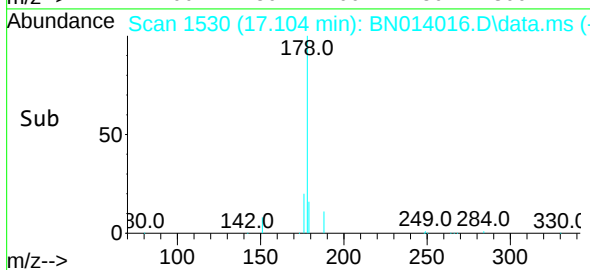

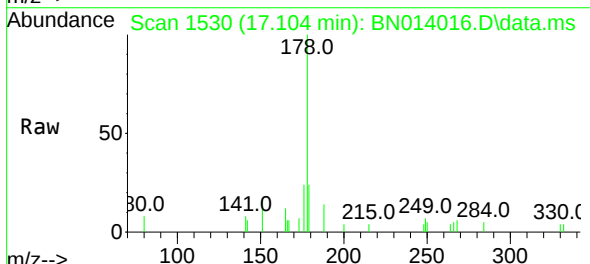




#27
Fluoranthene-d10
Concen: 0.42 ng
RT: 19.099 min Scan# 1823
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07




Instrument :
BNA_N
ClientSampleId :
DUP02-20210317


Tgt Ion:212 Resp: 28882
Ion Ratio Lower Upper
212 100
106 13.1 9.7 14.5
104 7.3 5.5 8.3

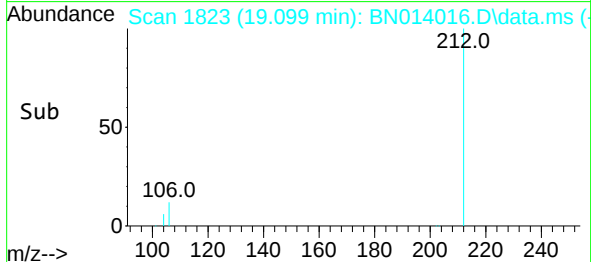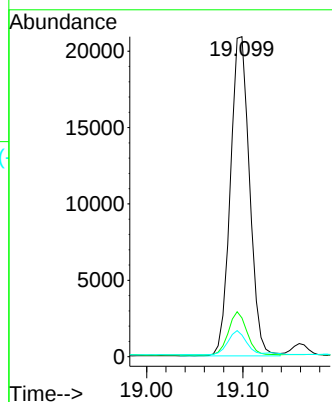

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014016.D
Acq: 22 Mar 2021 17:07

Tgt Ion:240 Resp: 25359
Ion Ratio Lower Upper
240 100
120 6.6 10.2 15.4#
236 25.1 21.3 31.9


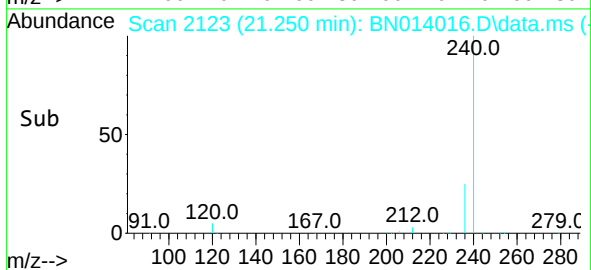

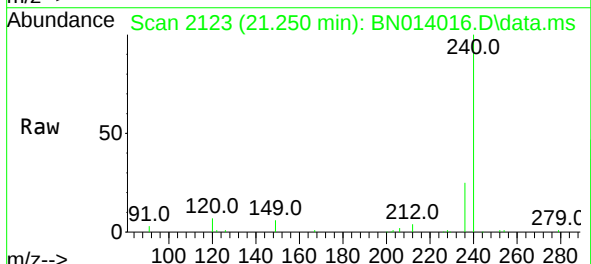




#31
 Terphenyl-d14
 Concen: 0.57 ng
 RT: 19.700 min Scan# 1944
 Delta R.T. 0.000 min
 Lab File: BN014016.D
 Acq: 22 Mar 2021 17:07




Instrument :
 BNA_N
 ClientSampleId :
 DUP02-20210317


Tgt Ion:244 Resp: 31824
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.1 9.1
 122 10.9 9.8 14.8

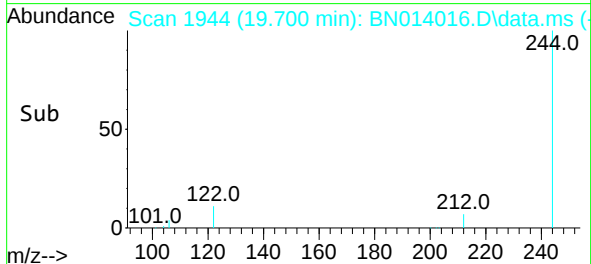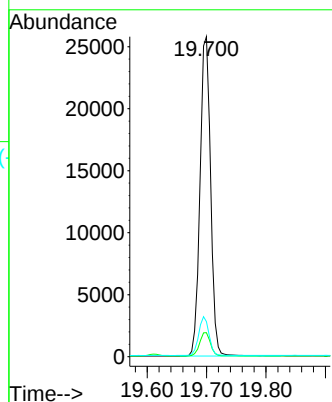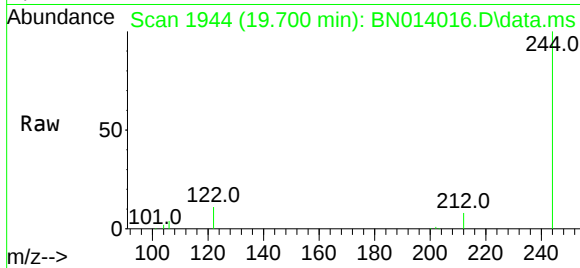

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.10 ng
 RT: 21.165 min Scan# 2115
 Delta R.T. 0.000 min
 Lab File: BN014016.D
 Acq: 22 Mar 2021 17:07


Tgt Ion:149 Resp: 2629
 Ion Ratio Lower Upper
 149 100
 167 29.3 22.1 33.1
 279 4.5 3.5 5.3

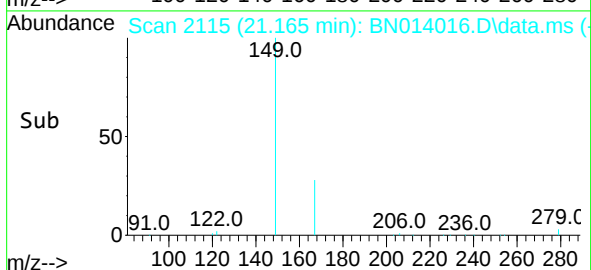

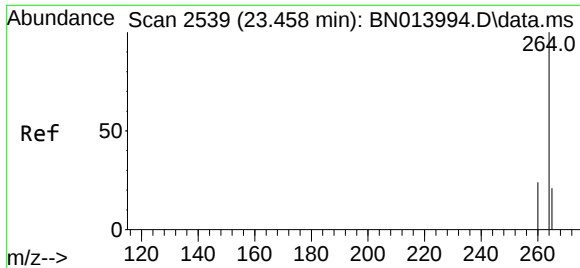

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.458 min Scan# 2539
 Delta R.T. 0.000 min
 Lab File: BN014016.D
 Acq: 22 Mar 2021 17:07

Instrument :
 BNA_N
 ClientSampleId :
 DUP02-20210317

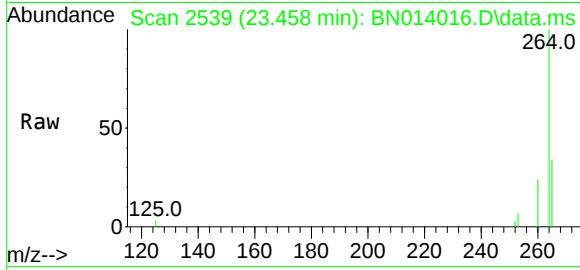

Tgt Ion:264 Resp: 22905

Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.3	28.9
265	33.9	66.2	99.4#

