
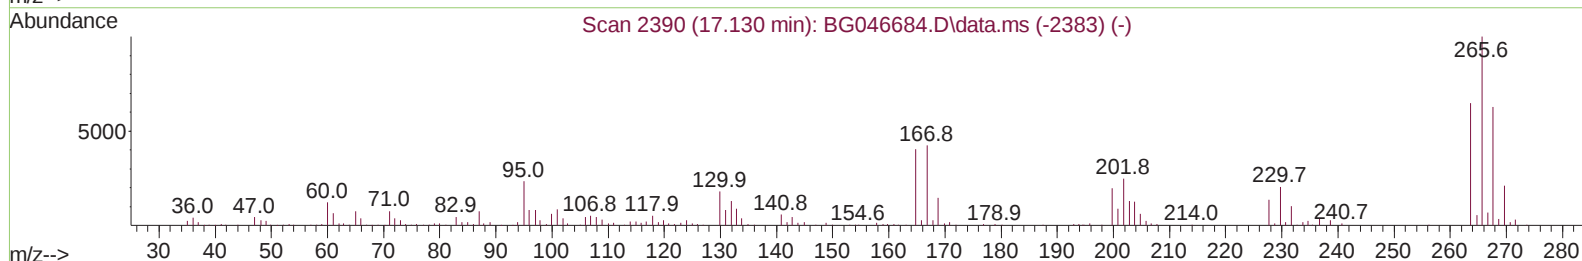
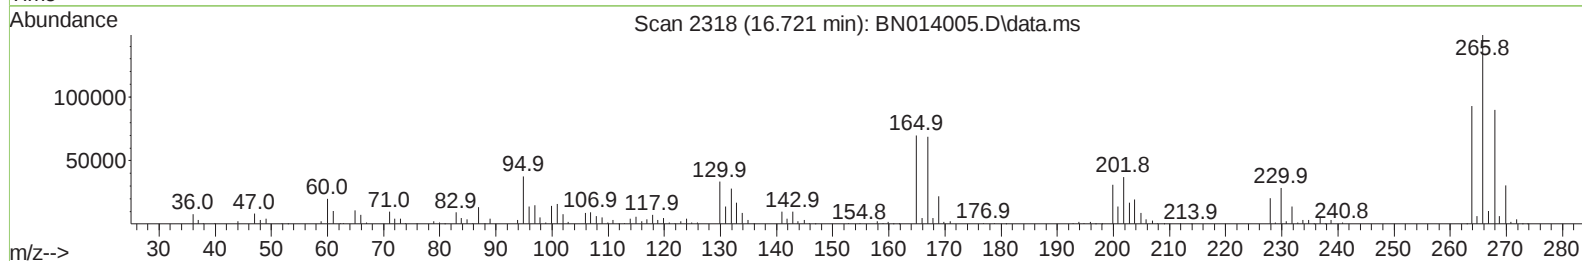


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
Data File : BN014005.D
Acq On : 22 Mar 2021 09:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 10:23:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

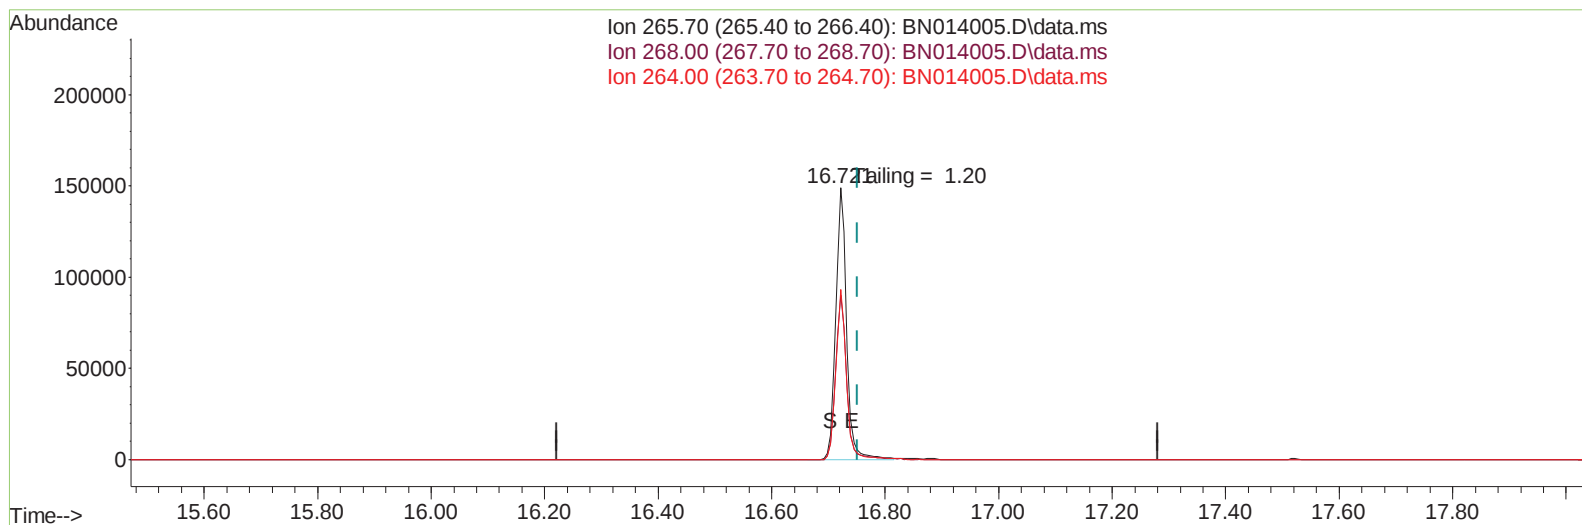

TIC: BN014005.D\data.ms

(70) Pentachlorophenol (C)




16.721min (-0.030) 21012.73 ng

response 198048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.57
264.00	61.60	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
Data File : BN014005.D
Acq On : 22 Mar 2021 09:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 10:23:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

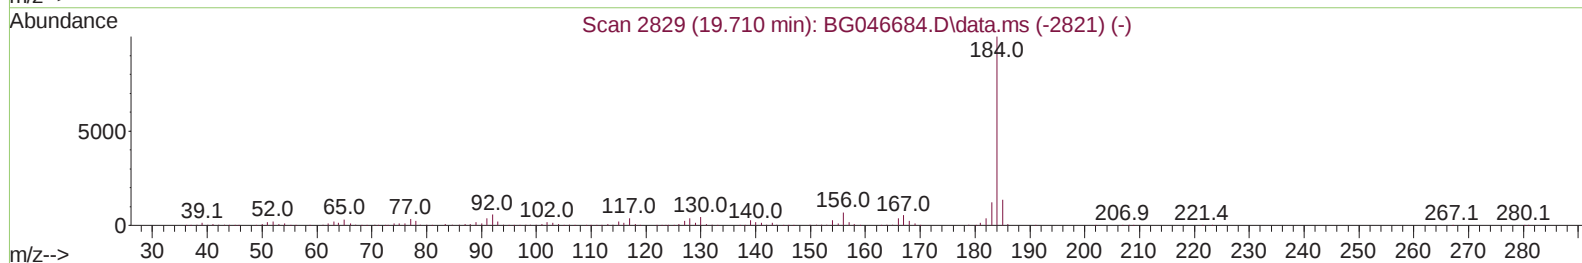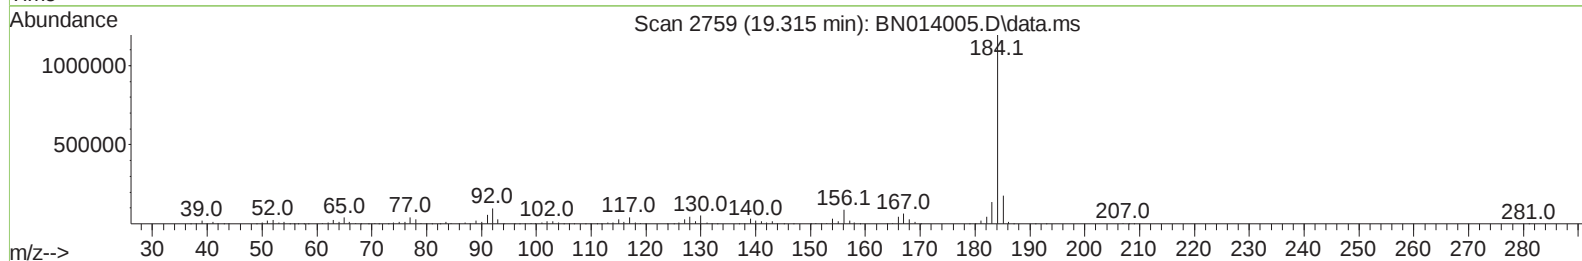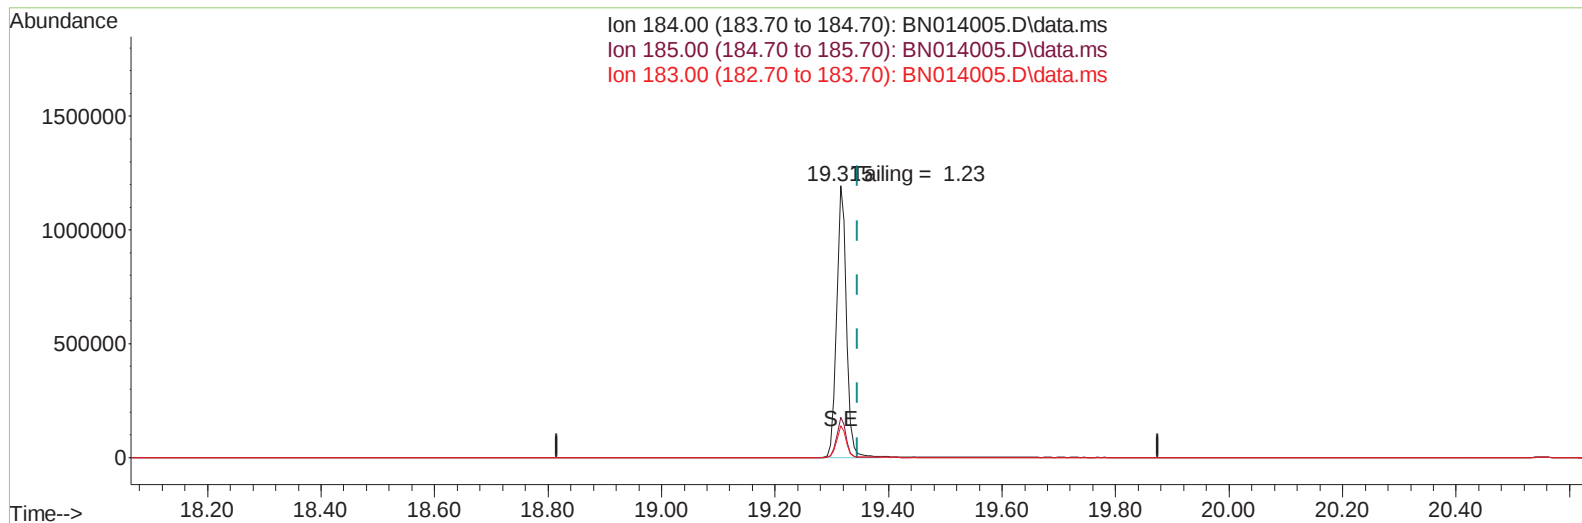

TIC: BN014005.D\data.ms

(77) Benzidine

19.315min (-0.030) 0.00 ng

response 1451437

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.82
183.00	13.20	11.70
0.00	0.00	0.00