
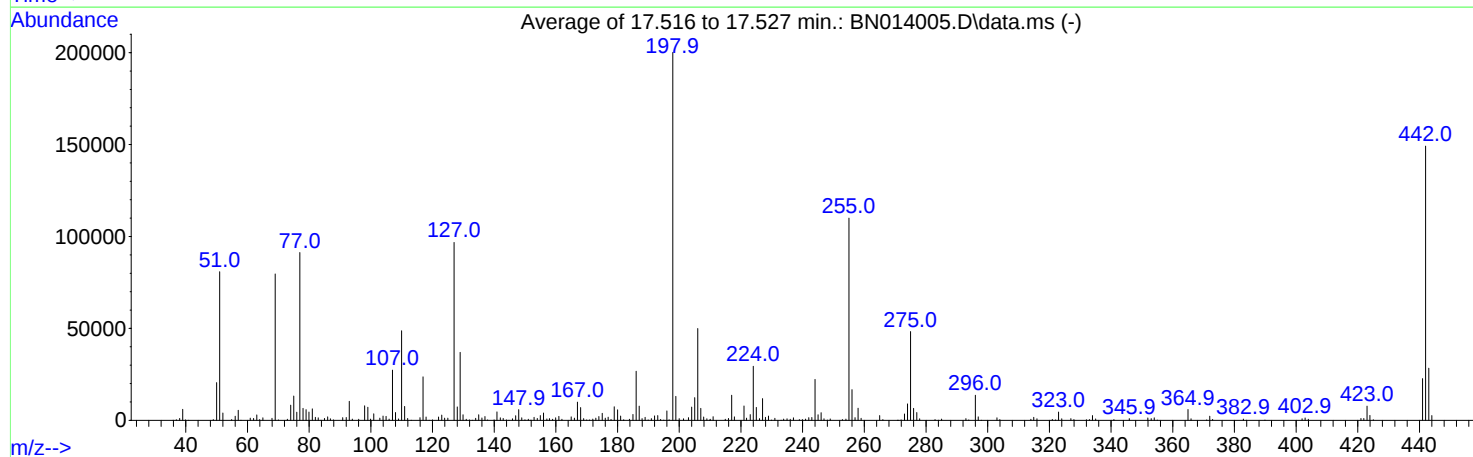


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
 Data File : BN014005.D
 Acq On : 22 Mar 2021 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

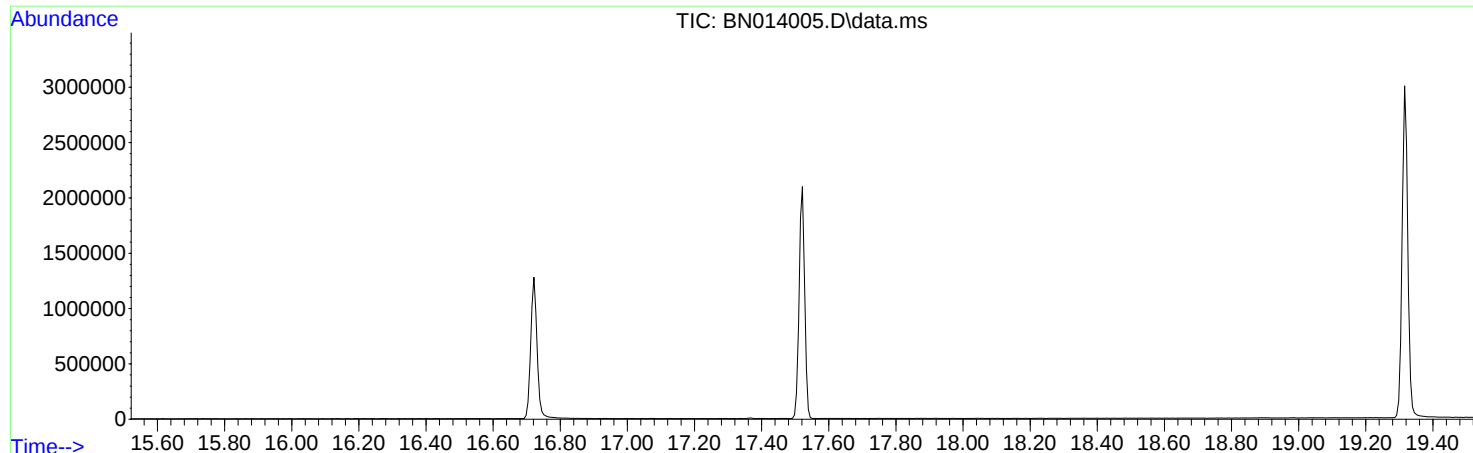




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	80824	PASS
68	69	0.00	2	1.4	1144	PASS
69	198	0.00	100	39.8	79605	PASS
70	69	0.00	2	0.4	304	PASS
127	198	10	80	48.4	96773	PASS
197	198	0.00	2	0.2	366	PASS
198	198	100	100	100.0	200064	PASS
199	198	5	9	6.5	13040	PASS
275	198	10	60	24.1	48285	PASS
365	198	1	100	3.0	5906	PASS
441	198	0.01	100	11.3	22680	PASS
442	442	50	100	100.0	149192	PASS
443	442	15	24	19.0	28339	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
Data File : BN014005.D
Acq On : 22 Mar 2021 09:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 22 10:23:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

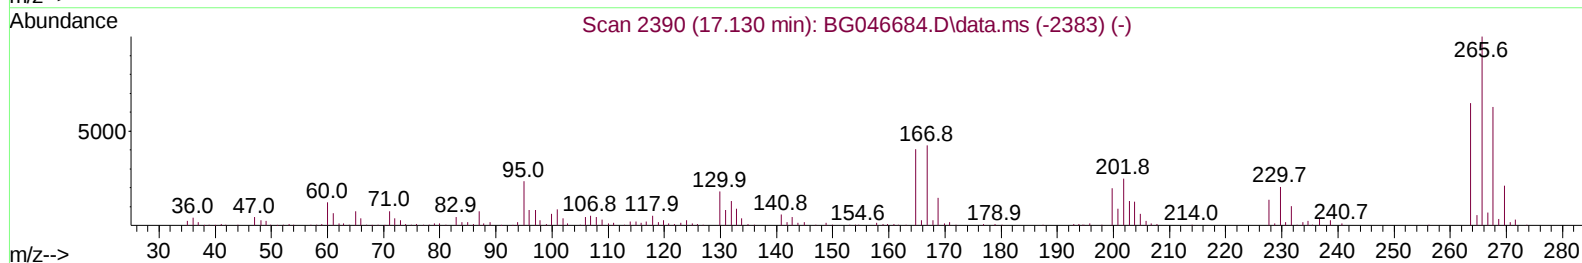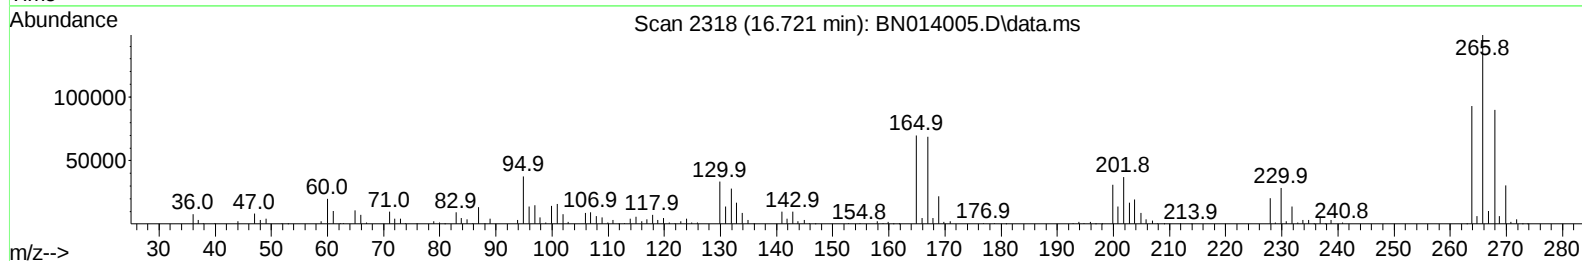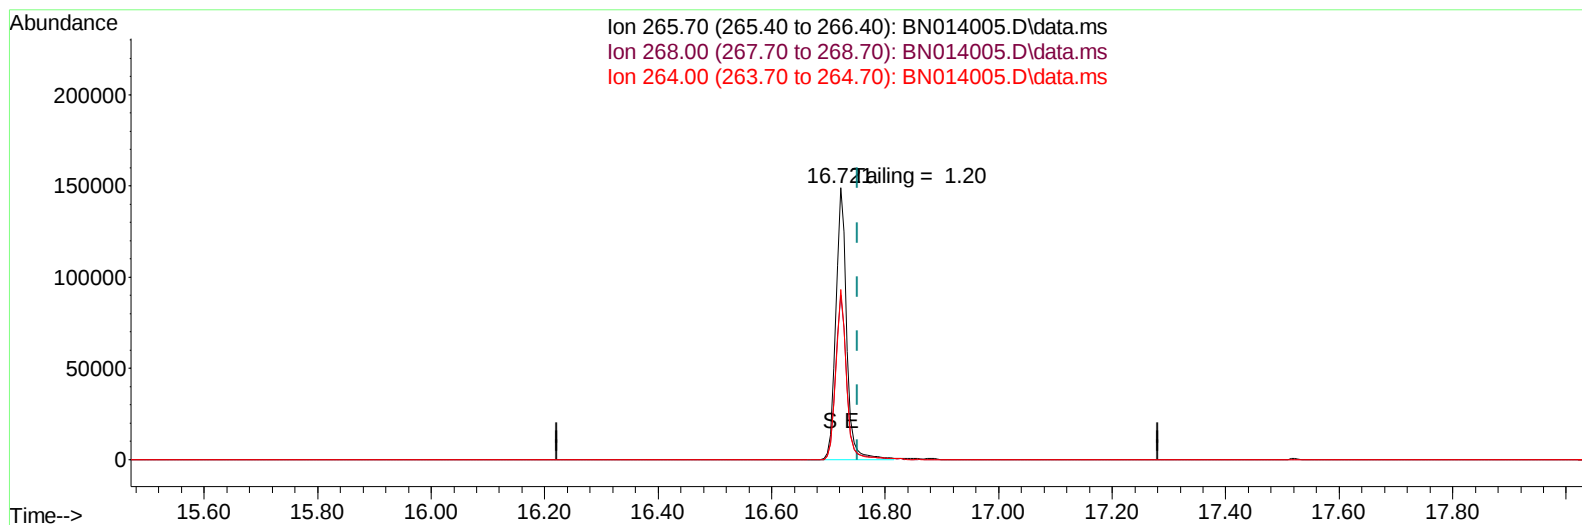

TIC: BN014005.D\data.ms

(70) Pentachloropheno1 (C)

16.721min (-0.030) 21012.73 ng




response 198048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.57
264.00	61.60	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
Data File : BN014005.D
Acq On : 22 Mar 2021 09:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 22 10:23:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

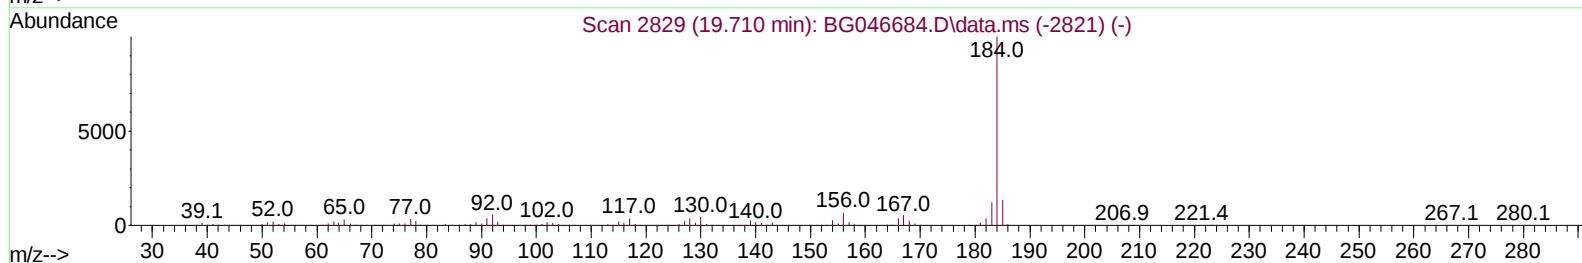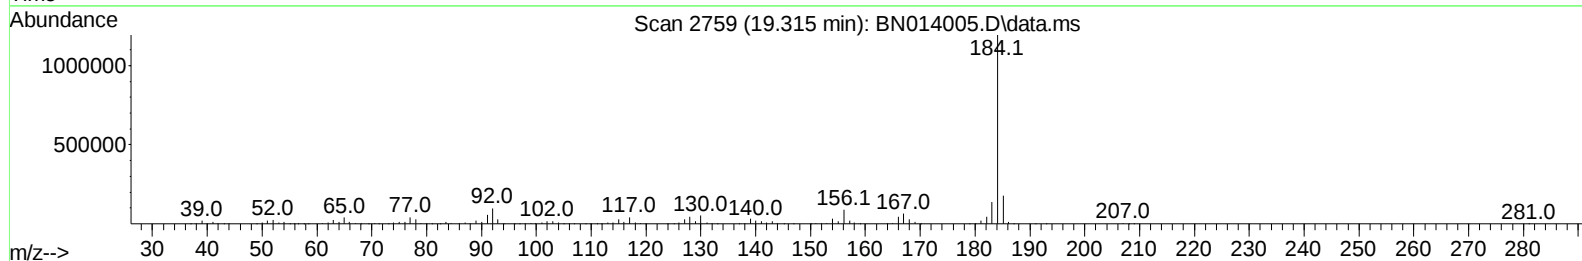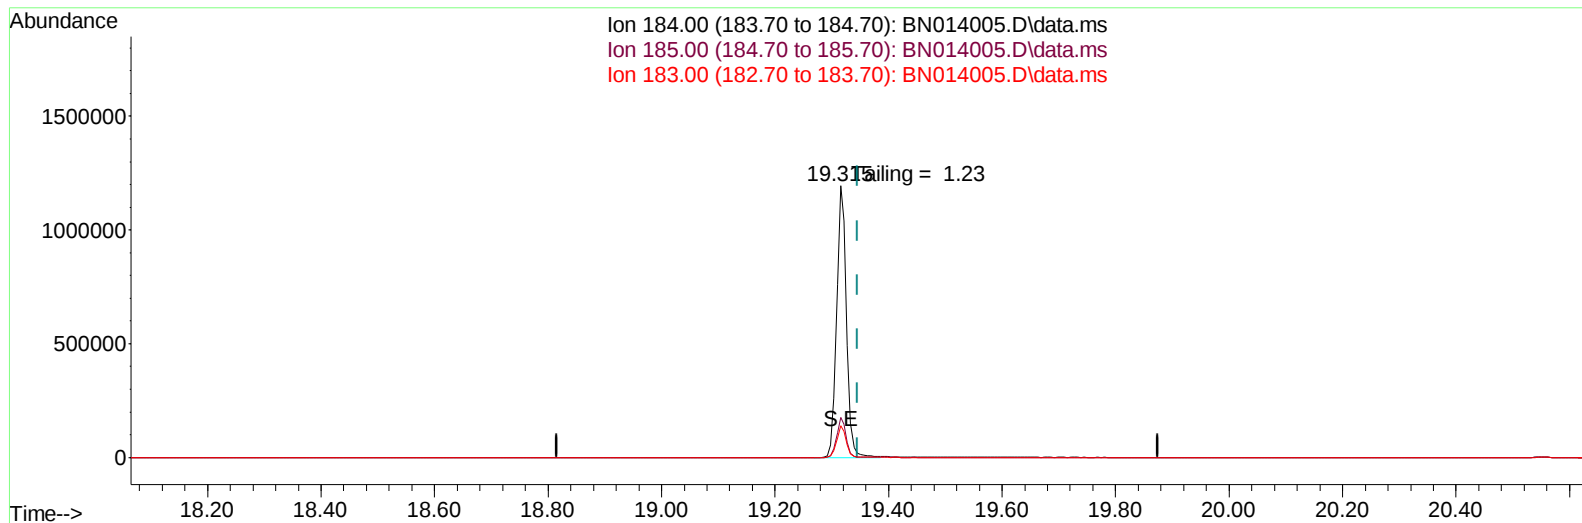

TIC: BN014005.D\data.ms

(77) Benzidine

19.315min (-0.030) 0.00 ng

response 1451437

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.82
183.00	13.20	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/22/2021	BNA_N	<u>BN014005.D</u>
Compound Name	Response	Retention Time
DDT	690693	20.55
DDD	1308	20.11
DDE	666	19.6
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1974	692667	0.28

Instrument :
BNA_N
ClientSampleId :
DFTPP