
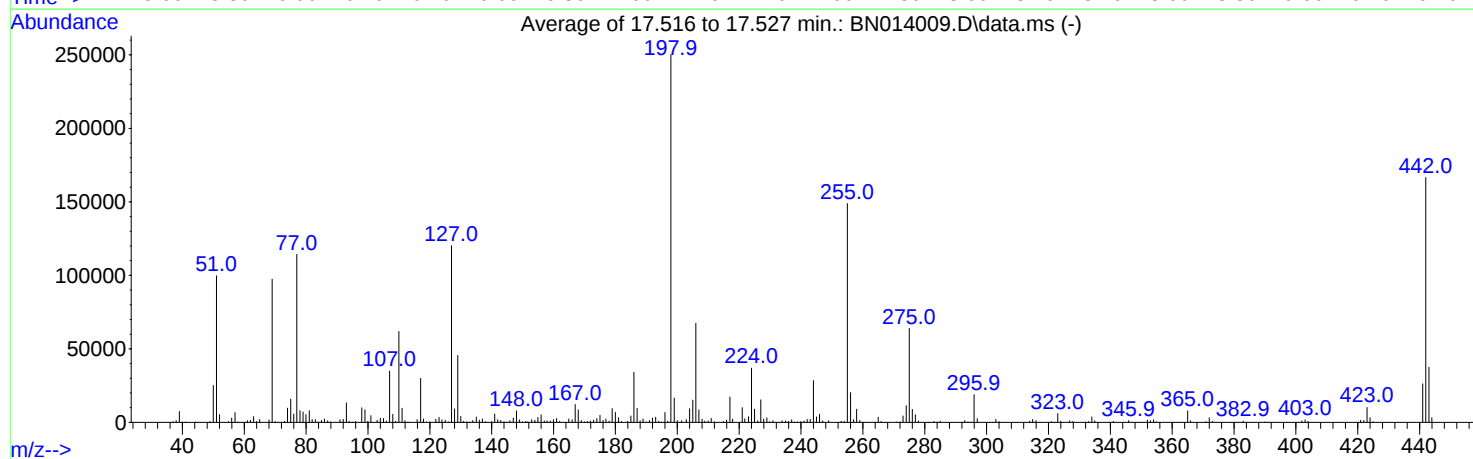


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
 Data File : BN014009.D
 Acq On : 22 Mar 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

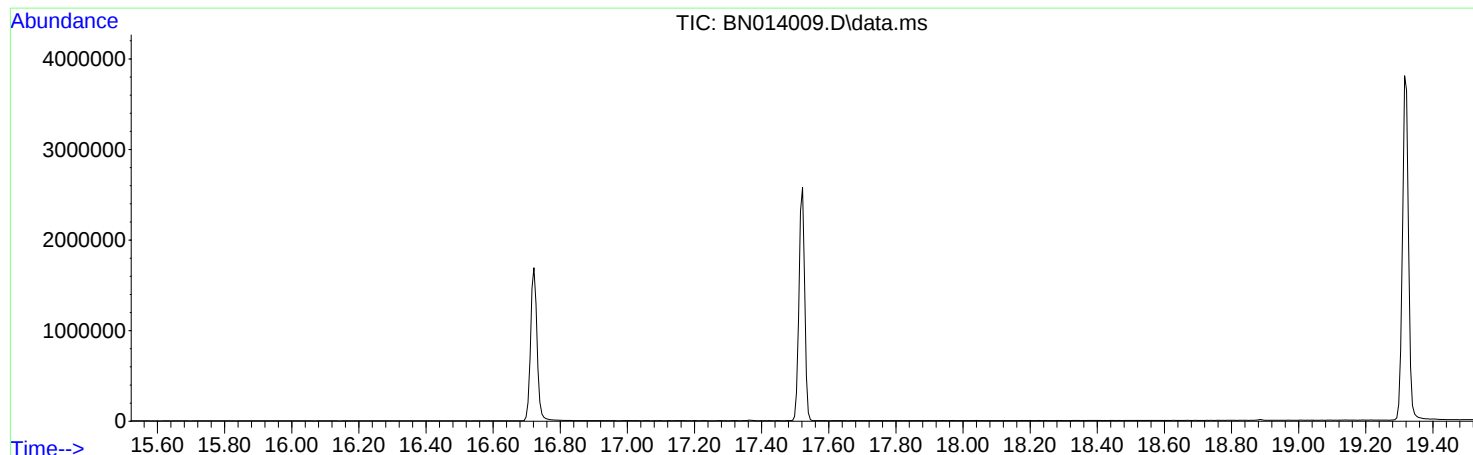




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	99755	PASS
68	69	0.00	2	1.7	1658	PASS
69	198	0.00	100	38.9	97461	PASS
70	69	0.00	2	0.5	535	PASS
127	198	10	80	48.0	120165	PASS
197	198	0.00	2	0.2	616	PASS
198	198	100	100	100.0	250261	PASS
199	198	5	9	6.6	16510	PASS
275	198	10	60	25.5	63888	PASS
365	198	1	100	3.1	7851	PASS
441	198	0.01	100	10.5	26240	PASS
442	442	50	100	100.0	166509	PASS
443	442	15	24	22.5	37461	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
 Data File : BN014009.D
 Acq On : 22 Mar 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 13:30:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 05 13:12:06 2021
 Response via : Initial Calibration

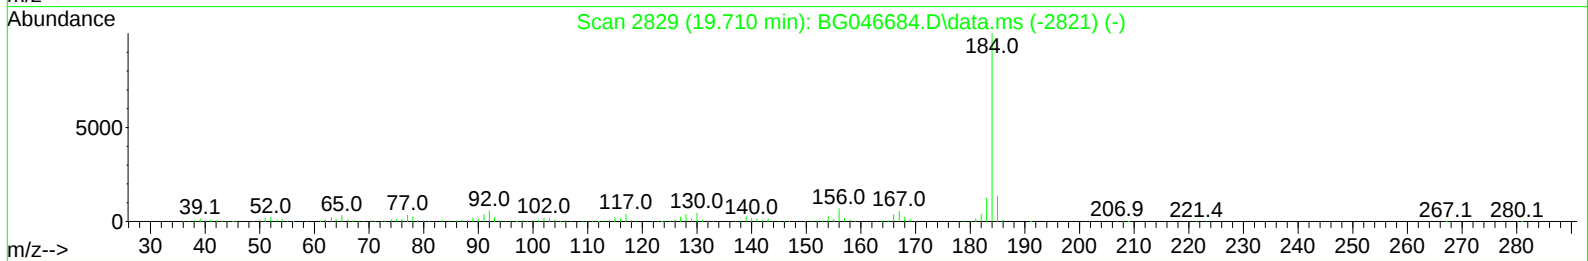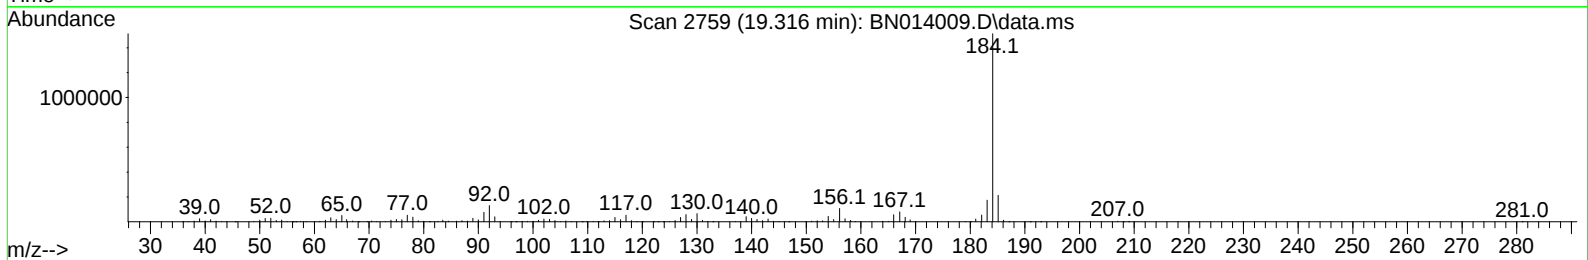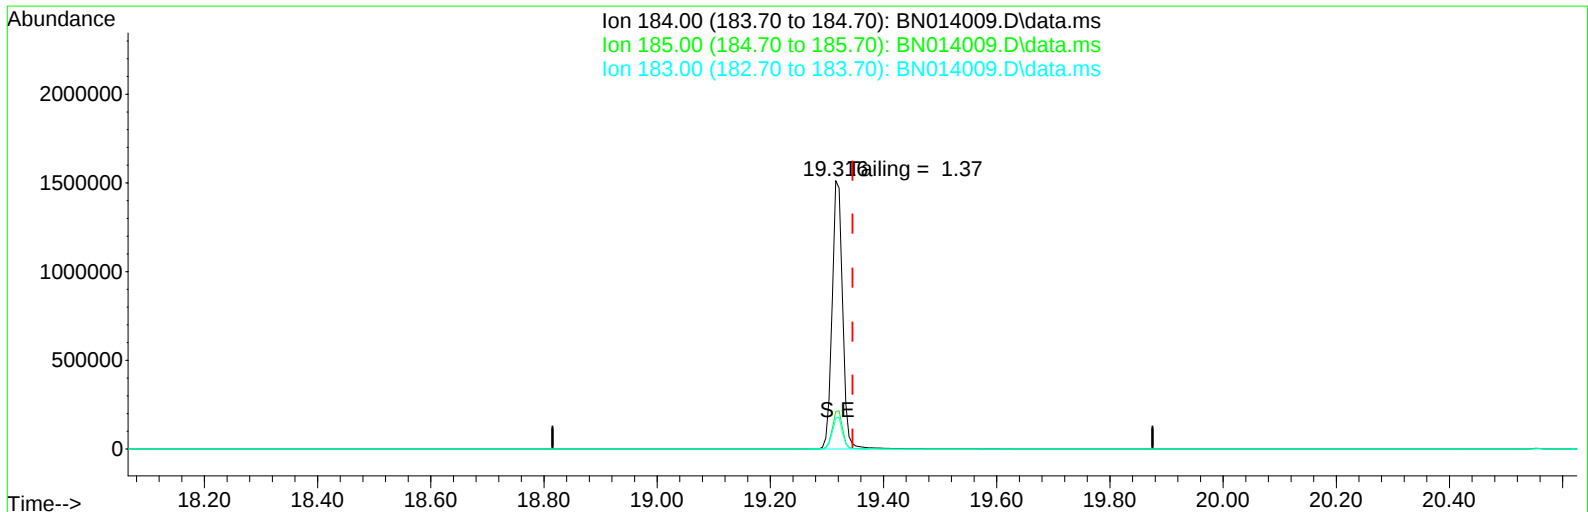

TIC: BN014009.D\data.ms

(77) Benzidine

19.316min (-0.029) 0.00 ng




response 1943679

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
 Data File : BN014009.D
 Acq On : 22 Mar 2021 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 13:30:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 05 13:12:06 2021
 Response via : Initial Calibration

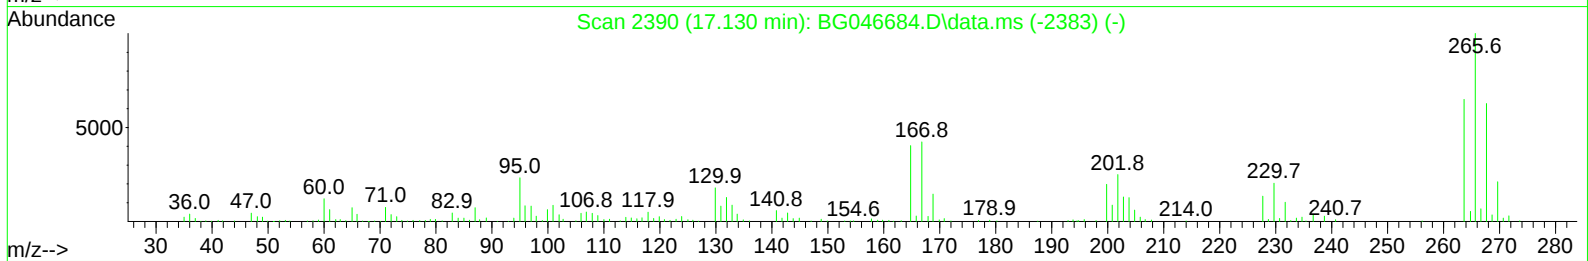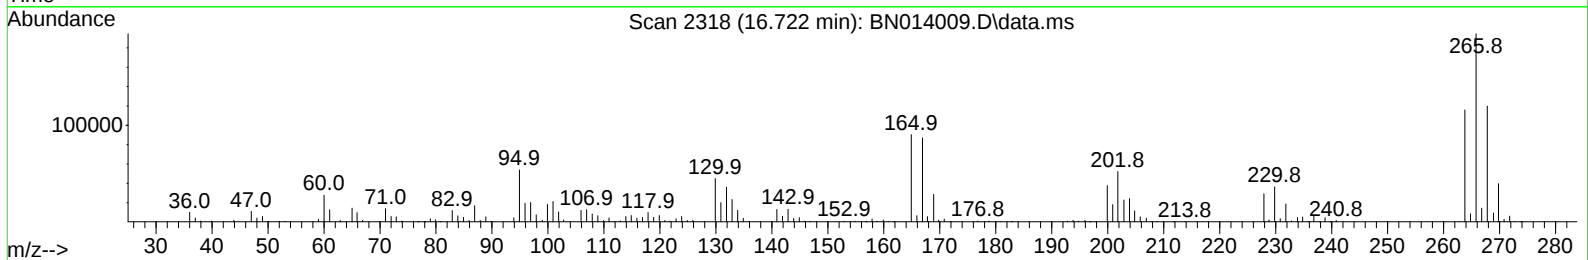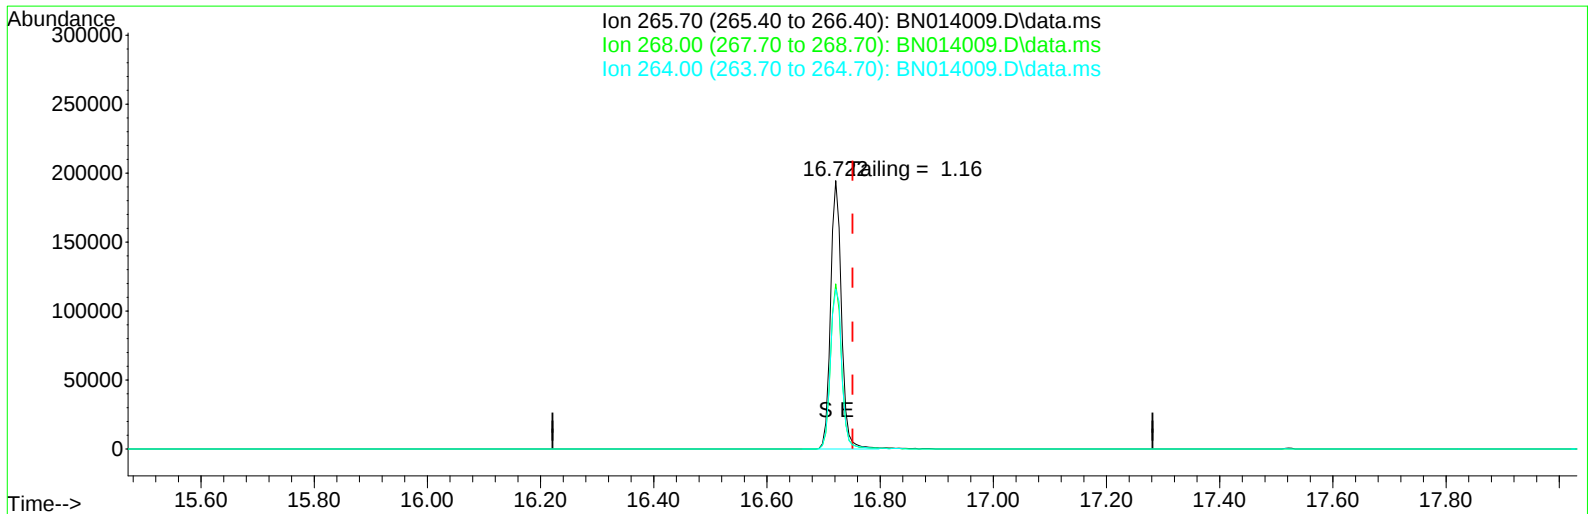

TIC: BN014009.D\data.ms

(70) Pentachlorophenol (C)

16.722min (-0.029) 22536.71 ng

response 259634

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.57
264.00	61.60	59.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/22/2021	BNA_N	<u>BN014009.D</u>
Compound Name	Response	Retention Time
DDT	919825	20.55
DDD	2873	20.11
DDE	931	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3804	923629	0.41