
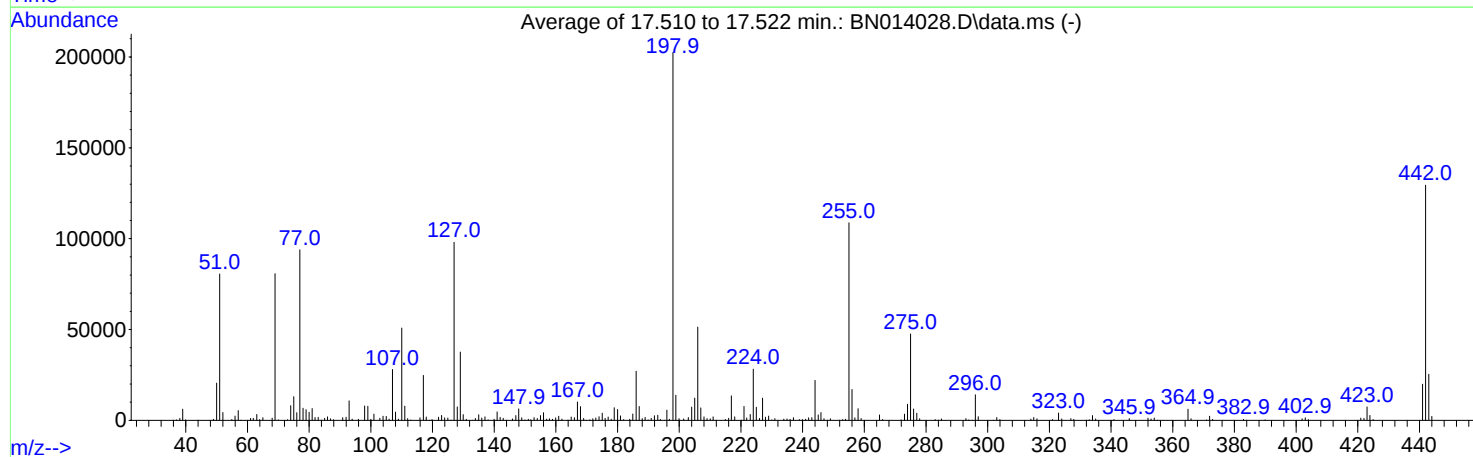


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
 Data File : BN014028.D
 Acq On : 23 Mar 2021 00:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

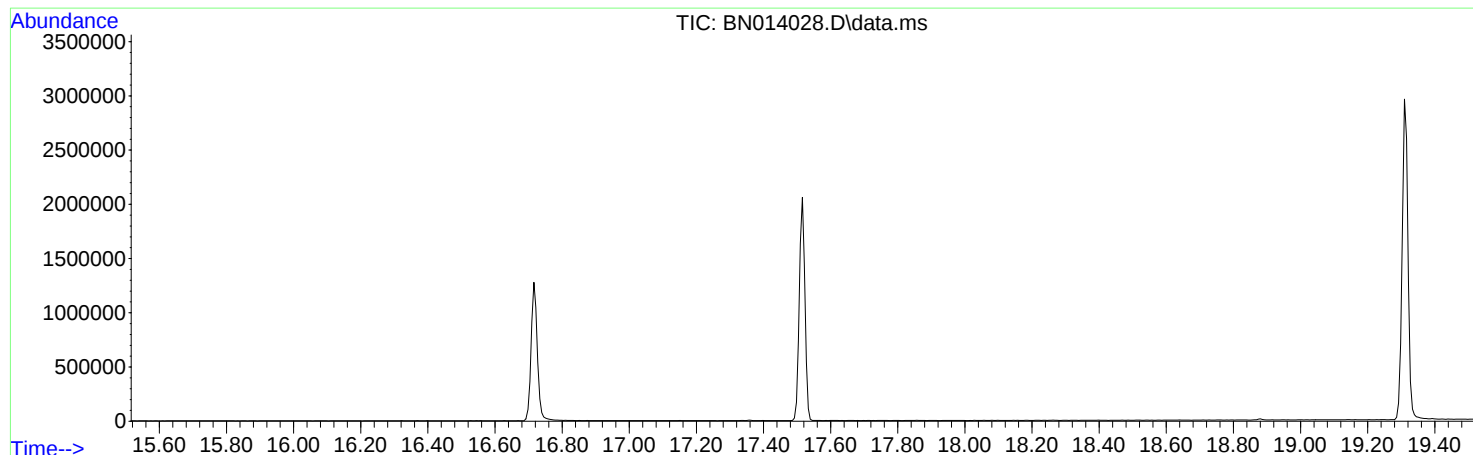




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	80595	PASS
68	69	0.00	2	1.6	1267	PASS
69	198	0.00	100	39.9	80731	PASS
70	69	0.00	2	0.4	289	PASS
127	198	10	80	48.4	97981	PASS
197	198	0.00	2	0.3	615	PASS
198	198	100	100	100.0	202453	PASS
199	198	5	9	6.8	13812	PASS
275	198	10	60	23.5	47539	PASS
365	198	1	100	3.0	6135	PASS
441	198	0.01	100	9.8	19926	PASS
442	442	50	100	100.0	129491	PASS
443	442	15	24	19.6	25381	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
Data File : BN014028.D
Acq On : 23 Mar 2021 00:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 23 01:27:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

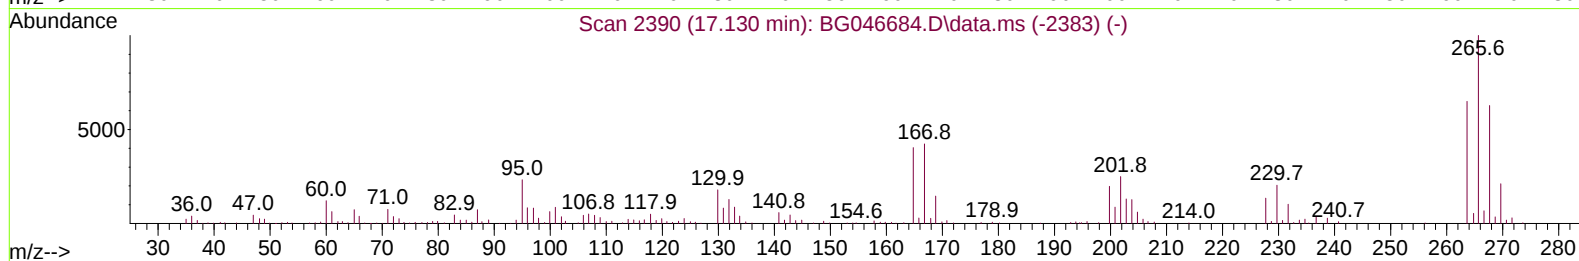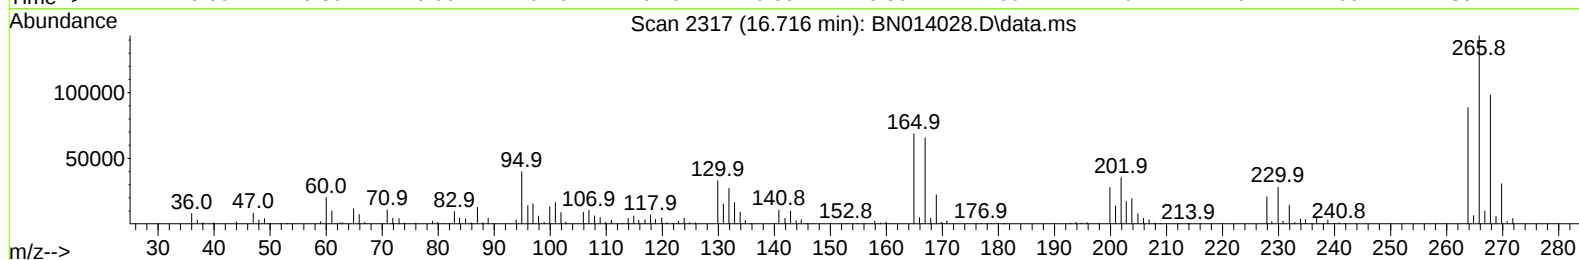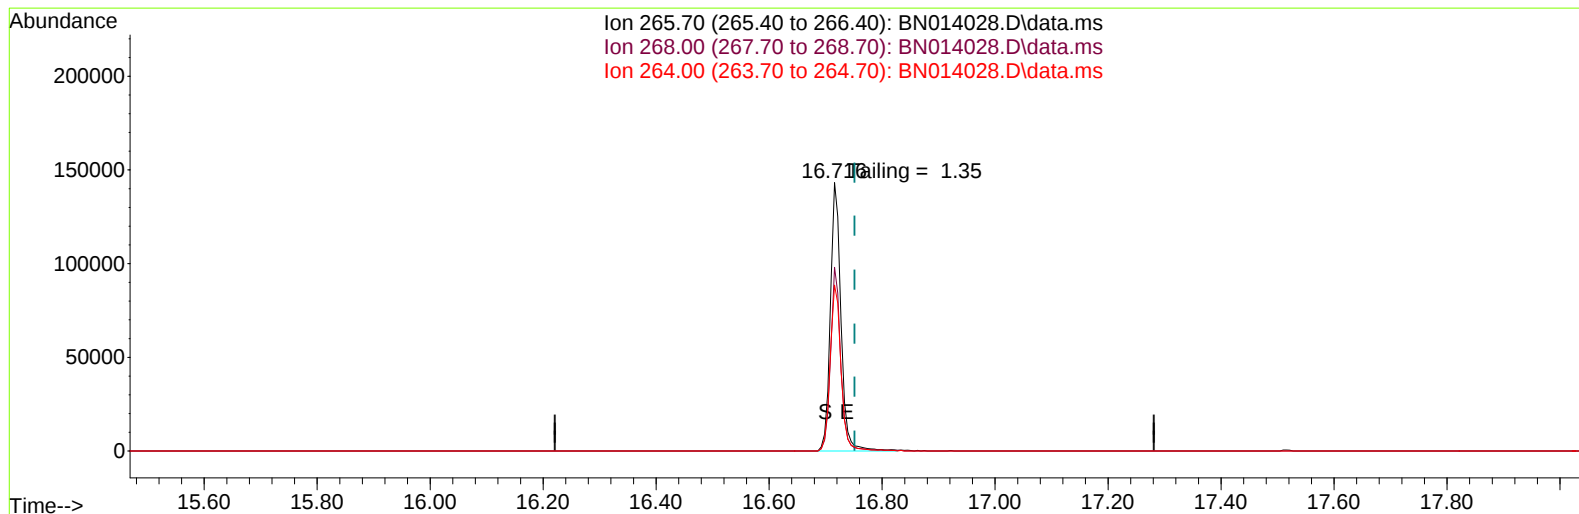

TIC: BN014028.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.035) 19698.83 ng




response 187674

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.48
264.00	61.60	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032221\
Data File : BN014028.D
Acq On : 23 Mar 2021 00:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 23 01:27:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

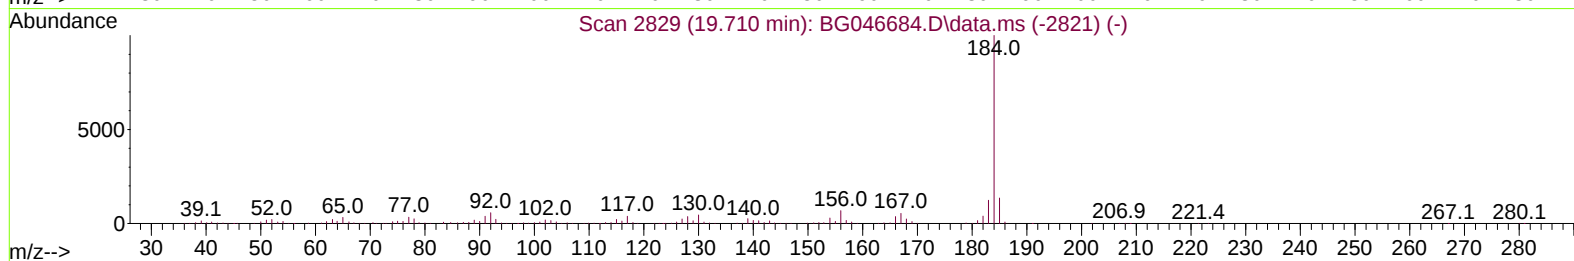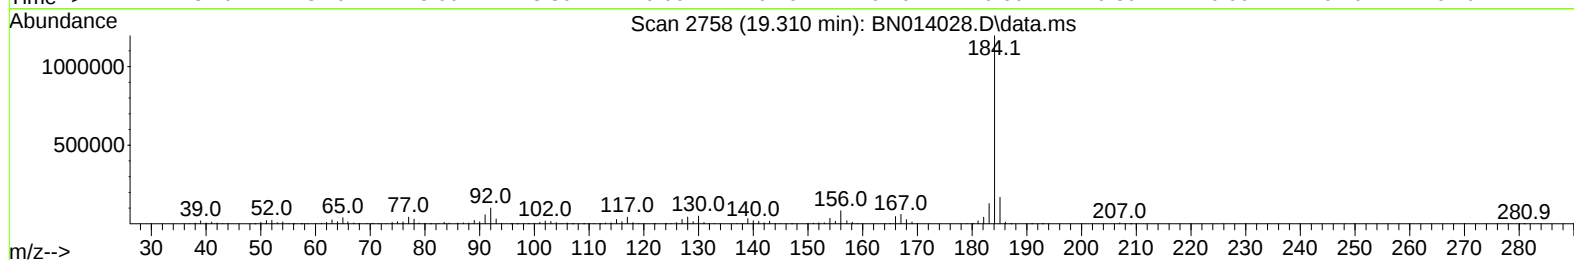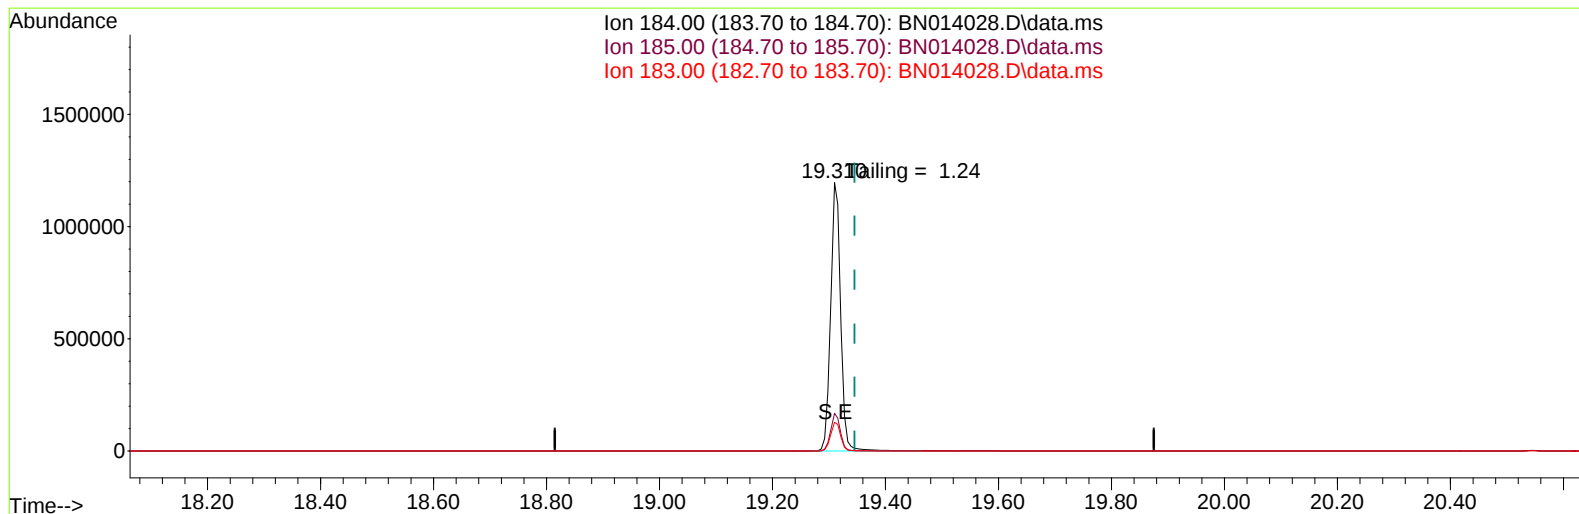

TIC: BN014028.D\data.ms

(77) Benzidine

19.310min (-0.035) 0.00 ng

response 1476768

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	10.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/22/2021	BNA_N	<u>BN014028.D</u>
Compound Name	Response	Retention Time
DDT	712918	20.545
DDD	4500	20.104
DDE	677	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5177	718095	0.72

Instrument :
BNA_N
ClientSampleId :
DFTPP