

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032420\
 Data File : BN010342.D
 Acq On : 25 Mar 2020 00:40
 Operator : CG/JU
 Sample : L1997-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE123D1-20200317

Quant Time: Mar 25 01:49:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 19 15:26:45 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	5248	0.40	ng	0.00
7) Naphthalene-d8	10.38	136	18689	0.40	ng	0.00
13) Acenaphthene-d10	14.24	164	10976	0.40	ng	-0.01
19) Phenanthrene-d10	16.99	188	26790	0.40	ng	0.00
27) Chrysene-d12	21.17	240	27369	0.40	ng	-0.01
34) Perylene-d12	23.35	264	29403	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.25	112	1772	0.17	ng	0.00
5) Phenol-d6	6.80	99	1352	0.10	ng	0.00
8) Nitrobenzene-d5	8.75	82	6694	0.56	ng	0.00
11) 2-Methylnaphthalene-d10	11.97	152	8895	0.30	ng	0.00
14) 2,4,6-Tribromophenol	15.73	330	1299	0.31	ng	0.00
15) 2-Fluorobiphenyl	12.85	172	26339	0.63	ng	-0.01
25) Fluoranthene-d10	19.02	212	25655	0.32	ng	0.00
29) Terphenyl-d14	19.63	244	33558	0.57	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.25	88	8023	1.628	ng	98
32) Bis(2-ethylhexyl)phthalate	21.12	149	5789	0.197	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN032420\
Data File : BN010342.D
Acq On : 25 Mar 2020 00:40
Operator : CG/JU
Sample : L1997-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE123D1-20200317

Quant Time: Mar 25 01:49:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 19 15:26:45 2020
Response via : Initial Calibration

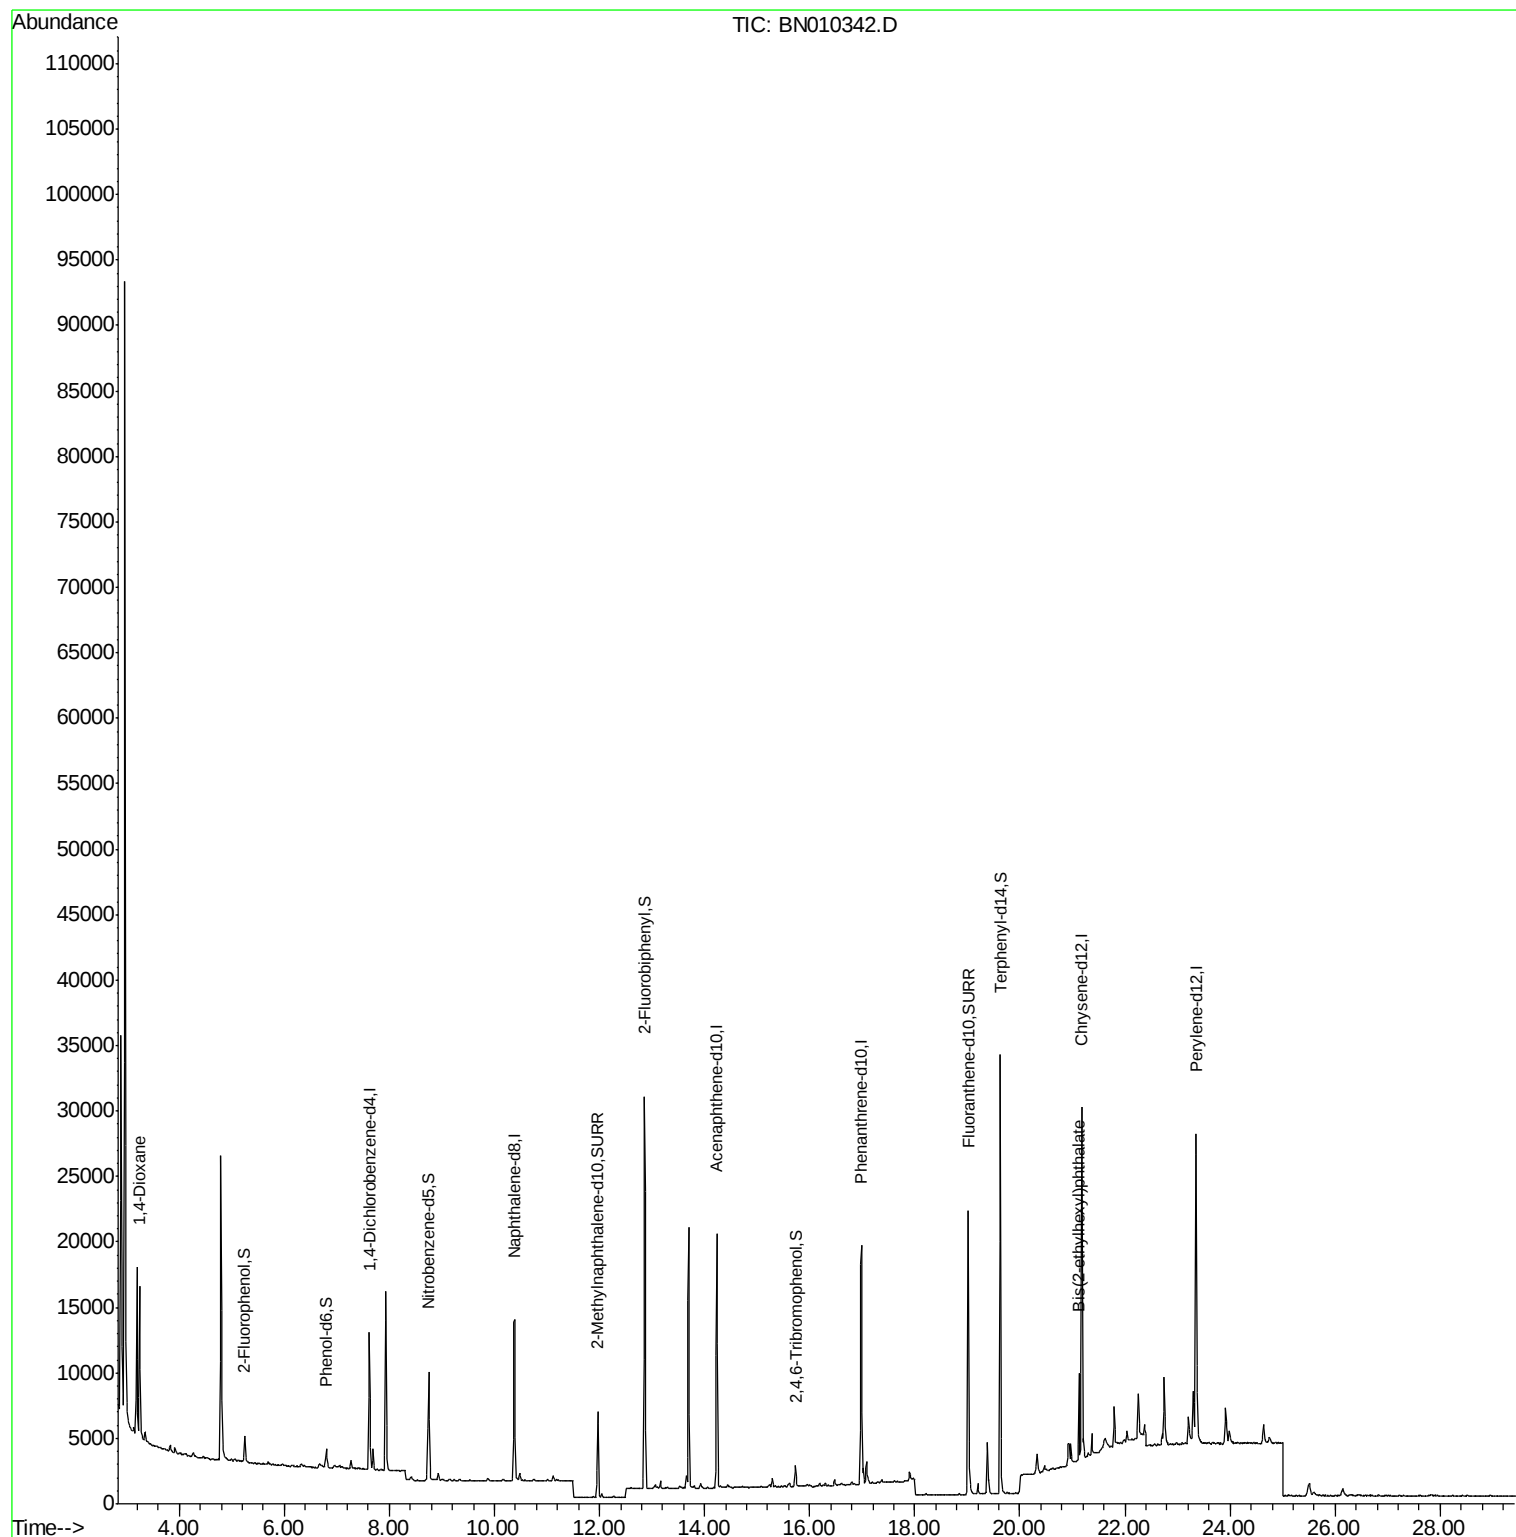

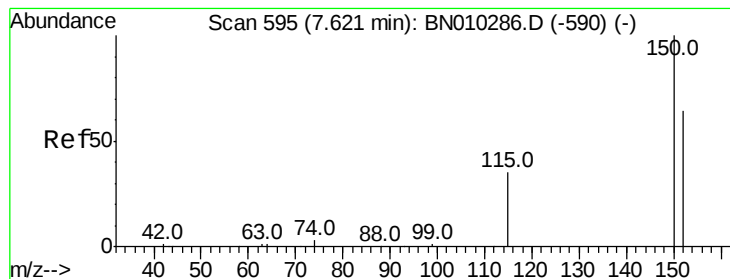

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.62 min Scan# 595

Delta R.T. 0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40

Instrument :

BNA_N

ClientSampleId :

RE123D1-20200317


Tot Ion:152 Resp: 5248

Ion Ratio Lower Upper

152 100

150 151.3 123.1 184.7




115 54.5 45.2 67.8

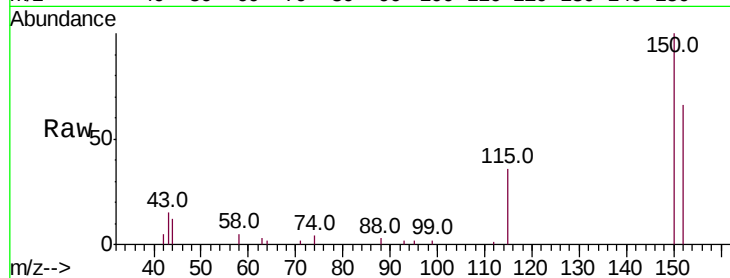

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

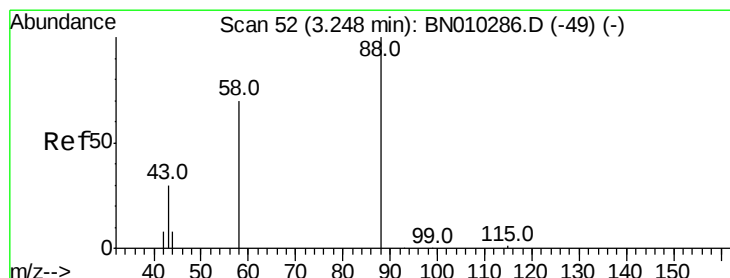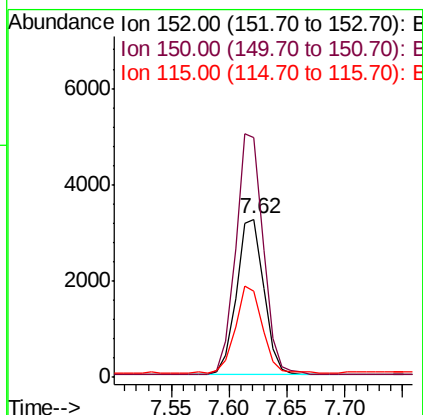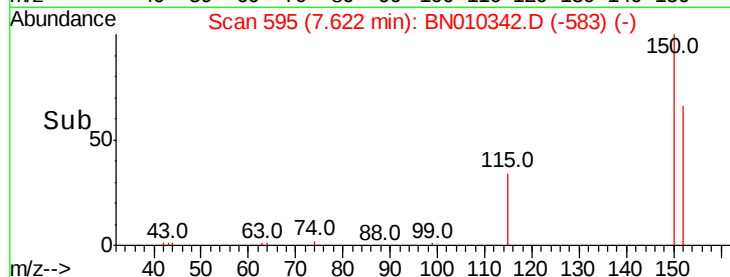

#2

1,4-Dioxane

Concen: 1.628 ng

RT: 3.25 min Scan# 52

Delta R.T. 0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40


Tgt Ion: 88 Resp: 8023

Ion Ratio Lower Upper

88 100

58 63.4 51.7 77.5



43 27.4 21.2 31.8

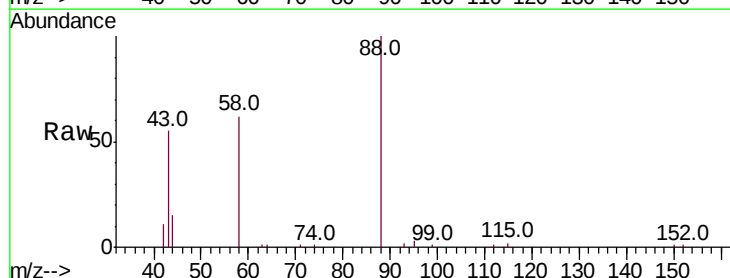


Abundance Ion 88.00 (87.70 to 88.70): BNC

Ion 58.00 (57.70 to 58.70): BNC

Ion 43.00 (42.70 to 43.70): BNC

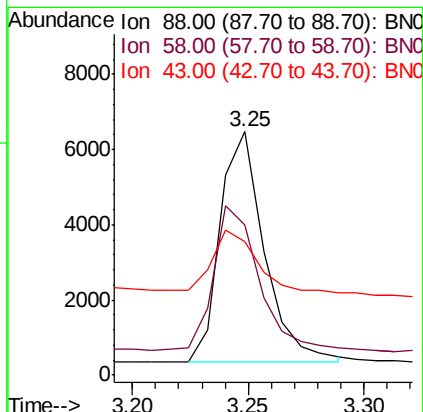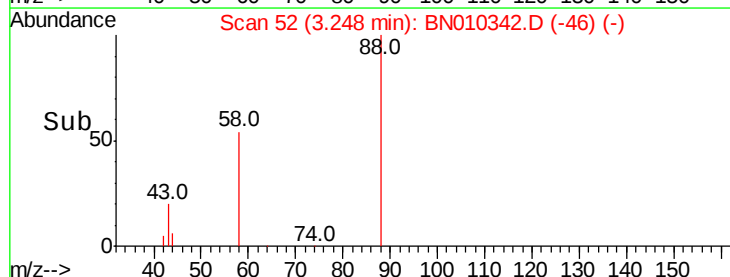

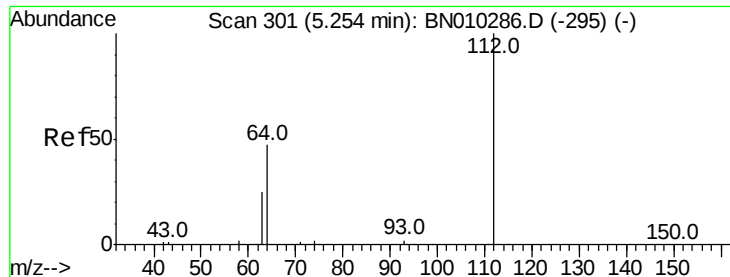

#4

2-Fluorophenol

Concen: 0.171 ng

RT: 5.25 min Scan# 301

Delta R.T. 0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40

Instrument :

BNA_N

ClientSampleId :

RE123D1-20200317


Tot Ion:112 Resp: 1772

Ion Ratio Lower Upper

112 100

64 49.5 41.4 62.2




63 26.6 22.9 34.3

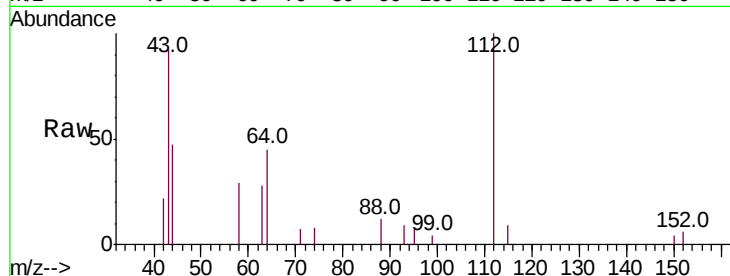

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

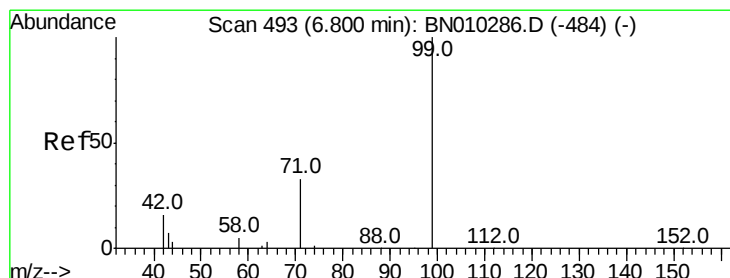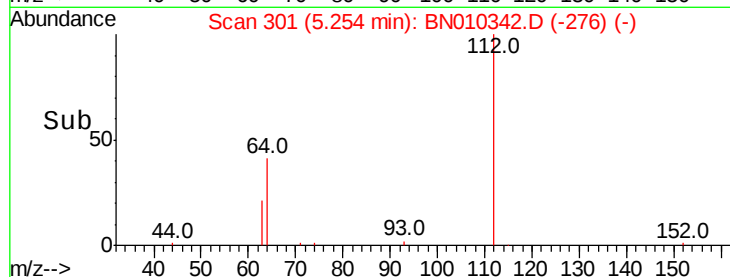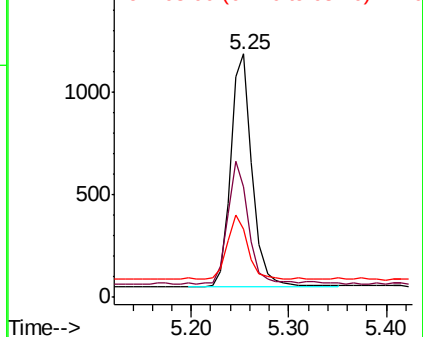

#5

Phenol-d6

Concen: 0.105 ng

RT: 6.80 min Scan# 493

Delta R.T. 0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40


Tgt Ion: 99 Resp: 1352

Ion Ratio Lower Upper

99 100

42 19.1 14.8 22.2



71 36.1 27.3 40.9

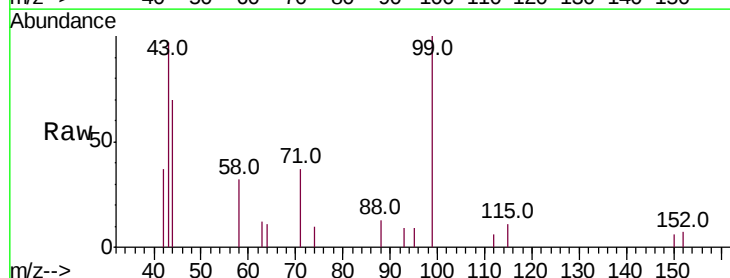


Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

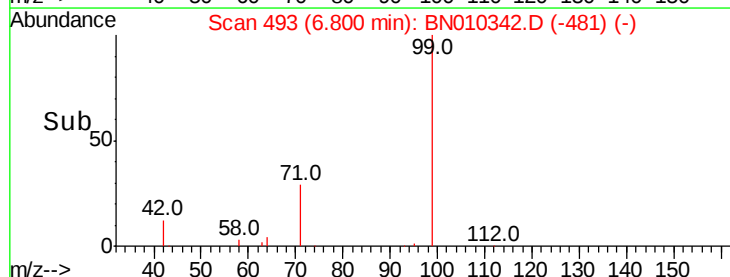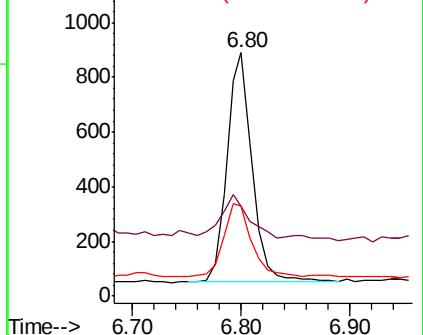

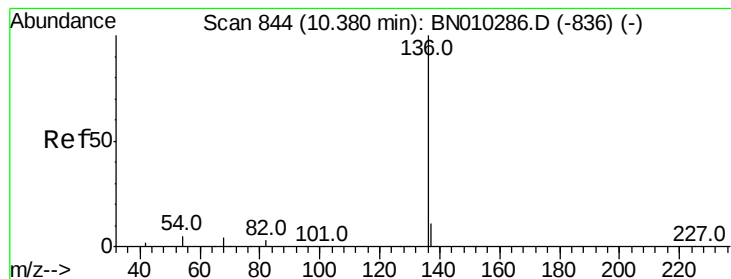

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.38 min Scan# 844

Delta R.T. 0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40

Instrument :

BNA_N

ClientSampleId :

RE123D1-20200317

Tot Ion:136 Resp: 18689



Ion Ratio Lower Upper

136 100

137 11.3 9.3 13.9

54 4.4 4.8 7.2#

68 3.9 4.1 6.1#





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

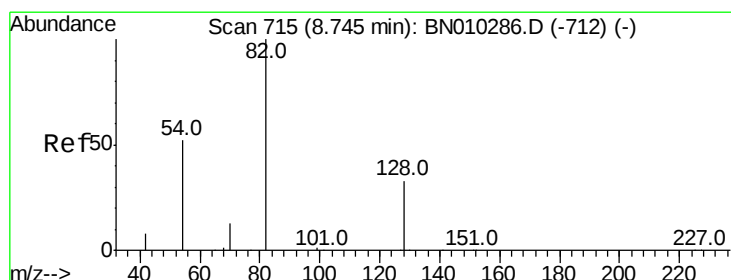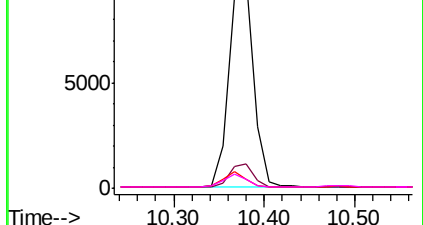

#8

Nitrobenzene-d5

Concen: 0.559 ng

RT: 8.75 min Scan# 715

Delta R.T. 0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40



Tgt Ion: 82 Resp: 6694

Ion Ratio Lower Upper

82 100

128 40.7 28.8 43.2


54 46.1 42.1 63.1




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC




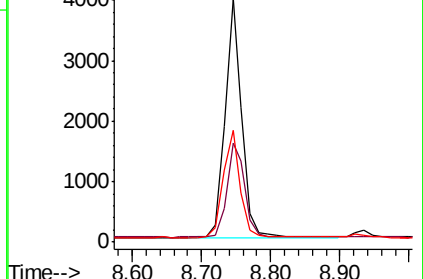




#11
2-Methylnaphthalene-d10
Concen: 0.298 ng
RT: 11.97 min Scan# 1037
Delta R.T. -0.00 min
Lab File: BN010342.D
Acq: 25 Mar 2020 00:40




Instrument :
BNA_N
ClientSampleId :
RE123D1-20200317


Tot Ion:152 Resp: 8895
Ion Ratio Lower Upper
152 100
151 19.4 15.4 23.2

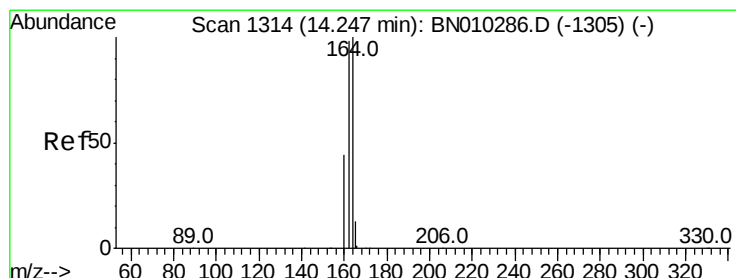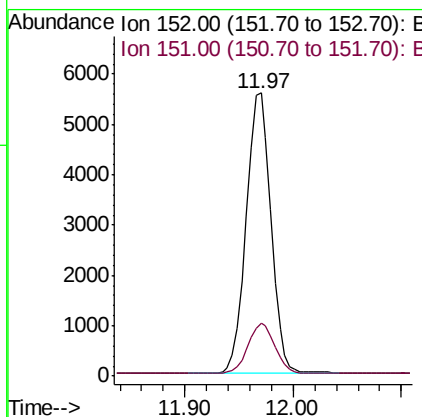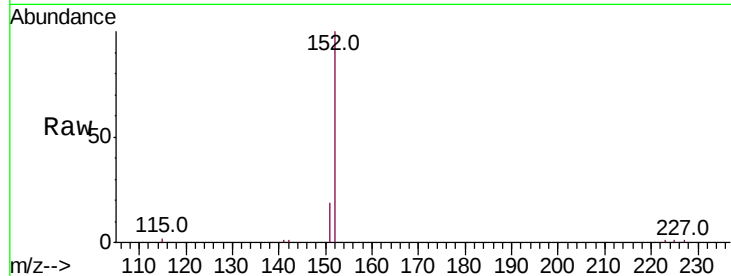

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.24 min Scan# 1313
Delta R.T. -0.01 min
Lab File: BN010342.D
Acq: 25 Mar 2020 00:40

Tgt Ion:164 Resp: 10976
Ion Ratio Lower Upper
164 100
162 101.0 78.2 117.2
160 47.7 35.8 53.6

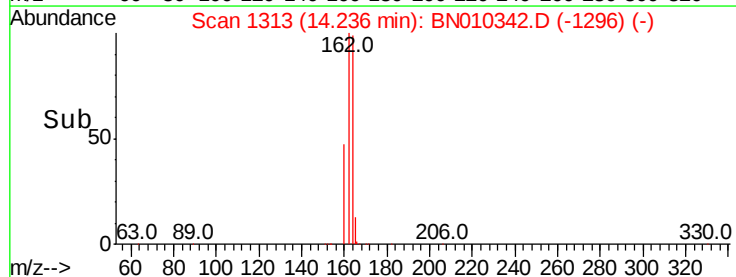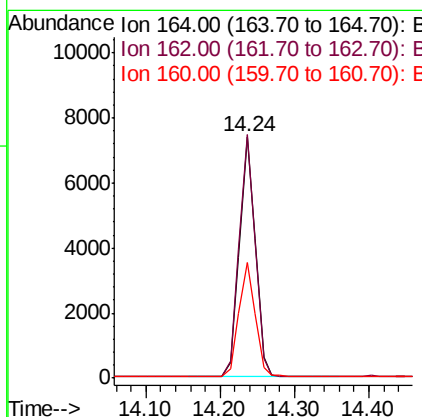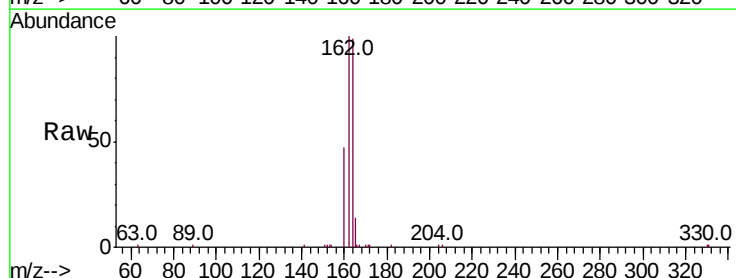







#14
2,4,6-Tribromophenol
Concen: 0.308 ng
RT: 15.73 min Scan# 1447
Delta R.T. 0.00 min
Lab File: BN010342.D
Acq: 25 Mar 2020 00:40

Instrument :
BNA_N
ClientSampleId :
RE123D1-20200317

Tot Ion:330 Resp: 1299
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.6 29.3 43.9

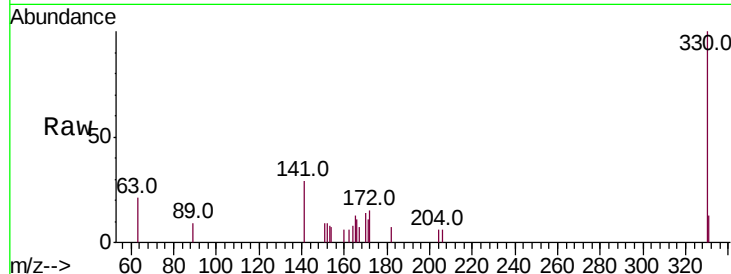


Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E


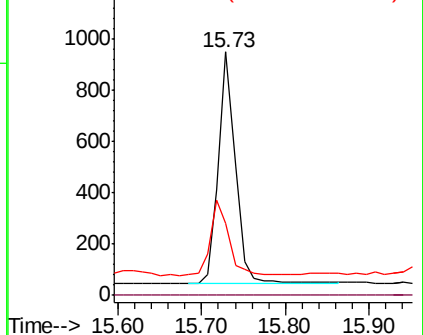



#15
2-Fluorobiphenyl
Concen: 0.627 ng
RT: 12.85 min Scan# 1189
Delta R.T. -0.01 min
Lab File: BN010342.D
Acq: 25 Mar 2020 00:40

Tgt Ion:172 Resp: 26339
Ion Ratio Lower Upper
172 100
171 35.3 27.6 41.4
170 23.8 18.5 27.7



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

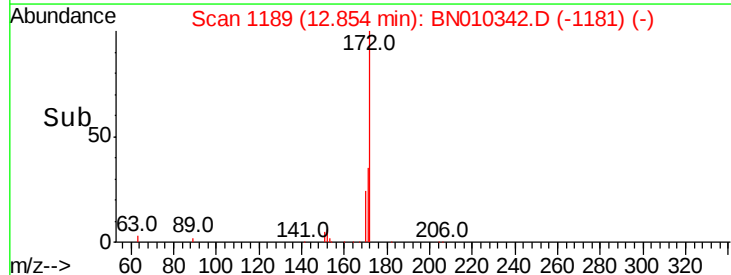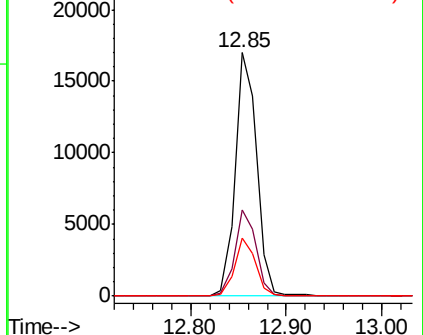

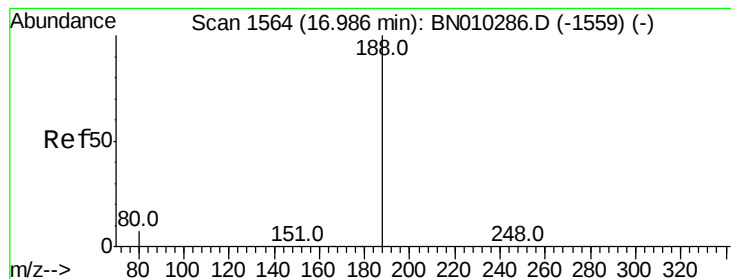

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.99 min Scan# 1564

Delta R.T. 0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40

Instrument :

BNA_N

ClientSampleId :

RE123D1-20200317


Tot Ion:188 Resp: 26790

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 5.8 6.0 9.0#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNO

Ion 80.00 (79.70 to 80.70): BNO

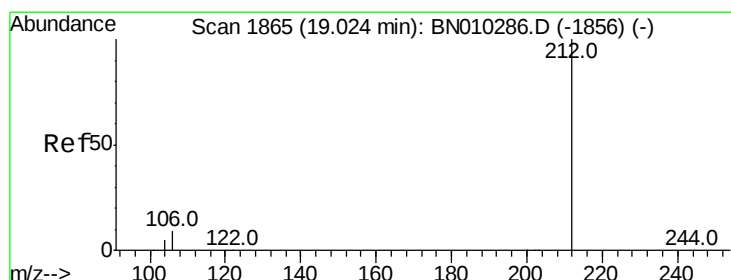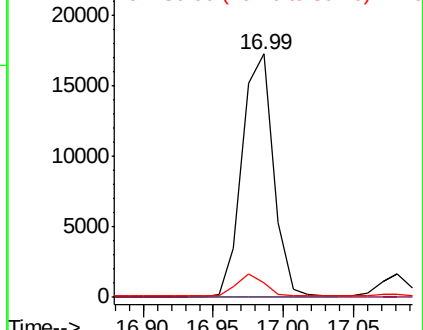

#25

Fluoranthene-d10

Concen: 0.318 ng

RT: 19.02 min Scan# 1864

Delta R.T. -0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40


Tgt Ion:212 Resp: 25655

Ion Ratio Lower Upper

212 100

106 9.7 7.4 11.2



104 5.4 4.2 6.4




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

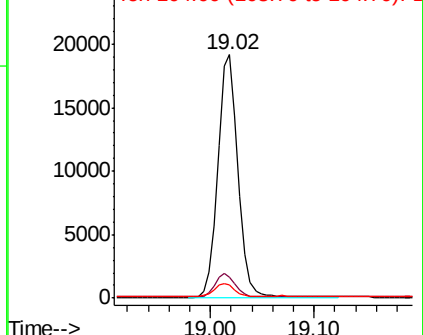



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.17 min Scan# 2173

Delta R.T. -0.01 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40

Instrument :

BNA_N

ClientSampleId :

RE123D1-20200317


Tot Ion:240 Resp: 27369

Ion Ratio Lower Upper

240 100

120 11.6 7.9 11.9




236 27.9 22.2 33.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

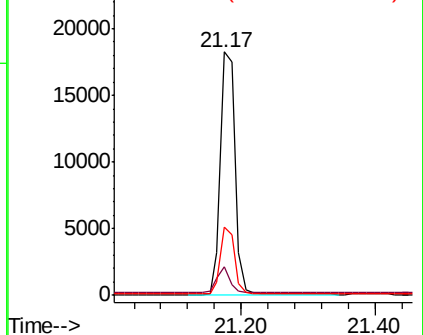

#29

Terphenyl-d14

Concen: 0.568 ng

RT: 19.63 min Scan# 1987

Delta R.T. -0.00 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40


Tgt Ion:244 Resp: 33558

Ion Ratio Lower Upper

244 100

212 8.1 6.3 9.5



122 8.8 7.6 11.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

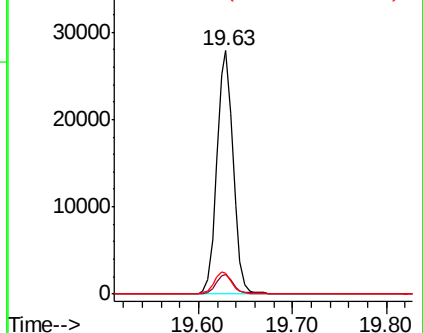



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.197 ng

RT: 21.12 min Scan# 2168

Delta R.T. -0.01 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40

Instrument :

BNA_N

ClientSampleId :

RE123D1-20200317


Tot Ion:149 Resp: 5789

Ion Ratio Lower Upper

149 100

167 27.9 23.0 34.6




279 5.5 3.8 5.8



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

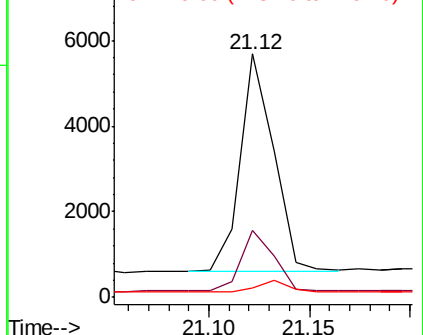

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.35 min Scan# 2565

Delta R.T. -0.01 min

Lab File: BN010342.D

Acq: 25 Mar 2020 00:40


Tgt Ion:264 Resp: 29403

Ion Ratio Lower Upper

264 100

260 24.5 19.5 29.3

265 38.8 32.4 48.6



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

